Cochrane Library

Cochrane Database of Systematic Reviews

Antibody tests for identification of current and past infection with SARS-CoV-2 (Review)

Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Spijker R, Taylor-Phillips S, Adriano A, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Dittrich S, Emperador D, Hooft L, Leeflang MMG, Van den Bruel A, Cochrane COVID-19 Diagnostic Test Accuracy Group

Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Spijker R, Taylor-Phillips S, Adriano A, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Dittrich S, Emperador D, Hooft L, Leeflang MMG, Van den Bruel A.
Antibody tests for identification of current and past infection with SARS-CoV-2.
Cochrane Database of Systematic Reviews 2020, Issue 6. Art. No.: CD013652.
DOI: 10.1002/14651858.CD013652.

www.cochranelibrary.com

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

WILEY

TABLE OF CONTENTS

HEADER 1
ABSTRACT 1
PLAIN LANGUAGE SUMMARY 3
SUMMARY OF FINDINGS 5
BACKGROUND 7
OBJECTIVES 8
METHODS 9
RESULTS 12
Figure 1. 13
Figure 2. 15
Figure 3. 17
Figure 4. 18
Figure 5. 20
Figure 6. 22
Figure 7. 25
Figure 8. 26
Figure 9. 27
DISCUSSION 28
AUTHORS' CONCLUSIONS 30
ACKNOWLEDGEMENTS 31
REFERENCES 33
CHARACTERISTICS OF STUDIES 49
DATA 218
Test 1. IgG (all time points) 222
Test 2. IgG (1 to 7 days) 223
Test 3. IgG (8 to 14 days) 224
Test 4. IgG (15 to 21 days) 225
Test 5. IgG (22 to 35 days) 226
Test 6. IgG (over 35 days) 226
Test 7. IgM (all time points) 227
Test 8. IgM (8 to 14 days) 228
Test 9. IgM (1 to 7 days) 229
Test 10. IgM (15 to 21 days) 230
Test 11. IgM (22 to 35 days) 231
Test 12. IgM (over 35 days) 231
Test 13. IgG/IgM (all time points) 232
Test 14. IgG/IgM (1 to 7 days) 233
Test 15. IgG/IgM (8 to 14 days) 233
Test 16. IgG/IgM (15 to 21 days) 234
Test 17. IgG/IgM (22 to 35 days) 234
Test 18. IgG/IgM (over 35 days) 235
Test 19. IgA (all time points) 235
Test 20. IgA (1 to 7 days) 235
Test 21. IgA (8 to 14 days) 235
Test 22. IgA (15 to 21 days) 236
Test 23. IgA (22 to 35 days) 236
Test 24. IgA (over 35 days) 236
Test 25. Total antibodies (Ab) (all time points) 236
Test 27. Total antibodies (Ab) (1 to 7 days) 237
Test 29. Total antibodies (Ab) (8 to 14 days) 237
Test 30. Total antibodies (Ab) (15 to 21 days) 237

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 31. Total antibodies (Ab) (21 to 35 days) 237
Test 32. Total antibodies (Ab) (over 35 days) 238
Test 33. IgA/IgG (all time points) 238
Test 34. IgA/IgG (1 to 7 days) 238
Test 35. IgA/IgG (8 to 14 days) 238
Test 36. IgA/IgG (15 to 21 days) 238
Test 37. IgA/IgG (22 to 35 days) 239
Test 38. IgA/IgM (all time points) 239
Test 39. IgG in PCR+ve (all time points) 239
Test 40. IgG in PCR +ve (1 to 7 days) 239
Test 41. IgG in PCR+ve (8 to 14 days) 239
Test 42. IgG in PCR+ve (15 to 21 days) 240
Test 43. IgG in PCR-ve (all time points) 240
Test 44. IgG in PCR-ve (1 to 7 days) 240
Test 45. IgG in PCR-ve (8 to 14 days) 240
Test 46. IgG in PCR-ve (15 to 21 days) 240
Test 47. IgM in PCR+ve (all time points) 241
Test 48. IgM in PCR+ve (1 to 7 days) 241
Test 49. IgM in PCR+ve (8 to 14 days) 241
Test 50. IgM in PCR+ve (15 to 21 days) 241
Test 51. IgM in PCR-ve (all time points) 242
Test 52. IgM in PCR-ve (1 to 7 days) 242
Test 53. IgM in PCR-ve (8 to 14 days) 242
Test 54. IgM in PCR-ve (15 to 21 days) 242
Test 55. IgG/IgM in PCR+ve (all time points) 243
Test 56. IgG/IgM in PCR+ve (1 to 7 days) 243
Test 57. IgG/IgM in PCR+ve (8 to 14 days) 243
Test 58. IgG/IgM in PCR+ve (15 to 21 days) 243
Test 59. IgG/IgM in PCR-ve (all time points) 243
Test 60. IgG/IgM in PCR-ve (1 to 7 days) 244
Test 61. IgG/IgM in PCR-ve (8 to 14 days) 244
Test 62. IgG/IgM in PCR-ve (15 to 21 days) 244
Test 63. IgG (moderate) 244
Test 64. IgG (severe) 244
Test 65. IgG (critical) 245
Test 66. IgM (moderate) 245
Test 67. IgM (severe) 245
Test 68. IgM (critical) 245
Test 69. RT-PCR (all time points - throat) 245
Test 70. RT-PCR (1 to 7 days throat) 246
Test 71. RT-PCR (8 to 14 days - throat) 246
Test 72. RT-PCR (15 to 21 days - throat) 246
Test 73. RT-PCR (all time points - sputum) 246
Test 74. RT-PCR (1 to 7 days - sputum) 246
Test 75. RT-PCR (8 to 14 days - sputum) 247
Test 76. RT-PCR (15 to 21 days - sputum) 247
ADDITIONAL TABLES 247
APPENDICES 264
Figure 10. 296
Figure 11. 298
Figure 12. 299
Figure 13. 299

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 14. 300
HISTORY 305
CONTRIBUTIONS OF AUTHORS 305
DECLARATIONS OF INTEREST 305
SOURCES OF SUPPORT 306
DIFFERENCES BETWEEN PROTOCOL AND REVIEW 306

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

[Diagnostic Test Accuracy Review]

Antibody tests for identification of current and past infection with SARS-CoV-2

Jonathan J Deeks[1,2], Jacqueline Dinnes[1,2], Yemisi Takwoingi[1,2], Clare Davenport[1,2], René Spijker[3,4], Sian Taylor-Phillips[1,5], Ada Adriano[1], Sophie Beese[1], Janine Dretzke[1], Lavinia Ferrante di Ruffano[1], Isobel M Harris[1], Malcolm J Price[1,2], Sabine Dittrich[6], Devy Emperador[6], Lotty Hooft[4], Mariska MG Leeflang[7,8], Ann Van den Bruel[9], Cochrane COVID-19 Diagnostic Test Accuracy Group[1]

[1]Test Evaluation Research Group, Institute of Applied Health Research, University of Birmingham, Birmingham, UK. [2]NIHR Birmingham Biomedical Research Centre, University Hospitals Birmingham NHS Foundation Trust and University of Birmingham, Birmingham, UK. [3]Medical Library, Amsterdam UMC, University of Amsterdam, Amsterdam Public Health, Amsterdam, Netherlands. [4]Cochrane Netherlands, Julius Center for Health Sciences and Primary Care, University Medical Center Utrecht, Utrecht University, Utrecht, Netherlands. [5]Division of Health Sciences, Warwick Medical School, University of Warwick, Coventry, UK. [6]FIND, Geneva, Switzerland. [7]Department of Clinical Epidemiology, Biostatistics and Bioinformatics, Amsterdam University Medical Centers, University of Amsterdam, Amsterdam, Netherlands. [8]Biomarker and Test Evaluation Programme (BiTE), Amsterdam UMC, University of Amsterdam, Amsterdam, Netherlands. [9]Department of Public Health and Primary Care, KU Leuven, Leuven, Belgium

Contact address: Jonathan J Deeks, j.deeks@bham.ac.uk.

Editorial group: Cochrane Infectious Diseases Group.
Publication status and date: New, published in Issue 6, 2020.

Citation: Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Spijker R, Taylor-Phillips S, Adriano A, Beese S, Dretzke J, Ferrante di Ruffano L, Harris IM, Price MJ, Dittrich S, Emperador D, Hooft L, Leeflang MMG, Van den Bruel A. Antibody tests for identification of current and past infection with SARS-CoV-2. *Cochrane Database of Systematic Reviews* 2020, Issue 6. Art. No.: CD013652. DOI: 10.1002/14651858.CD013652.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ABSTRACT

Background

The severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) virus and resulting COVID-19 pandemic present important diagnostic challenges. Several diagnostic strategies are available to identify current infection, rule out infection, identify people in need of care escalation, or to test for past infection and immune response. Serology tests to detect the presence of antibodies to SARS-CoV-2 aim to identify previous SARS-CoV-2 infection, and may help to confirm the presence of current infection.

Objectives

To assess the diagnostic accuracy of antibody tests to determine if a person presenting in the community or in primary or secondary care has SARS-CoV-2 infection, or has previously had SARS-CoV-2 infection, and the accuracy of antibody tests for use in seroprevalence surveys.

Search methods

We undertook electronic searches in the Cochrane COVID-19 Study Register and the COVID-19 Living Evidence Database from the University of Bern, which is updated daily with published articles from PubMed and Embase and with preprints from medRxiv and bioRxiv. In addition, we checked repositories of COVID-19 publications. We did not apply any language restrictions. We conducted searches for this review iteration up to 27 April 2020.

Selection criteria

We included test accuracy studies of any design that evaluated antibody tests (including enzyme-linked immunosorbent assays, chemiluminescence immunoassays, and lateral flow assays) in people suspected of current or previous SARS-CoV-2 infection, or where tests were used to screen for infection. We also included studies of people either known to have, or not to have SARS-CoV-2 infection.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

We included all reference standards to define the presence or absence of SARS-CoV-2 (including reverse transcription polymerase chain reaction tests (RT-PCR) and clinical diagnostic criteria).

Data collection and analysis

We assessed possible bias and applicability of the studies using the QUADAS-2 tool. We extracted 2x2 contingency table data and present sensitivity and specificity for each antibody (or combination of antibodies) using paired forest plots. We pooled data using random-effects logistic regression where appropriate, stratifying by time since post-symptom onset. We tabulated available data by test manufacturer. We have presented uncertainty in estimates of sensitivity and specificity using 95% confidence intervals (CIs).

Main results

We included 57 publications reporting on a total of 54 study cohorts with 15,976 samples, of which 8526 were from cases of SARS-CoV-2 infection. Studies were conducted in Asia (n = 38), Europe (n = 15), and the USA and China (n = 1). We identified data from 25 commercial tests and numerous in-house assays, a small fraction of the 279 antibody assays listed by the Foundation for Innovative Diagnostics. More than half (n = 28) of the studies included were only available as preprints.

We had concerns about risk of bias and applicability. Common issues were use of multi-group designs (n = 29), inclusion of only COVID-19 cases (n = 19), lack of blinding of the index test (n = 49) and reference standard (n = 29), differential verification (n = 22), and the lack of clarity about participant numbers, characteristics and study exclusions (n = 47). Most studies (n = 44) only included people hospitalised due to suspected or confirmed COVID-19 infection. There were no studies exclusively in asymptomatic participants. Two-thirds of the studies (n = 33) defined COVID-19 cases based on RT-PCR results alone, ignoring the potential for false-negative RT-PCR results. We observed evidence of selective publication of study findings through omission of the identity of tests (n = 5).

We observed substantial heterogeneity in sensitivities of IgA, IgM and IgG antibodies, or combinations thereof, for results aggregated across different time periods post-symptom onset (range 0% to 100% for all target antibodies). We thus based the main results of the review on the 38 studies that stratified results by time since symptom onset. The numbers of individuals contributing data within each study each week are small and are usually not based on tracking the same groups of patients over time.

Pooled results for IgG, IgM, IgA, total antibodies and IgG/IgM all showed low sensitivity during the first week since onset of symptoms (all less than 30.1%), rising in the second week and reaching their highest values in the third week. The combination of IgG/IgM had a sensitivity of 30.1% (95% CI 21.4 to 40.7) for 1 to 7 days, 72.2% (95% CI 63.5 to 79.5) for 8 to 14 days, 91.4% (95% CI 87.0 to 94.4) for 15 to 21 days. Estimates of accuracy beyond three weeks are based on smaller sample sizes and fewer studies. For 21 to 35 days, pooled sensitivities for IgG/IgM were 96.0% (95% CI 90.6 to 98.3). There are insufficient studies to estimate sensitivity of tests beyond 35 days post-symptom onset. Summary specificities (provided in 35 studies) exceeded 98% for all target antibodies with confidence intervals no more than 2 percentage points wide. False-positive results were more common where COVID-19 had been suspected and ruled out, but numbers were small and the difference was within the range expected by chance.

Assuming a prevalence of 50%, a value considered possible in healthcare workers who have suffered respiratory symptoms, we would anticipate that 43 (28 to 65) would be missed and 7 (3 to 14) would be falsely positive in 1000 people undergoing IgG/IgM testing at days 15 to 21 post-symptom onset. At a prevalence of 20%, a likely value in surveys in high-risk settings, 17 (11 to 26) would be missed per 1000 people tested and 10 (5 to 22) would be falsely positive. At a lower prevalence of 5%, a likely value in national surveys, 4 (3 to 7) would be missed per 1000 tested, and 12 (6 to 27) would be falsely positive.

Analyses showed small differences in sensitivity between assay type, but methodological concerns and sparse data prevent comparisons between test brands.

Authors' conclusions

The sensitivity of antibody tests is too low in the first week since symptom onset to have a primary role for the diagnosis of COVID-19, but they may still have a role complementing other testing in individuals presenting later, when RT-PCR tests are negative, or are not done. Antibody tests are likely to have a useful role for detecting previous SARS-CoV-2 infection if used 15 or more days after the onset of symptoms. However, the duration of antibody rises is currently unknown, and we found very little data beyond 35 days post-symptom onset. We are therefore uncertain about the utility of these tests for seroprevalence surveys for public health management purposes. Concerns about high risk of bias and applicability make it likely that the accuracy of tests when used in clinical care will be lower than reported in the included studies. Sensitivity has mainly been evaluated in hospitalised patients, so it is unclear whether the tests are able to detect lower antibody levels likely seen with milder and asymptomatic COVID-19 disease.

The design, execution and reporting of studies of the accuracy of COVID-19 tests requires considerable improvement. Studies must report data on sensitivity disaggregated by time since onset of symptoms. COVID-19-positive cases who are RT-PCR-negative should be included as well as those confirmed RT-PCR, in accordance with the World Health Organization (WHO) and China National Health Commission of the People's Republic of China (CDC) case definitions. We were only able to obtain data from a small proportion of available tests, and action is needed to ensure that all results of test evaluations are available in the public domain to prevent selective reporting. This is a fast-moving field and we plan ongoing updates of this living systematic review.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

PLAIN LANGUAGE SUMMARY

What is the diagnostic accuracy of antibody tests for the detection of infection with the COVID-19 virus?

Background

COVID-19 is an infectious disease caused by the SARS-CoV-2 virus that spreads easily between people in a similar way to the common cold or 'flu. Most people with COVID-19 have a mild to moderate respiratory illness, and some may have no symptoms (asymptomatic infection). Others experience severe symptoms and need specialist treatment and intensive care.

The immune system of people who have COVID-19 responds to infection by developing proteins that can attack the virus (antibodies) in their blood. Tests to detect antibodies in peoples' blood might show whether they currently have COVID-19 or have had it previously.

Why are accurate tests important?

Accurate testing allows identification of people who might need treatment, or who need to isolate themselves to prevent the spread of infection. Failure to detect people with COVID-19 when it is present (a false negative result) may delay treatment and risk further spread of infection to others. Incorrect identification of COVID-19 when it is not present (a false positive result) may lead to unnecessary further testing, treatment, and isolation of the person and close contacts. Correct identification of people who have previously had COVID-19 is important in measuring disease spread, assessing the success of public health interventions (like isolation), and potentially in identifying individuals with immunity (should antibodies in the future be shown to indicate immunity).

To identify false negative and false positive results, antibody test results are compared in people known to have COVID-19 and known not to have COVID-19. Study participants are classified as to whether they are known or not known to have COVID-19 based on criteria known as the 'reference standard'. Many studies use samples taken from the nose and throat to identify people with COVID-19. The samples undergo a test called reverse transcriptase polymerase chain reaction (RT-PCR). This testing process can sometimes miss infection (false negative result), but additional tests can identify COVID-19 infection in people with a negative RT-PCR result. These include measuring clinical symptoms, like coughing or high temperature, or 'imaging' tests like chest X-rays. People known not to have COVID-19 are sometimes identified from stored blood samples taken before COVID-19 existed, or from patients with respiratory symptoms found to be caused by other diseases.

What did the review study?

The studies looked at three types of antibody, IgA, IgG and IgM. Most tests measure both IgG and IgM, but some measure a single antibody or combinations of the three antibodies.

Levels of antibodies rise and fall at different times after infection. IgG is the last to rise but lasts longest. Levels of antibodies are usually highest a few weeks after infection.

Some antibody tests need specialist laboratory equipment. Others use disposable devices, similar to pregnancy tests. These tests can be used in laboratories or wherever the patient is (point-of-care), in hospital or at home.

We wanted to find out whether antibody tests:

- are accurate enough to diagnose infection in people with or without symptoms of COVID-19, and

- can be used to find out if someone has already had COVID-19.

What did we do?

We looked for studies that measured the accuracy of antibody tests compared with reference standard criteria to detect current or past COVID-19 infection. Studies could assess any antibody test compared with any reference standard. People could be tested in hospital or the community. Studies could test people known to have – or not to have – or be suspected of having COVID-19.

Study characteristics

We found 54 relevant studies. Studies took place in Asia (38), Europe (15), and in both USA and China (1).

Forty-six studies included people who were in hospital with suspected or confirmed COVID-19 infection only. Twenty-nine studies compared test results in people with COVID-19 with test results in healthy people or people with other diseases.

Not all studies provided details about participants' age and gender. Often, we could not tell whether studies were evaluating current or past infection, as few reported whether participants were recovering. We did not find any studies that tested only asymptomatic people.

Main results

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Our findings come mainly from 38 studies that provided results based on the time since people first noticed symptoms.

Antibody tests one week after first symptoms only detected 30% of people who had COVID-19. Accuracy increased in week 2 with 70% detected, and was highest in week 3 (more than 90% detected). Little evidence was available after week 3. Tests gave false positive results in 2% of those without COVID-19.

Results from IgG/IgM tests three weeks after symptoms started suggested that if 1000 people had antibody tests, and 50 (5%) of them really had COVID-19 (as we might expect in a national screening survey):

- 58 people would test positive for COVID-19. Of these, 12 people (21%) would not have COVID-19 (false positive result).

- 942 people would test negative for COVID-19. Of these, 4 people (0.4%) would actually have COVID-19 (false negative result).

If we tested 1000 healthcare workers (in a high-risk setting) who had had symptoms, and 500 (50%) of them really had COVID-19:

- 464 people would test positive for COVID-19. Of these, 7 people (2%) would not have COVID-19 (false positive result).

- 537 people would test negative for COVID-19. Of these, 43 (8%) would actually have COVID-19 (false negative result).

We did not find convincing differences in accuracy for different types of antibody test.

How reliable were the results of the studies of this review?

Our confidence in the evidence is limited for several reasons. In general, studies were small, did not use the most reliable methods and did not report their results fully. Often, they did not include patients with COVID-19 who may have had a false negative result on PCR, and took their data for people without COVID-19 from records of tests done before COVID-19 arose. This may have affected test accuracy, but it is impossible to identify by how much.

Who do the results of this review apply to?

Most participants were in hospital with COVID-19, so were likely to have more severe disease than people with mild symptoms who were not hospitalised. This means that we don't know how accurate antibody tests are for people with milder disease or no symptoms.

More than half of the studies assessed tests they had developed themselves, most of which are not available to buy. Many studies were published quickly online as ‘preprints’. Preprints do not undergo the normal rigorous checks of published studies, so we are not certain how reliable they are.

As most studies took place in Asia, we don't know whether test results would be similar elsewhere in the world.

What are the implications of this review?

The review shows that antibody tests could have a useful role in detecting if someone has had COVID-19, but the timing of when the tests are used is important. Antibody tests may help to confirm COVID-19 infection in people who have had symptoms for more than two weeks and do not have a RT-PCR test, or have negative RT-PCR test results. The tests are better at detecting COVID-19 in people two or more weeks after their symptoms started, but we do not know how well they work more than five weeks after symptoms started. We do not know how well the tests work for people who have milder disease or no symptoms, because the studies in the review were mainly done in people who were in hospital. In time, we will learn whether having previously had COVID-19 provides individuals with immunity to future infection.

Further research is needed into the use of antibody tests in people recovering from COVID-19 infection, and in people who have experienced mild symptoms or who never experienced symptoms.

How up-to-date is this review?

This review includes evidence published up to 27 April 2020. Because a lot of new research is being published in this field, we will update this review frequently.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

SUMMARY OF FINDINGS

Summary of findings 1. What is the diagnostic accuracy of antibody tests, for the diagnosis of current or prior SARS-CoV-2 infection?

Question	What is the diagnostic accuracy of antibody tests, for the diagnosis of current or prior SARS-CoV-2 infection?
Population	Adults or children suspected of • current SARS-CoV-2 infection • prior SARS-CoV-2 infection or populations undergoing screening for SARS-CoV-2 infection, including • asymptomatic contacts of confirmed COVID-19 cases • community screening
Index test	Any test for detecting antibodies to SARS-CoV-2, including: • laboratory-based methods * ELISA * CLIA * other laboratory-based methods • rapid tests; lateral flow assays, including * tests that can be used at point-of-care, such as CGIA * rapid diagnostic tests, such as FIA
Target condition	Detection of • current SARS-CoV-2 infection • prior SARS-CoV-2 infection
Reference standard	RT-PCR alone, clinical diagnosis of COVID-19 based on established guidelines or combinations of clinical features and for non-COVID-19 cases, the use of pre-pandemic sources of samples for testing
Action	The current evidence-base for antibody tests is inadequate to be clear about their utility (mainly because of small numbers of small studies for each test, few data available outside of acute hospital settings, and many issues in likely bias and applicability of the studies). The sensitivity of antibody tests is too low early in disease for use as a primary test of diagnosis, but they may have value for late diagnosis, for identifying previous infection, and for sero-prevalence studies.
Limitations in the evidence	
Risk of bias	**Participant selection:** high risk of bias in 48 studies (89%) **Application of index tests:** high risk of bias in 14 studies (26%) **Reference standard:** high risk of bias in 17 studies (31%) **Flow and timing:** high risk of bias in 29 studies (54%)
Concerns about applicability of the evidence	**Participants:** high concerns in 44 studies (81%) **Index test:** high concerns in 17 studies (31%) **Reference standard:** high concerns in 33 studies (61%)
Findings	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

- We included 54 studies evaluating 15,976 samples. 8256 samples were from COVID-19 cases.
- Data were not available for most antibody tests that have regulatory approval.
- Most studies reported on detection of IgG, IgM, or IgG/IgM antibodies.
- Test sensitivity was strongly related to time since onset of symptoms, with low sensitivity between 1 and 14 days, and sensitivity for IgG/IgM tests exceeding 90% between 15 and 35 days. Little evidence was available beyond 35 days.
- Specificity was high (> 98%) for all types of antibody. There was some variation in sensitivity between test methods, with laboratory-based methods appearing to outperform (point-of-care) tests using disposable devices.
- Small sample sizes, low numbers of studies and concerns and bias and applicability hinder trustworthy comparisons being made between test brands.

Quantity of evidence	**Number of studies**	**Total participants or samples**		**Total cases**
	54	15,976		8526
	Sensitivity (95% CI) ***Studies (TP/COVID cases)***			**Specificity (95%CI)** ***Studies (FP/non-COVID cases)***
	Days 8-14	**Days 15-21**	**Days 22-35**	**All time points**
IgG	66.5% (57.9 to 74.2)	88.2% (83.5 to 91.8)	80.3% (72.4 to 86.4)	99.1% (98.3% to 99.6%)
	22 (766/1200)	22 (974/1110)	12 (417/502)	44 (159/6136)
IgM	58.4% (45.5 to 70.3)	75.4% (64.3 to 83.8)	68.1% (55.0 to 78.9)	98.7% (97.4% to 99.3%)
	21 (724/1171)	21 (800/1074)	11 (378/507)	41 (183/6103)
IgG/IgM*	72.2% (63.5 to 79.5)	91.4% (87.0 to 94.4)	96.0% (90.6 to 98.3)	98.7% (97.2% to 99.4%)
	9 (441/608)	9 (636/692)	5 (146/152)	23 (78/5761)
Numbers applied to a hypothetical cohort of 1000 patients, using summary data for IgG/IgM at days 15 to 21 as an exemplar (sensitivity 91.4% (87.0 to 94.4) and specificity 98.7% (97.2 to 99.4))				
Prevalence of COVID-19	**TP (95% CI)**	**FP (95% CI)**	**FN (95% CI)**	**TN (95% CI)**
2%	18 (17 to 20)	13 (6 to 27)	2 (1 to 3)	967 (953 to 974)
5%	46 (44 to 47)	12 (6 to 27)	4 (3 to 7)	938 (923 to 944)
10%	91 (87 to 94)	12 (5 to 25)	9 (6 to 13)	888 (875 to 895)
20%	183 (174 to 189)	10 (5 to 22)	17 (11 to 26)	790 (778 to 795)
50%	457 (435 to 472)	7 (3 to 14)	43 (28 to 65)	494 (486 to 497)

CGIA: colloidal gold immunoassays; **CI:** confidence interval; **CLIA:** chemiluminescence immunoassays; **ELISA:** enzyme-linked immunosorbent assays; **FIA:** fluorescence-labelled immunochromatographic assays; **FN:** false negative; **FP:** false positive; **RT-PCR:** reverse transcription polymerase chain reaction; **TN:** true negative; **TP:** true positive; * Positive if either IgG or IgM positive.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

BACKGROUND

The severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) virus and resulting COVID-19 pandemic present important diagnostic evaluation challenges. These range from understanding the value of signs and symptoms in predicting possible infection, assessing whether existing biochemical and imaging tests can identify infection and people needing critical care, and evaluating whether new diagnostic tests can allow accurate rapid and point-of-care testing, either to identify current infection, rule out infection, identify people in need of care escalation, or to test for past infection and immunity.

We are creating and maintaining a suite of living systematic reviews to cover the roles of tests and characteristics in the diagnosis of COVID-19. This review summarises evidence of the accuracy of COVID-19 antibody tests; both laboratory-based tests and point-of-care tests.

Target condition being diagnosed

COVID-19 is the disease caused by infection with the SARS-CoV-2 virus. The key target conditions for this suite of reviews are current SARS-CoV-2 infection, current COVID-19 disease, and past SARS-CoV-2 infection.

Antibody tests are being considered and evaluated for both:

- identification of past SARS-CoV-2 infection, and
- current infection.

For current infection the severity of the disease is of importance. SARS-CoV-2 infection can be asymptomatic (no symptoms); mild or moderate (symptoms such as fever, cough, aches, lethargy but without difficulty breathing at rest); severe (symptoms with breathlessness and increased respiratory rate indicative of pneumonia); or critical (requiring respiratory support due to severe acute respiratory syndrome (SARS) or acute respiratory distress syndrome (ARDS). People with COVID-19 pneumonia (severe or critical disease) require different patient management, and it is important to be able to identify them. There is no consideration that antibody tests are able to distinguish severity of disease, thus, in this review, we consider their role for detecting SARS-CoV-2 infection of any severity (asymptomatic or symptomatic).

Index test(s)

Antibody tests

This review evaluates serology tests to measure antibodies to the SARS-CoV-2 virus. Antibodies are formed by the body's immune system in response to infections, and can be detected in whole blood, plasma or serum. Antibodies are specific to the virus, and therefore can be used to differentiate between different infections. There are three types of antibody created in response to infection: IgA, IgG and IgM; these rise and fall at different times after the onset of infection. IgG is used in most antibody tests as it persists for the longest time and may reflect longer-term immunity, although it is the last to rise after infection. Many tests assess both IgG and IgM. IgM typically rises quickly with infection and declines soon after an infection is cleared. Alternatively tests may combine IgA with IgG, or measure all antibodies (IgA, IgG and IgM).

Antibody tests are available for laboratory use including enzyme-linked immunosorbent assay (ELISA) methods, or more advanced chemiluminescence immunoassays (CLIA). There are also laboratory-independent, point-of-care lateral flow assays, which use disposable devices, akin to a pregnancy test, that use a minimal amount of blood on a testing strip. Antibody detection is indicated by visible lines appearing on the test strip, or through fluorescence, which can be detected using a reader device. Many of these tests are known as colloidal gold-based immunoassays, as they use COVID-19 antigen conjugated to gold nanoparticles.

Following the emergence of COVID-19 there has been prolific industry activity to develop accurate antibody tests. The Foundation for Innovative Diagnostics (FIND) and Johns Hopkins Centre for Health Security have maintained online lists of these and other molecular-based tests for COVID-19. At the time of writing (21 May 2020), FIND listed 279 antibody tests, 196 of which are produced by commercial companies and are commercially available. Reguatory approval in the European Union (EU; CE-IVD) had been awarded to 185 on the list, whereas in China only seven had been approved, and eight by the FDA (US Food and Drug Administration). For a period of time the FDA allowed commercialisation of antibody tests in the USA without FDA approval, resulting in around 100 tests being placed on the market. Both the content of the list, and these figures will increase over time.

Clinical pathway

Broadly speaking, there are four considered uses of antibody tests.

1. In diagnosis of acute suspected COVID-19 in patients who presented with symptoms, particularly where molecular testing had failed to detect the virus.
2. In assessment of immune response in patients with severe disease.
3. For individuals to assess whether they have had a SARS-CoV-2 infection and have an immune response.
4. In seroprevalence surveys for public health management purposes.

For 1, the standard approach to diagnosis of COVID-19 is through a reverse transcription polymerase chain reaction (RT-PCR) test, which detects the presence of virus in swab samples taken from nose, throat or fluid from the lungs. However, the test is known to give false negative results, and can only detect COVID-19 in the acute phase of the illness. Both the World Health Organization (WHO) and the China CDC (National Health Commission of the People's Republic of China), have produced case definitions for COVID-19 that include RT-PCR-negative cases that display other convincing clinical evidence (Appendix 1). The most recent case definition from the China CDC includes positive serology tests. Confirming an acute clinical diagnosis using a serology test requires detectable virus-specific IgM and IgG in serum, or detectable virus-specific IgG, or a 4-fold or greater increase in titration to be observed during convalescence compared with the acute phase.

For 2, this is largely a question of monitoring patients, and we will not cover this in this review. Assessment of the accuracy of a test used for assessment of immune response would involve comparison with a reference standard test of antibody response, rather than evidence of infection.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Use 3 involves testing individuals during periods of convalescence (after symptoms have resolved) whereas 4 will involve testing people at a mixture of time points, including long follow-up. A key difference between 3 and 4 is the likelihood of disease, which is expected to be much higher for 3 than 4.

An extended version of use case scenarios is available in Appendix 2.

Prior test(s)

Prior testing depends on the purpose of the test. For 1 we would anticipate that patients were symptomatic and had most likely undergone RT-PCR testing and possible computed tomography (CT) imaging. Uses 3 and 4 will most likely include people who have not been tested, and may include people who are asymptomatic as well as symptomatic.

Alternative test(s)

This review is one of six planned reviews that cover the range of tests and characteristics being considered in the management of COVID-19 (Deeks 2020; McInnes 2020). Full details of the alternative tests and evidence of their accuracy will be summarised in these reviews.

Laboratory-based molecular tests

Testing for presence of the SARS-CoV-2 virus has been undertaken using quantitative RT-PCR (qRT-PCR). RT-PCR tests for SARS-CoV-2 identify viral ribonucleic acid (RNA). Reagents for the assay were rapidly produced once the viral RNA sequence was published. Testing is undertaken in central laboratories and can be very labour-intensive, with several points along the path of performing a single test where errors may occur, although some automation of parts of the process is possible. Although the actual qRT-PCR test does not take long, the stages of extraction, sample processing and data management mean that test results are typically available in 24 to 48 hours, although faster processes are being implemented. Other nucleic acid amplification methods such as loop-mediated isothermal amplification (LAMP), or CRISPR-based nucleic acid detection methods are also being developed, with the potential to reduce the time to produce test results to minutes, but the time for the whole process may still be significant. RT-PCR tests use upper and lower respiratory samples. Sputum is currently considered better than oropharynx swabs or nasopharynx swabs but is more difficult (and hazardous) to obtain and will only ever be available in a subset of patients.

Laboratory-independent point-of-care and near-patient molecular and antigen tests

Laboratory-independent RT-PCR devices can also be used for identification of infection near patients and even at the bedside. These are small platforms for testing which use matching test cartridges. Several companies have suitable existing technology systems and are producing the required new cartridges for diagnosis of SARS-CoV-2 infection. Test results are based on the same samples as those for qRT-PCR, with results available within minutes or hours. Antigen tests are based on the direct detection of the virus, indicating active infection (i.e. replication of the virus) similar to the detection of RNA. Antigen tests are mainly in the form of lateral flow assays. They will capture the relevant viral antigen using dedicated antibodies, and visualisation is either manual or using a reader device.

Signs and symptoms

Signs and symptoms are used in the initial diagnosis of suspected COVID-19, and in identifying people with COVID-19 pneumonia. Key symptoms that have been associated with mild to moderate COVID-19 include: troublesome dry cough (for example, coughing more than usual over a one-hour period, or three or more coughing episodes in 24 hours), fever greater than 37.8°C, diarrhoea, headache, breathlessness on light exertion, muscle pain, fatigue, and loss of sense of smell and taste. Red flags indicating possible pneumonia include: breathlessness at rest, increased respiratory rate (above 20 breaths per minute), increased heart rate (above 100 beats per minute), chest tightness, loss of appetite, confusion, pain or pressure in the chest, blue lips or face, and temperature above 38°C. Hypoxia based on measuring pulse oximetry is often used, with various arbitrary thresholds (for example, 93%).

Routinely available biomarkers

Routinely available biomarkers for infection and inflammation may be considered in the investigation of people with possible COVID-19. For example, many healthcare facilities have access to standard laboratory tests for infection, such as C-reactive protein (CRP), procalcitonin, measures of anticoagulation, and white blood cell count with different lymphocyte subsets. Evaluation of these commonly available tests, particularly in low-resource settings, may be helpful for the triage of people with potential COVID-19.

Imaging tests

Chest X-ray, ultrasound, and CT are widely used diagnostic imaging tests to identify COVID-19 pneumonia. Availability and usage varies between settings.

Rationale

It is essential to understand the clinical accuracy of tests and diagnostic features to identify the best way they can be used in different settings to develop effective diagnostic and management pathways. The suite of Cochrane 'living systematic reviews' summarises evidence on the clinical accuracy of different tests and diagnostic features, grouped according to the research questions and settings that we are aware of. Estimates of accuracy from these reviews will help inform diagnosis, screening, isolation, and patient management decisions.

Particularly for antibody tests, new tests are being developed and evidence is emerging at an unprecedented rate during the COVID-19 pandemic. Tests are being purchased in bulk for seroprevalence studies, and made available for personal purchase online. This review will be updated as often as is feasible to ensure that it provides current evidence about the accuracy of antibody tests.

OBJECTIVES

To assess the diagnostic accuracy of antibody tests to determine if a person presenting in the community or in primary or secondary care has SARS-CoV-2 infection, or has previously had SARS-CoV-2 infection, and the accuracy of antibody tests for use in seroprevalence surveys.

Secondary objectives

Where data are available, we will investigate the accuracy (either by stratified analysis or meta-regression) according to:

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

- current infection or past infection;
- test method and brand;
- days since onset of symptoms;
- reference standard;
- study design;
- setting.

METHODS

Criteria for considering studies for this review

Types of studies

We applied broad eligibility criteria in order to include all patient groups and all variations of a test (that is, if patient population was unclear, we included the study).

We included studies of all designs that produce estimates of test accuracy or provide data from which estimates can be computed, including the following.

- Studies restricted to participants confirmed to have (or to have had) the target condition (to estimate sensitivity) or confirmed not to have (or have had) the target condition (to estimate specificity). These types of studies may be excluded in later review updates.
- Single-group studies, which recruit participants before disease status has been ascertained
- Multi-group studies, where people with and without the target condition are recruited separately (often referred to as two-gate or diagnostic case-control studies)
- Studies based on either patients or samples

We excluded studies from which we could not extract data to compute either sensitivity or specificity.

We carefully considered the limitations of different study designs in the quality assessment and analyses.

We included studies reported in published articles and as preprints.

Participants

We included studies recruiting people presenting with suspicion of current or prior SARS-CoV-2 infection or those recruiting populations where tests were used to screen for disease (for example, contact tracing or community screening).

We also included studies that recruited people either known to have SARS-CoV-2 infection or known not to have SARS-CoV-2 infection (multi-group studies).

We excluded small studies with fewer than 10 samples or participants. Although the size threshold of 10 is arbitrary, such small studies are likely to give unreliable estimates of sensitivity or specificity and may be biased.

Index tests

We included studies evaluating any test for detecting antibodies to SARS-CoV-2, including laboratory-based methods and tests designed to be used at point-of-care. Test methods include the following.

Laboratory-based:

- enzyme-linked immunosorbent assays (ELISA)
- chemiluminescence immunoassays (CLIA)
- other laboratory-based methods (e.g. indirect immunofluorescence tests (IIFT), luciferase immunoprecipitation system (LIPS)

Rapid diagnostic tests:

- lateral flow assays, including both colloidal gold or fluorescence-labelled immunochromatographic assays (CGIA or FIA).

In this first version of the review we have included both commercially available tests, which have regulatory approval, with in-house assays and assays in development. Future versions of the review are likely to be restricted to only commercially available assays.

We identified the regulatory status of index tests using two main resources:

- WHO: COVID-19 listing in International Medical Device Regulators Forum (IMDRF) jurisdictions (www.who.int/diagnostics_laboratory/EUL/en/), which includes listings of FDA, Health Canada, Japan, Australia (Therapeutic Goods Administration), Singapore (Health Sciences Authority), Brazil (Agência Nacional de Vigilância Sanitária), South Korea (Ministry of Food and Drug Safety), China (National Medical Products Administration), and Russia (Roszdravnadzor);
- FIND: SARS-COV-2 Diagnostic Pipeline (www.finddx.org/covid-19/pipeline/), which overlaps with the WHO list, but in addition includes CE-IVD and IVD India.

In addition, we checked key national websites, including US FDA (www.fda.gov/medical-devices/emergency-situations-medical-devices/emergency-use-authorizations#coronavirus2019) and China FDA (subsites.chinadaily.com.cn/nmpa/2020 03/27/c_465663.htm?bsh_bid=5496527208).

Target conditions

The target conditions were the identification of:

- current SARS-CoV-2 infection (in symptomatic cases);
- past SARS-CoV-2 infection (in convalescent (post-symptomatic) or asymptomatic cases).

Reference standards

We anticipated that studies would use a range of reference standards to define both the presence and absence of SARS-CoV-2 infection but were unclear at the start of the review exactly what methods would be encountered. For the QUADAS-2 (Quality Assessment tool for Diagnostic Accuracy Studies; Whiting 2011), assessment we categorised each method of defining COVID-19 cases according to the risk of bias (the chances that it would misclassify COVID-19 participants as non-COVID-19) and whether it defined COVID-19 in an appropriate way that reflected cases encountered in practice. Likewise, we considered the risk of bias in definitions of non-COVID-19, and whether the definition reflected those who, in practice, would be tested.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Search methods for identification of studies

Electronic searches

We conducted a single literature search to cover our suite of Cochrane COVID-19 diagnostic test accuracy (DTA) reviews (Deeks 2020; McInnes 2020).

We conducted electronic searches using two primary sources. Both of these searches aimed to identify all published articles and preprints related to COVID-19, and were not restricted to those evaluating biomarkers or tests. Thus, there are no test terms, diagnosis terms, or methodological terms in the searches. Searches were limited to 2019 and 2020, and for this version of the review have been conducted to 27 April 2020.

Cochrane COVID-19 Study Register searches

We used the Cochrane COVID-19 Study Register (covid-19.cochrane.org/), for searches conducted to 28 March 2020. At that time, the register was populated by searches of PubMed, as well as trials registers at ClinicalTrials.gov and the WHO International Clinical Trials Registry Platform (ICTRP).

Search strategies were designed for maximum sensitivity, to retrieve all human studies on COVID-19 and with no language limits. See Appendix 3.

COVID-19 Living Evidence Database from the University of Bern

From 28 March 2020, we used the COVID-19 Living Evidence database from the Institute of Social and Preventive Medicine (ISPM) at the University of Bern (www.ispm.unibe.ch), as the primary source of records for the Cochrane COVID-19 DTA reviews. This search includes PubMed, Embase, and preprints indexed in bioRxiv and medRxiv databases. The strategies as described on the ISPM website are described here (ispmbern.github.io/covid-19/). See Appendix 4.

The decision to focus primarily on the 'Bern' feed was due to the exceptionally large numbers of COVID-19 studies available only as preprints. The Cochrane COVID-19 Study Register has undergone a number of iterations since the end of March and we anticipate moving back to the Register as the primary source of records for subsequent review updates.

Searching other resources

We identified Embase records obtained through Martha Knuth for the Centers for Disease Control and Prevention (CDC), Stephen B Thacker CDC Library, COVID-19 Research Articles Downloadable Database (www.cdc.gov/library/researchguides/2019novelcoronavirus/researcharticles.html), and de-duplicated them against the Cochrane COVID-19 Study Register up to 1 April 2020. See Appendix 5.

We also checked our search results against two additional repositories of COVID-19 publications including:

- the Evidence for Policy and Practice Information and Co-ordinating Centre (EPPI-Centre) 'COVID-19: Living map of the evidence' (eppi.ioe.ac.uk/COVID19_MAP/covid_map_v4.html);
- the Norwegian Institute of Public Health 'NIPH systematic and living map on COVID-19 evidence' (www.nornesk.no/forskningskart/NIPH_diagnosisMap.html)

Both of these repositories allow their contents to be filtered according to studies potentially relating to diagnosis, and both have agreed to provide us with updates of new diagnosis studies added. For this iteration of the review, we examined all diagnosis studies from either source up to 16 April 2020.

In addition we have used the list of potentially eligible index tests (documented in Criteria for considering studies for this review), to search company and product websites for studies about test accuracy and to contact companies to request further information or studies using their tests. We will include the result of this process in a future iteration of this review.

We have also contacted research groups undertaking test evaluations (for example, UK Public Health England-funded studies, and FIND studies (www.finddx.org/). We appeal to researchers to supply details of additional published or unpublished studies at the following email address, which we will consider for inclusion in future updates (coviddta@contacts.bham.ac.uk).

We did not apply any language restrictions.

Data collection and analysis

Selection of studies

A team of experienced systematic reviewers from the University of Birmingham screened the titles and abstracts of all records retrieved from the literature searches. Two review authors independently screened studies in Covidence. A third, senior review author resolved any disagreements. We tagged all records selected as potentially eligible according to the Cochrane COVID-19 DTA review(s) that they might be eligible for and we then exported them to separate Covidence reviews for each review title.

We obtained the full texts for all studies flagged as potentially eligible. Two review authors independently screened the full texts for one of the COVID-19 molecular or antibody test reviews. We resolved any disagreements on study inclusion through discussion with a third review author.

Data extraction and management

One review author carried out data extraction, which was checked by a second review author. Items that we extracted are listed in Appendix 6. Both review authors independently performed data extraction of 2x2 contingency tables of the number of true positives, false positives, false negatives and true negatives. They resolved disagreements by discussion.

We encourage study authors to contact us regarding missing details on the included studies (coviddta@contacts.bham.ac.uk).

Where possible we extracted 2x2 tables according to time since onset of symptoms. We predefined groups of interest as 1-7, 8-14, 15-21, 22-35 and over 35 days since onset of symptoms. Where the data presented did not exactly match these categorisations we entered data in the time group that had the greatest overlap with our groupings. Where a study presented data for a group without stating an upper time limit (e.g. more than 21 days) we placed the data in the first category above the stated value (e.g. 22-35 days).

Where possible, we separately extracted data related to each class of antibody (IgA, IgG and IgM), and combinations of classes (IgA/

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

IgM, IgA/IgG, IgG/IgM, where a positive is defined as either or both classes of antibody being detected). We also extracted data on total antibodies where this was reported.

Assessment of methodological quality

Two review authors independently assessed risk of bias and applicability concerns using the QUADAS-2 checklist tailored to this review (Appendix 7; Whiting 2011). The two review authors resolved any disagreements by discussion.

Ideally, studies should prospectively recruit a representative sample of participants presenting with signs and symptoms of COVID-19, either in community or primary care settings or to a hospital setting, and they should clearly record the time of testing after the onset of symptoms. Studies should perform antibody tests in their intended use setting, using appropriate sample types as described in the 'Instructions for use' sheet (e.g. fingerprick blood for tests being evaluated for use as point-of-care tests), and tests should be performed by relevant personnel (e.g. healthcare workers), and should be interpreted blinded to the final diagnosis (COVID-19 or not). Serology samples should be taken at time points that reflect the intended use (either whilst symptomatic for diagnosis of infection, or during a convalescent period (after resolution of symptoms) for diagnosis of previous infection). The reference standard diagnosis should be blinded to the result of the antibody test, and should not incorporate the result of the index test or any other serology test. If the reference standard includes clinical diagnosis of COVID-19, then established criteria should be used. Studies including samples from participants known not to have COVID-19 should use pre-pandemic sources or contemporaneous samples with at least one RT-PCR-negative test result. Data should be reported for all study participants, including those where the result of the antibody test was inconclusive, or participants in whom the final diagnosis of COVID-19 was uncertain. If studies obtained multiple samples for testing over time from the same study participants, then they should disaggregate results by time post-symptom onset.

Statistical analysis and data synthesis

We grouped data by study and test. Thus studies that evaluated multiple tests in the same participants were included multiple times. We present estimates of sensitivity and specificity for each antibody (or combination of antibodies) using paired forest plots in tables, and also summarise them in tables as appropriate.

For analysis purposes, unlike in most DTA reviews we considered estimates of sensitivity and specificity separately, because many of the included studies presented only estimates of sensitivity. Estimates of specificity were typically exceptionally high, thus the correlation between sensitivity and specificity across studies was unlikely to be high (Macaskill 2010; Takwoingi 2017). We considered the heterogeneity in the study findings through visual inspection of forest plots when deciding to meta-analyse study estimates, and have not computed summary estimates where they were likely to be regarded as misleading.

Where we pooled results, we fitted random-effects logistic regression models using the meqrlogit command in Stata v15.1 (Stata). In a small number of instances, the random-effects logistic regression analyses failed to converge (usually when there were very small numbers of studies), and we have computed estimates and confidence intervals by summing the counts of true positive, false positive, false negative and true negative across 2x2 tables. These analyses are clearly marked in the tables. We present all estimates with 95% confidence intervals.

Investigations of heterogeneity

We investigated sources of heterogeneity in two ways. First, for analysis of sensitivity for time since onset of symptoms, we extracted data by week and extended the random-effects logistic regression model to include indicator variables for each week. There was a strong relationship between time since onset of symptoms and sensitivity, thus we elected to fit all subsequent models for investigation of heterogeneity in sensitivity stratifying by week. We excluded studies for which stratified data were not available at this stage. For analysis of sensitivity according to the RT-PCR status of patients (RT-PCR positive ‘confirmed’ and RT-PCR negative ‘suspect’), we extracted 2x2 tables stratified by RT-PCR result (as well as week) and extended the random-effects logistic regression to include terms for week and RT-PCR status.

We investigated heterogeneity related to study design, reference standard and test technology by including indicator variables in the random-effects logistic regression model alongside the variables for week since onset of symptoms. We present estimates from these models by test or reference standard type for the sensitivity of the test in the third week since onset of symptoms (since this is the time point most commonly recommended for post-infection testing to start to be undertaken).

We did not fit models to compare test brands due to the small number of studies available, but we do report estimates with confidence intervals for each brand.

Sensitivity analyses

We planned to undertake sensitivity analyses by excluding:

- unpublished studies;
- studies identified only from industry 'Instructions for use' documentation;
- studies using sample banks or spiked samples;
- studies with inadequate reference standards;
- for previous infection, we also planned to assess increasing lengths of time since symptoms cleared.

In this version of the review we did not undertake any of these analyses because the majority of studies were preprints, we did not include any company documents, and no study used spiked samples. We investigated issues with reference standards and time as part of the investigations of heterogeneity.

Assessment of reporting bias

We made no formal assessment of reporting bias. However we were aware of the manner in which results in studies could be suppressed by test developers or manufacturers, and detail where we believe this may have happened.

Summary of findings

We summarised key findings in a 'Summary of findings' table indicating the strength of evidence for each test and findings, and highlighted important gaps in the evidence.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Updating

We are aware that a substantial number of studies have been published since the search date of 27 April 2020 and plan to update this review imminently. We have already completed searches for the update up until 25 May 2020, and report the number of studies that we anticipate will be added to this review in the first update.


RESULTS

Results of the search

We screened 10,965 unique references (published or preprints) for inclusion in the complete suite of reviews to assist in the diagnosis of COVID-19 (Deeks 2020; McInnes 2020). Of 1430 records selected for further assessment for inclusion in any of the six reviews, we assessed 267 full-text reports for inclusion in this review. See Figure 1 for the PRISMA flow diagram of search and eligibility results (McInnes 2018; Moher 2009). We included 54 studies from 57 reports in this review, three studies are awaiting assessment including two foreign language papers and one study of neutralising antibodies (Characteristics of studies awaiting classification), 34 are ongoing studies (Characteristics of ongoing studies), and we excluded 172 publications. Exclusions were mainly due to ineligible study designs (n = 84) or index tests (n = 40), or because we could not extract or reconstruct 2x2 data (n = 21). The reasons for exclusion of all 172 publications are provided in Characteristics of excluded studies.


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 1. Study flow diagram

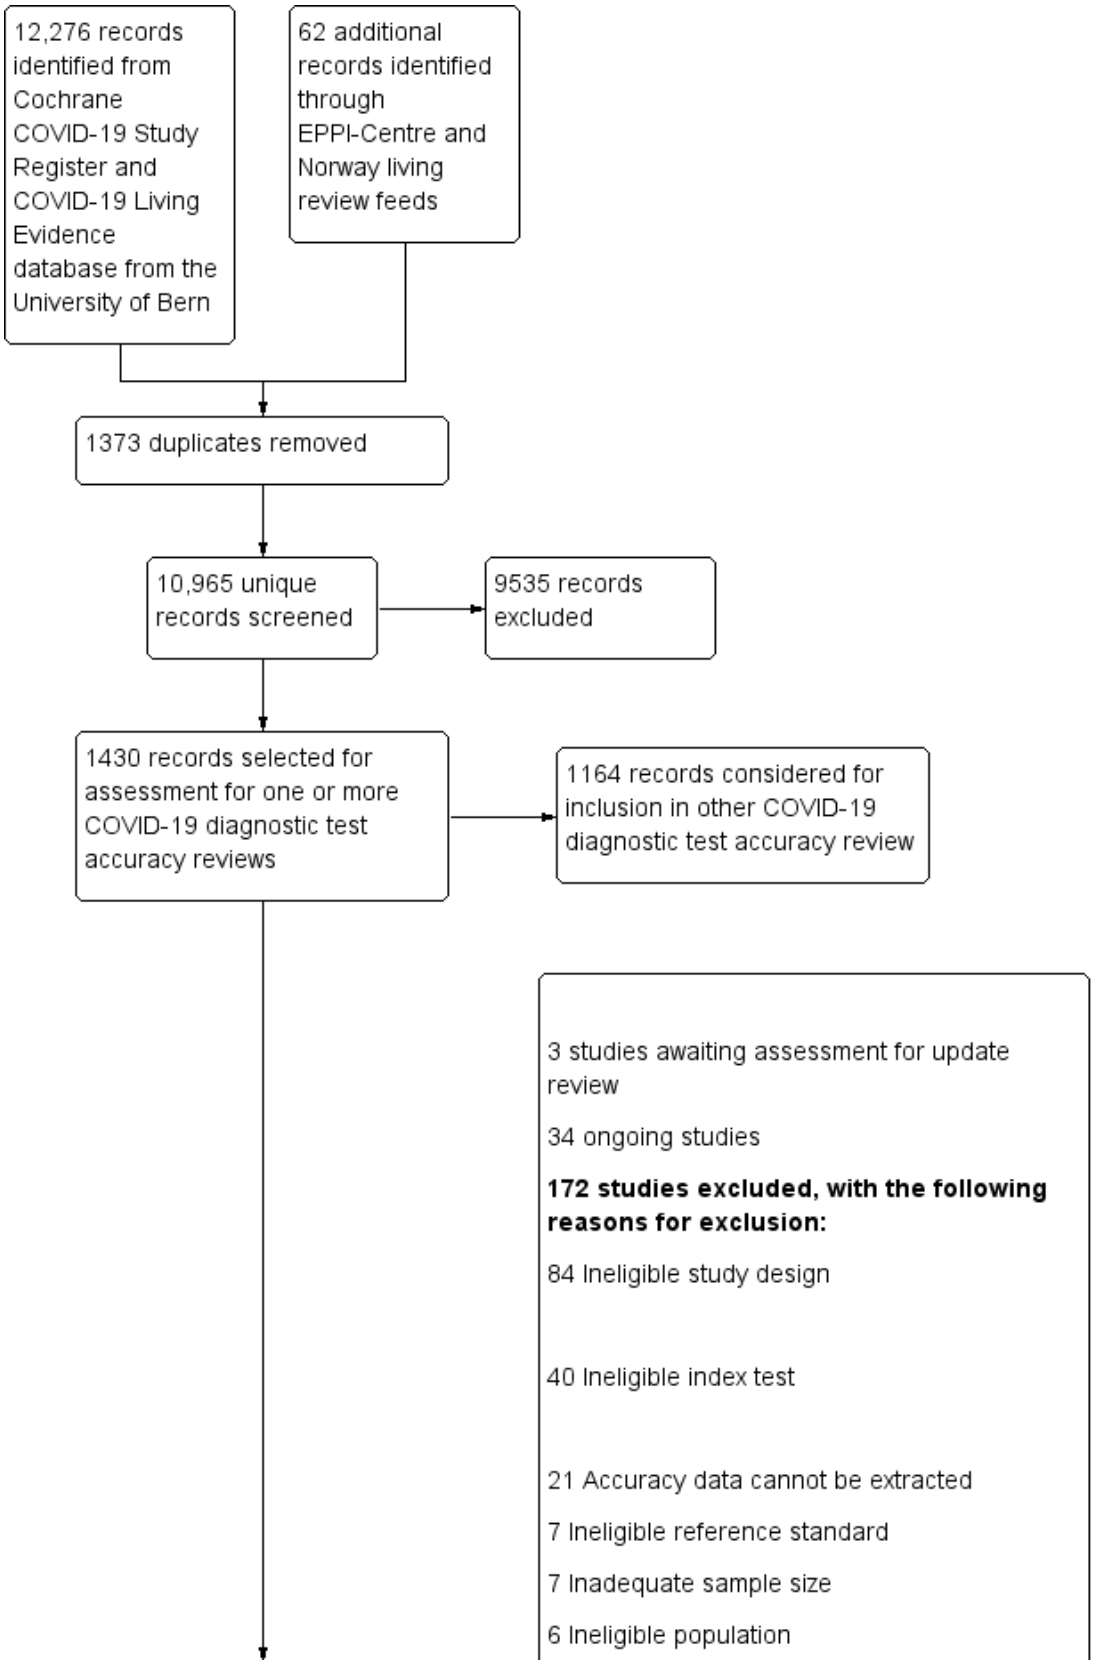

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 1. (Continued)

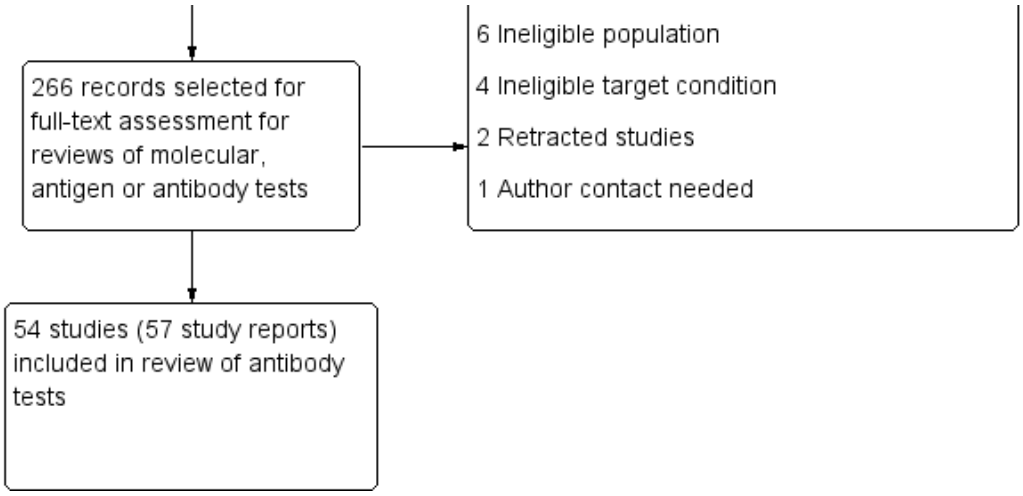

The 57 included study reports relate to 54 separate studies, six studies (Gao 2020a; Liu 2020d [A]; Pan 2020a; Okba 2020a; Wang 2020a [A]; Zhao 2020a), having two publications each, and three studies providing data for two separate cohorts of participants (Cassaniti 2020 (A); Cassaniti 2020 (B); Garcia 2020 (A); Garcia 2020 (B); Long 2020 (A); Long 2020 (B)). Of the 57 study reports, 28 studies are available only as preprints and four as preprints with subsequent journal publications. (Please note when naming studies, we use the letters (A), (B), (C) in standard brackets to indicate multiple studies from the same publication, and the letters [A], [B], [C] etc. in square brackets to indicate data on different tests evaluated in the same study).

Description of included studies

The 54 studies include a total of 15,976 samples, with 8526 samples from cases of COVID-19. Summary study characteristics are presented in Table 1 with further details of study design and index test details in Appendix 8 and Appendix 9. The median sample size across the included studies is 129.5 (interquartile range (IQR) 57 to 347) and median number of COVID-19 cases included is 62 (IQR 31 to 151). Thirty-eight studies were conducted in Asia: China (n = 36); Hong Kong (n = 1); or Singapore (n = 1). Fifteen studies were conducted in Europe, and the remaining study included samples from more than one country (Bendavid 2020). Forty-four studies included only hospital inpatient cases, one included hospital outpatients, two included participants attending emergency departments, two, community screening (including one study of close contacts). Five studies were conducted in mixed or unclear settings.

Participant characteristics

Twenty-three studies included cases during the early phase of illness only (< 21 days post-symptom onset), two only included cases 21 days or more post-symptom onset, 23 included mixed groups and six did not report days post-symptom onset. Few studies were clear whether participants were symptomatic or convalescent (i.e. symptoms had resolved) at the time of testing. It is therefore difficult to clearly separate out studies that detected current infection from studies that detected past infection. Thus the two target conditions we defined cannot clearly be distinguished. There were no studies exclusively in asymptomatic participants.

The mean or median age of included COVID-19 cases ranges from 37 to 76 years (reported in 31 studies), and 26% to 87% of participants were male (reported in 31 studies). Full details are in the Characteristics of included studies table.

Study designs

We identified six studies that recruited suspected COVID-19 cases before it was ascertained whether the patients did or did not have COVID-19. These six studies identified people with suspected COVID-19 based on symptoms or as close contacts of confirmed cases (symptomatic and asymptomatic). Sample sizes of these studies ranged from 50 to 814 with between 3 and 154 COVID-19 cases. Four of these studies defined the presence or absence of COVID-19 based on RT-PCR alone, and two also included clinically confirmed RT-PCR-negative cases based on undefined clinical suspicion or CT findings. The absence of SARS-CoV-2 infection was confirmed by a single RT-PCR-negative result in five of the six and by two or more negative RT-PCR results in one study.

The other forty-eight studies retrospectively recruited patients when it was already known whether or not they had COVID-19.

Twenty-nine studies used two- or multi-group study designs with separate selection of COVID-19 cases and healthy participants or non-COVID-19 participants with another disease. Sample sizes ranged from 17 to 3481 with between 7 and 276 COVID-19 cases. Nineteen of these studies defined COVID-19 cases based on a positive RT-PCR test, six included clinically defined RT-PCR-negative cases in addition to RT-PCR-positive cases and the remaining four studies used mixed or unclear criteria to define the presence of COVID-19. Four of the 29 studies included participants with suspected COVID-19 but who had subsequently been ruled out on the basis of one (2 studies) or more (2 studies) negative RT-PCR tests. Ten included contemporaneous non-COVID-19 groups, including samples from healthy participants (5 studies), patients with other diseases (one study) or both (4 studies), only two of which used RT-PCR testing to exclude the presence of SARS-CoV-2. Twelve studies included pre-pandemic non-COVID 19 groups, using samples from either healthy people (n = 5), participants with other diseases (n = 3), or both (n = 4). The remaining three studies included control samples from mixed sources including pre-

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

pandemic and contemporaneous samples, with or without RT-PCR testing.

Nineteen studies included only a single group of only COVID-19 cases, thus only allowing estimation of sensitivity. They determined COVID-19 cases based on positive RT-PCR alone (n = 9), clinically defined criteria including RT-PCR-negative cases (n = 8, 7 of which used Chinese government-issued COVID-19 guidelines to define cases), one using undefined clinical criteria, and one study that did not report how COVID-19 cases were defined.

Index tests

Forty-three studies evaluated only one test, five compared two tests, three compared 3 tests, one 5 tests, one 9 and one 10 tests. In total the 54 studies reported on a total of 89 test evaluations.


There were 52 evaluations of laboratory-based methods (27 ELISA, 19 CLIA, 6 other methods), including 32 using commercially available laboratory-based kits produced by 11 different commercial companies (16 ELISAs, 15 CLIAs and 1 IIFT), two where the manufacturer name was withheld, and 20 classified as using in-house methods (11 ELISA, 4 CLIA and 5 other approaches).

There were 34 evaluations of lateral flow assays, 23 were described as or discovered to be CGIA, two were FIAs and nine were not described. Thirty-one of the 34 evaluations used commercially available lateral flow assays and three were in-house (including two CGIA and one FIA). Of the 34 evaluations, only three used whole blood (two using the Vivadiag test), and only two used the assays as point-of-care tests rather than in a laboratory setting.

Methodological quality of included studies

We report the overall methodological quality assessed using the QUADAS-2 tool for all included studies (n = 54) in Figure 2 (Whiting 2011). See Appendix 10 for study-level ratings by quality.

Figure 2. Risk of bias and applicability concerns graph: review authors' judgements about each domain presented as percentages across included studies

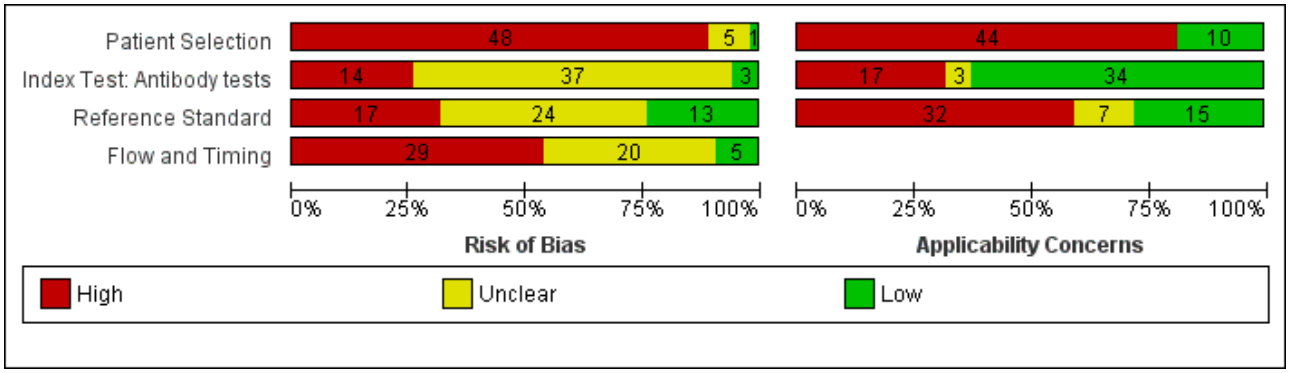

Overall, we judged risk of bias to be high in 48 (89%) studies concerning how participants were selected, 14 (26%) studies related to application of the index test, 17 (31%) through concerns about the reference standard and 29 (54%) for issues related to participant flow and timing. No study had low risk in all domains. We judged that there were high concerns about the applicability of the evidence related to participants in 44 (81%) studies, 17 (31%) related to the index test and 32 (59%) related to the reference standard. Explanations of how we have reached these judgements are given below and in the Characteristics of included studies table.

Participant selection

For participant selection, we judged only one study to be at low risk of bias and five to be of unclear risk. The remaining 48 (89%) we judged to be at high risk of bias (n = 44) either due to the use of a multi-group design with healthy or other disease controls (n = 26) or recruitment of only COVID-19 cases (n = 19), inappropriate exclusions (n = 2) or inappropriate inclusions (n = 15). Numbers per group are not mutually exclusive. Eleven studies (20%) reported consecutive or random recruitment of participants.

We had high concerns about the applicability of the selection of participants in 44 studies (81%) meaning that the participants who were recruited were unlikely to be similar to those in whom the test would be used in clinical practice. This was largely because studies only recruited hospitalised, confirmed cases of COVID-19, often with severe symptoms (18 studies) or recruited healthy or other disease non-COVID-19 groups (26 studies). We judged 10 (19%) studies likely to have selected an appropriate patient group, including the six studies that recruited participants suspected of COVID-19 prior to definitive testing and four multi-group studies that separately recruited COVID-19 cases and suspected COVID-19 control groups.

Index tests

Eight studies explicitly reported that they had undertaken the index test with knowledge of whether individuals did or did not have COVID-19, and eight studies determined the threshold to define test positivity by analysing the data, rather than it being pre-determined. In 37 studies, reporting of one or both of these issues was too unclear to be able to rule out the possibility of bias. These issues led to the index test performance in 14 studies being rated as at high risk of bias. We judged only three studies to have implemented the index test in a way that protected against the risk of bias.

In 34 studies (63%) we judged the test to be implemented as it would be in practice. Twenty-two of these were evaluations of laboratory-based, commercially available tests, and 12 were evaluations of lateral flow assays associated with commercial test manufacturers, primarily evaluated in an inpatient setting. Two of the 12 evaluated the assays as point-of-care tests in an emergency

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

room setting. Sixteen studies raised concerns that the tests could not be purchased (high concerns for applicability). The remaining four studies provided inadequate information to make a judgement due to withholding of the names of the commercial tests (one additional study also withheld the names of the lateral flow assays evaluated but scored high concerns as it also reported results for an in-house ELISA test).

Reference standards

We judged 13 studies (24%) to have used an appropriate reference standard and implemented it in ways that prevented bias. In six studies there was a risk of misclassification, as they had used a single, negative RT-PCR result to define the absence of disease in people with suspected COVID-19; eight studies did not report any RT-PCR testing to confirm COVID-19 status for contemporaneous healthy or other disease non-COVID-19 groups; and one study used serology results in part to determine the reference standard diagnosis, thus risking incorporation bias. We judged 24 studies as having unclear risk of bias due to lack of information about blinding of the reference standard to the index test (19/24) or unclear descriptions of the reference standards used (6/24).

We judged the reference standard to be equivalent to WHO or China CDC definitions of COVID-19 in 15 studies (28%). We judged studies that used a definition based only on RT-PCR-positive results as high concern (32 (59%) of studies), and seven studies reported inadequate detail to assess the reference standard.

Flow and timing

Twenty-nine (54%) studies were at high risk of bias due to using different reference standards to verify COVID-19 and non-COVID-19 cases (n = 19), participants being excluded from the analysis (n = 15), or the inclusion of multiple samples per participant (n = 7). In 20 (37%) studies we could not make judgements on one or more of these issues, primarily due to lack of clarity around participant inclusion and exclusion from analyses. Five studies reported adequate detail to rule out these risks of bias. None of the included studies reported a Standards of Reporting Diagnostic Accuracy Studies (STARD)-style participant flow diagram (Bossuyt 2015), and none mentioned that they aimed to report in line with STARD reporting recommendations for test accuracy studies.

In 39 studies all authors declared no conflicts of interest although four included co-authors affiliated to test manufacturers. Ten studies did not provide a conflict of interest statement (two of these included co-authors affiliated to test manufacturers or biotechnology companies); and in the five remaining studies at least one author declared conflicts of interest in relation to test manufacturers (four studies) or vaccine companies (one study).

Nine studies provided no funding statement, six reported no funding sources to declare, and 39 studies reported one or more funding sources. The reported funding sources were primarily public funding sources. Two studies reported receipt of equipment ‘in kind’ from test manufacturers and two studies reported private donors.

Findings

We included 54 different studies, which were reported in 57 publications. Fourteen of the 54 studies evaluated more than one test (Table 1), up to a maximum of 10 tests per study. To incorporate all results from all tests, in these analyses we have treated results from different tests of the same samples within a study as separate data points, such that data are available on 89 test-study combinations. This leads to individual samples being included in some analyses multiple times where they have been evaluated using different tests. To identify where estimates are based on multiple assessments of the same sample sets, the tables include both the number of test-study combinations and the number of studies. The numbers of true positives, false positives, COVID-19 samples and non-COVID samples are based on test result counts.

Overall analyses

We are unable to distinguish between studies that evaluated the accuracy of antibody tests to identify current infection from past infection. Whilst time since onset of symptoms is strongly related to whether an infection was current or past, few studies reported whether participants' symptoms had resolved (and thus they were in a convalescent state) when serology samples were taken. Whilst 21 days post-symptom onset is assumed to be a point where COVID-19 cases are likely to be convalescent, many participants in these studies were hospitalised for prolonged periods and likely to reflect those with more severe and long-lasting symptoms.


A key aspect of interpreting the sensitivity of the tests is the relationship between accuracy and days since onset of symptoms. Sixteen (30%) studies only presented results aggregated over 0 to more than 35 days since onset, and did not present data (or provide datasets) that disaggregated data by week. The figures in Appendix 11 show forest plots of sensitivity and specificity estimates including these studies for IgG, IgM, and IgG/IgM (either positive), which clearly depict substantial heterogeneity in sensitivity, with estimates ranging from 0% to 100% for all three markers. Forest plots of results for IgA, total antibodies, IgA/IgG, IgA/IgM (Appendix 11), show similar heterogeneity with smaller numbers of studies. Given the heterogeneity and the known strong relationship of sensitivity with time, computation of an average estimate of sensitivity from these studies would be misleading and serves no purpose.

Sensitivity by time since onset of symptoms

Table 2 and Figure 3 present the results disaggregated by week of testing since onset of symptoms for IgG (from 23 studies), IgA (from 4 studies), IgM (from 24 studies), total antibodies (from 5 studies), combination of IgG/IgM (from 21 studies), and IgA/IgG (from 1 study; these results are based on a maximum of 12 participants per time period and we will not comment on them further). We did not find any data disaggregated by week for IgA/IgM. Forest plots of these data are given in Figure 4, Figure 5 and Figure 6. We have undertaken meta-analyses of data stratified by week as heterogeneity, whilst still present, is substantially less. As indicated in Table 2, the strength of the relationship of time with sensitivity shows exceptionally high levels of statistical significance ($P < 0.0005$). All further analyses of sensitivity in this report are thus stratified by week since symptom onset.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 3. Meta-analytical estimates of sensitivity (with 95% CI) by antibody class and time since onset of symptoms

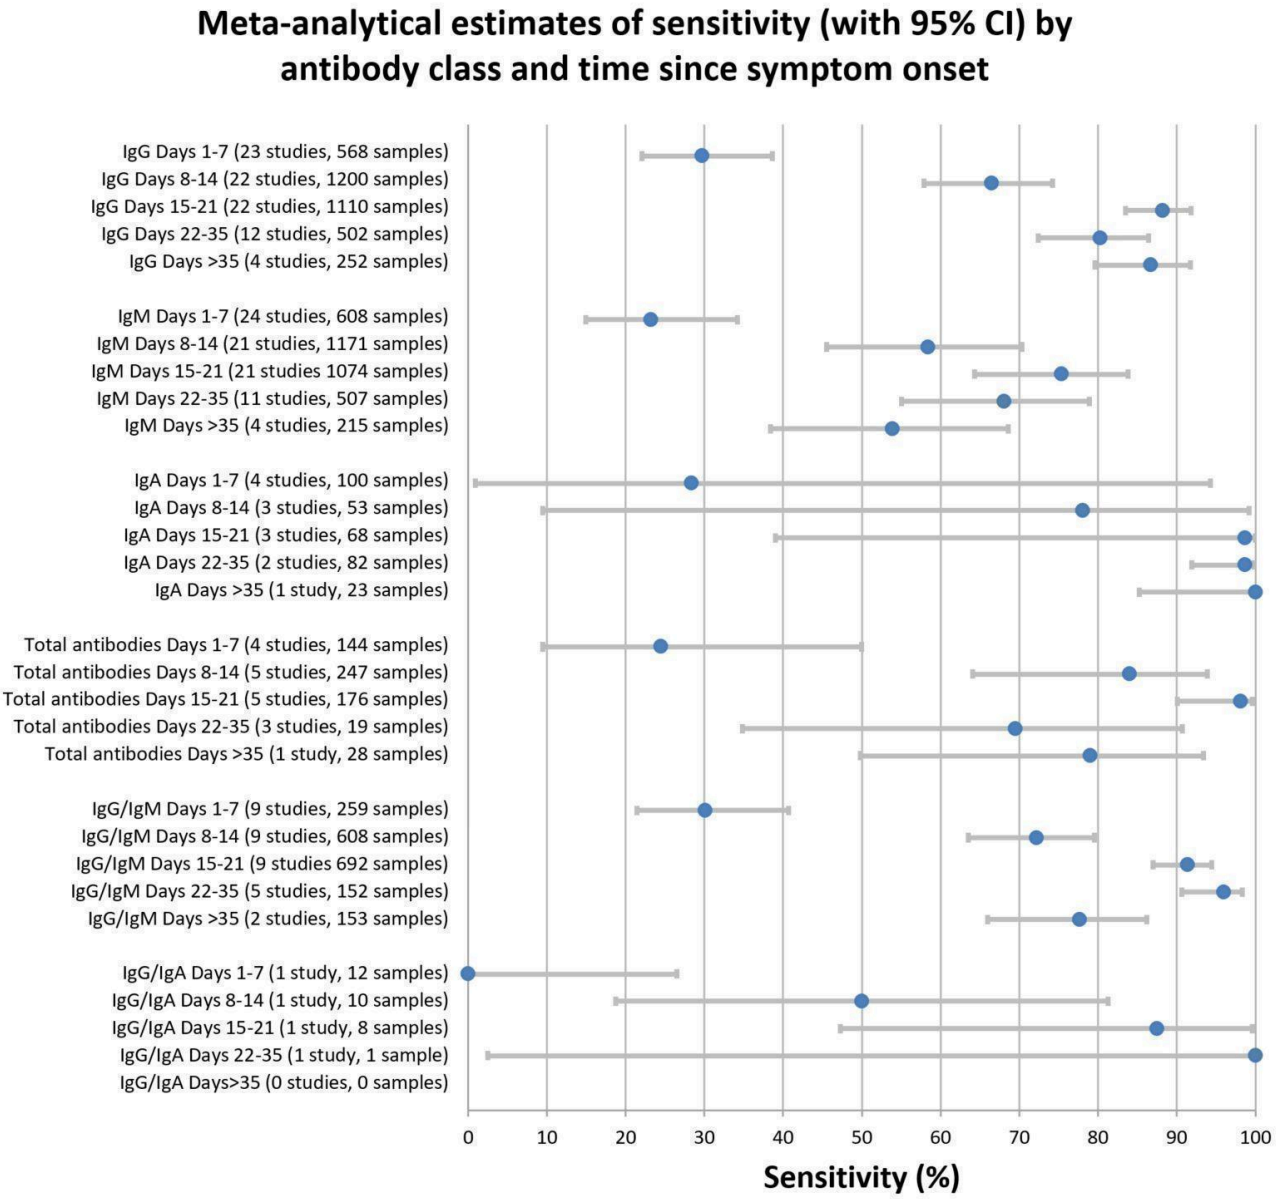


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 4. Forest plot of studies evaluating tests for detection of IgG according to week post-symptom onset and type of test


IgG (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	2	0	8	0	CGIA	Beijing Beier Bioengineering	0.20 [0.03, 0.56]	Not estimable
Garcia 2020 (A)	1	0	7	0	CGIA	Hangzhou Alltest - IgG/IgM	0.13 [0.00, 0.53]	Not estimable
Gao 2020a	7	0	6	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.54 [0.25, 0.81]	Not estimable
Liu 2020a	2	0	14	0	CGIA	Withheld	0.13 [0.02, 0.38]	Not estimable
Pan 2020a	5	0	31	0	CGIA	Zhuhai Livzon	0.14 [0.05, 0.29]	Not estimable
Gao 2020b [A]	4	0	6	0	CLIA	Beijing Beier Bioengineering	0.40 [0.12, 0.74]	Not estimable
Hu 2020a	11	0	14	0	CLIA	Bioscience Co (Chongqing)	0.44 [0.24, 0.65]	Not estimable
Long 2020 (B)	32	0	35	0	CLIA	Bioscience Co (Chongqing)	0.48 [0.35, 0.60]	Not estimable
Lin 2020a [A]	8	0	4	0	CLIA	In-house	0.67 [0.35, 0.90]	Not estimable
Ma 2020a	15	0	2	0	CLIA	In-house	0.88 [0.64, 0.99]	Not estimable
Jin 2020	2	0	4	0	CLIA	Shenzhen YHLO	0.33 [0.04, 0.78]	Not estimable
Xiao 2020a	0	0	2	0	CLIA	Shenzhen YHLO	0.00 [0.00, 0.84]	Not estimable
Lippi 2020 [A]	7	0	23	0	CLIA	Snibe Diagnostic - MAGLUMI	0.23 [0.10, 0.42]	Not estimable
Padoan 2020	4	0	6	0	CLIA	Snibe Diagnostic - MAGLUMI	0.40 [0.12, 0.74]	Not estimable
Gao 2020b [C]	4	0	6	0	ELISA	Beijing Beier Bioengineering	0.40 [0.12, 0.74]	Not estimable
Liu 2020d [B]	9	0	13	0	ELISA	Beijing Hotgen	0.41 [0.21, 0.64]	Not estimable
Lou 2020 [A]	13	0	26	0	ELISA	Beijing Wantai	0.33 [0.19, 0.50]	Not estimable
Zhao 2020a	18	0	76	0	ELISA	Beijing Wantai	0.19 [0.12, 0.29]	Not estimable
Lippi 2020 [B]	0	0	30	0	ELISA	EUROIMMUN	0.00 [0.00, 0.12]	Not estimable
Okba 2020a	0	0	12	0	ELISA	EUROIMMUN Beta	0.00 [0.00, 0.26]	Not estimable
Adams 2020 [A]	0	0	4	0	ELISA	In-house	0.00 [0.00, 0.60]	Not estimable
Liu 2020b	4	0	13	0	ELISA	Zhuhai Livzon	0.24 [0.07, 0.50]	Not estimable
Liu 2020d [A]	7	0	15	0	ELISA	Zhuhai Livzon	0.32 [0.14, 0.55]	Not estimable
Xiang 2020b	6	0	8	0	ELISA	Zhuhai Livzon	0.43 [0.18, 0.71]	Not estimable
Zeng 2020a	0	0	27	0	ELISA	Zhuhai Livzon	0.00 [0.00, 0.13]	Not estimable
Wan 2020 [A]	1	0	3	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [D]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [H]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [J]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable

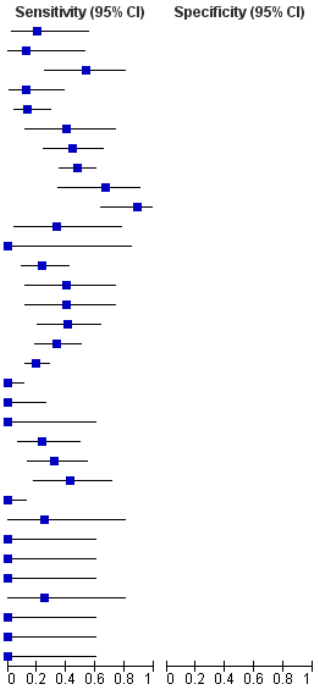


IgG (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	6	0	7	0	CGIA	Beijing Beier Bioengineering	0.46 [0.19, 0.75]	Not estimable
Garcia 2020 (A)	6	0	18	0	CGIA	Hangzhou Alltest - IgG/IgM	0.25 [0.10, 0.47]	Not estimable
Garcia 2020 (B)	15	0	3	0	CGIA	Hangzhou Alltest - IgG/IgM	0.83 [0.59, 0.96]	Not estimable
Gao 2020a	7	0	1	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.88 [0.47, 1.00]	Not estimable
Liu 2020a	5	0	1	0	CGIA	Withheld	0.83 [0.36, 1.00]	Not estimable
Pan 2020a	20	0	14	0	CGIA	Zhuhai Livzon	0.59 [0.41, 0.75]	Not estimable
Gao 2020b [A]	6	0	7	0	CLIA	Beijing Beier Bioengineering	0.46 [0.19, 0.75]	Not estimable
Hu 2020a	97	0	48	0	CLIA	Bioscience Co (Chongqing)	0.67 [0.59, 0.74]	Not estimable
Long 2020 (B)	32	0	35	0	CLIA	Bioscience Co (Chongqing)	0.48 [0.35, 0.60]	Not estimable
Lin 2020a [A]	24	0	9	0	CLIA	In-house	0.73 [0.54, 0.87]	Not estimable
Ma 2020a	29	0	1	0	CLIA	In-house	0.97 [0.83, 1.00]	Not estimable
Jin 2020	26	0	1	0	CLIA	Shenzhen YHLO	0.96 [0.81, 1.00]	Not estimable
Xiao 2020a	2	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.16, 1.00]	Not estimable
Lippi 2020 [A]	12	0	6	0	CLIA	Snibe Diagnostic - MAGLUMI	0.67 [0.41, 0.87]	Not estimable
Padoan 2020	28	0	7	0	CLIA	Snibe Diagnostic - MAGLUMI	0.80 [0.63, 0.92]	Not estimable
Gao 2020b [C]	8	0	5	0	ELISA	Beijing Beier Bioengineering	0.62 [0.32, 0.86]	Not estimable
Liu 2020d [B]	60	0	32	0	ELISA	Beijing Hotgen	0.65 [0.55, 0.75]	Not estimable
Lou 2020 [A]	57	0	18	0	ELISA	Beijing Wantai	0.76 [0.65, 0.85]	Not estimable
Zhao 2020a	73	0	62	0	ELISA	Beijing Wantai	0.54 [0.45, 0.63]	Not estimable
Lassauniere 2020 [B]	6	0	1	0	ELISA	EUROIMMUN	0.86 [0.42, 1.00]	Not estimable
Lippi 2020 [B]	7	0	11	0	ELISA	EUROIMMUN	0.39 [0.17, 0.64]	Not estimable
Okba 2020a	3	0	7	0	ELISA	EUROIMMUN Beta	0.30 [0.07, 0.65]	Not estimable
Adams 2020 [A]	11	0	2	0	ELISA	In-house	0.85 [0.55, 0.98]	Not estimable
Liu 2020b	62	0	48	0	ELISA	Zhuhai Livzon	0.56 [0.47, 0.66]	Not estimable
Liu 2020d [A]	54	0	38	0	ELISA	Zhuhai Livzon	0.59 [0.48, 0.69]	Not estimable
Xiang 2020b	47	0	39	0	ELISA	Zhuhai Livzon	0.55 [0.44, 0.65]	Not estimable
Wan 2020 [A]	3	0	2	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.60 [0.15, 0.95]	Not estimable
Adams 2020 [D]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [E]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [F]	9	0	4	0	LFA (no details)	Withheld	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [G]	8	0	5	0	LFA (no details)	Withheld	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [H]	9	0	4	0	LFA (no details)	Withheld	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [I]	8	0	5	0	LFA (no details)	Withheld	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [J]	6	0	7	0	LFA (no details)	Withheld	0.46 [0.19, 0.75]	Not estimable

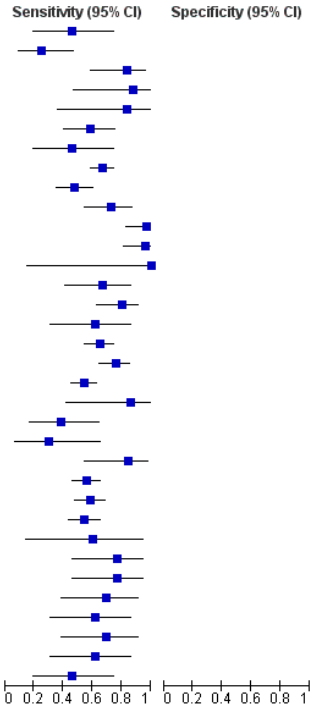

IgG (15 to 21 days)


Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	11	0	3	0	CGIA	Beijing Beier Bioengineering	0.79 [0.49, 0.95]	Not estimable
Garcia 2020 (A)	16	0	7	0	CGIA	Hangzhou Alltest - IgG/IgM	0.70 [0.47, 0.87]	Not estimable
Garcia 2020 (B)	41	0	4	0	CGIA	Hangzhou Alltest - IgG/IgM	0.91 [0.79, 0.98]	Not estimable
Gao 2020a	21	0	2	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.91 [0.72, 0.99]	Not estimable
Liu 2020a	68	0	0	0	CGIA	Withheld	1.00 [0.95, 1.00]	Not estimable
Pan 2020a	35	0	3	0	CGIA	Zhuhai Livzon	0.92 [0.79, 0.98]	Not estimable



Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.


Figure 4. (Continued)

Gao 2020a	21	0	2	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.91 [0.72, 0.99]	Not estimable
Liu 2020a	68	0	0	0	CGIA	Withheld	1.00 [0.95, 1.00]	Not estimable
Pan 2020a	35	0	3	0	CGIA	Zhuhai Livzon	0.92 [0.79, 0.98]	Not estimable
Gao 2020b [A]	9	0	5	0	CLIA	Beijing Beier Bioengineering	0.64 [0.35, 0.87]	Not estimable
Hu 2020a	81	0	29	0	CLIA	Bioscience Co (Chongqing)	0.74 [0.64, 0.82]	Not estimable
Long 2020 (B)	127	0	7	0	CLIA	Bioscience Co (Chongqing)	0.95 [0.90, 0.98]	Not estimable
Lin 2020a [A]	33	0	1	0	CLIA	In-house	0.97 [0.85, 1.00]	Not estimable
Ma 2020a	55	0	0	0	CLIA	In-house	1.00 [0.94, 1.00]	Not estimable
Jin 2020	21	0	1	0	CLIA	Shenzhen YHLO	0.95 [0.77, 1.00]	Not estimable
Xiao 2020a	4	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.40, 1.00]	Not estimable
Padoan 2020	25	0	0	0	CLIA	Snibe Diagnostic - MAGLUMI	1.00 [0.86, 1.00]	Not estimable
Gao 2020b [C]	12	0	2	0	ELISA	Beijing Beier Bioengineering	0.86 [0.57, 0.98]	Not estimable
Liu 2020d [B]	51	0	4	0	ELISA	Beijing Hotgen	0.93 [0.82, 0.98]	Not estimable
Lou 2020 [A]	56	0	4	0	ELISA	Beijing Wantai	0.93 [0.84, 0.98]	Not estimable
Zhao 2020a	71	0	18	0	ELISA	Beijing Wantai	0.80 [0.70, 0.88]	Not estimable
Lassauniere 2020 [B]	14	0	1	0	ELISA	EUROIMMUN	0.93 [0.68, 1.00]	Not estimable
Okba 2020a	7	0	1	0	ELISA	EUROIMMUN Beta	0.88 [0.47, 1.00]	Not estimable
Adams 2020 [A]	4	0	0	0	ELISA	In-house	1.00 [0.40, 1.00]	Not estimable
Liu 2020b	102	0	9	0	ELISA	Zhuhai Livzon	0.92 [0.85, 0.96]	Not estimable
Liu 2020d [A]	48	0	7	0	ELISA	Zhuhai Livzon	0.87 [0.76, 0.95]	Not estimable
Xiang 2020b	47	0	10	0	ELISA	Zhuhai Livzon	0.82 [0.70, 0.91]	Not estimable
Wan 2020 [A]	3	0	0	0	IIFT	EUROIMMUN Anti-SARS-Cov	1.00 [0.29, 1.00]	Not estimable
Adams 2020 [D]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [E]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [F]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [G]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [H]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [I]	2	0	2	0	LFA (no details)	Withheld	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [J]	2	0	2	0	LFA (no details)	Withheld	0.50 [0.07, 0.93]	Not estimable

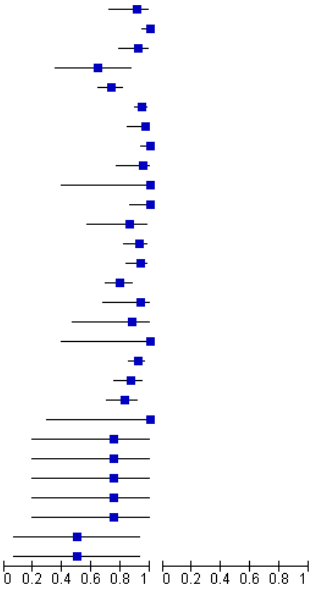


IgG (22 to 35 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Hu 2020a	85	0	66	0	CLIA	Bioscience Co (Chongqing)	0.56 [0.48, 0.64]	Not estimable
Long 2020 (B)	13	0	0	0	CLIA	Bioscience Co (Chongqing)	1.00 [0.75, 1.00]	Not estimable
Ma 2020a	91	0	0	0	CLIA	In-house	1.00 [0.96, 1.00]	Not estimable
Jin 2020	45	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.92, 1.00]	Not estimable
Xiao 2020a	19	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.82, 1.00]	Not estimable
Du 2020	7	0	0	0	CLIA	Withheld	1.00 [0.59, 1.00]	Not estimable
Liu 2020d [B]	39	0	6	0	ELISA	Beijing Hotgen	0.87 [0.73, 0.95]	Not estimable
Lassauniere 2020 [B]	8	0	0	0	ELISA	EUROIMMUN	1.00 [0.63, 1.00]	Not estimable
Okba 2020a	1	0	0	0	ELISA	EUROIMMUN Beta	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [A]	2	0	0	0	ELISA	In-house	1.00 [0.16, 1.00]	Not estimable
Liu 2020d [A]	41	0	4	0	ELISA	Zhuhai Livzon	0.91 [0.79, 0.98]	Not estimable
Xiang 2020b	50	0	9	0	ELISA	Zhuhai Livzon	0.85 [0.73, 0.93]	Not estimable
Wan 2020 [A]	1	0	0	0	IIFT	EUROIMMUN Anti-SARS-Cov	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [D]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [E]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [F]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	2	0	0	0	LFA (no details)	Withheld	1.00 [0.16, 1.00]	Not estimable

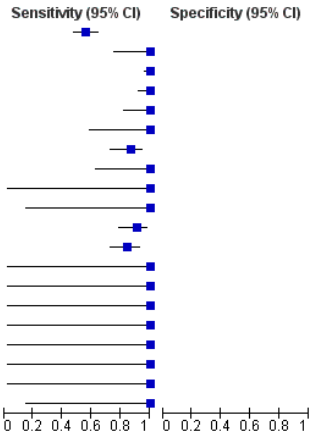

IgG (over 35 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Hu 2020a	75	0	1	0	CLIA	Bioscience Co (Chongqing)	0.99 [0.93, 1.00]	Not estimable
Ma 2020a	23	0	0	0	CLIA	In-house	1.00 [0.85, 1.00]	Not estimable
Xiao 2020a	7	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.59, 1.00]	Not estimable
Du 2020	53	0	0	0	CLIA	Withheld	1.00 [0.93, 1.00]	Not estimable
Adams 2020 [A]	17	0	0	0	ELISA	In-house	1.00 [0.80, 1.00]	Not estimable
Adams 2020 [D]	7	0	4	0	LFA (no details)	Withheld	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [E]	11	0	5	0	LFA (no details)	Withheld	0.69 [0.41, 0.89]	Not estimable
Adams 2020 [F]	5	0	4	0	LFA (no details)	Withheld	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [G]	4	0	5	0	LFA (no details)	Withheld	0.44 [0.14, 0.79]	Not estimable
Adams 2020 [H]	7	0	4	0	LFA (no details)	Withheld	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [I]	4	0	6	0	LFA (no details)	Withheld	0.40 [0.12, 0.74]	Not estimable
Adams 2020 [J]	7	0	10	0	LFA (no details)	Withheld	0.41 [0.18, 0.67]	Not estimable

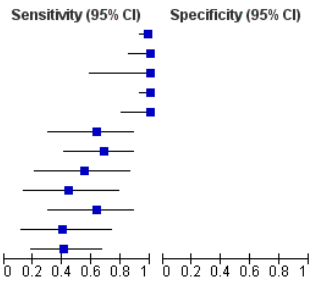


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 5. Forest plot of studies evaluating tests for detection of IgM according to week post-symptom onset and type of test


IgM (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	5	0	5	0	CGIA	Beijing Beier Bioengineering	0.50 [0.19, 0.81]	Not estimable
Wang 2020a [B]	14	0	0	0	CGIA	Beijing Hotgen	1.00 [0.77, 1.00]	Not estimable
Garcia 2020 (A)	0	0	8	0	CGIA	Hangzhou Alltest - IgG/IgM	0.00 [0.00, 0.37]	Not estimable
Gao 2020a	3	0	10	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.23 [0.05, 0.54]	Not estimable
Liu 2020a	3	0	13	0	CGIA	Withheld	0.19 [0.04, 0.46]	Not estimable
Pan 2020a	5	0	31	0	CGIA	Zhuhai Livzon	0.14 [0.05, 0.29]	Not estimable
Gao 2020b [A]	4	0	6	0	CLIA	Beijing Beier Bioengineering	0.40 [0.12, 0.74]	Not estimable
Hu 2020a	7	0	14	0	CLIA	Bioscience Co (Chongqing)	0.33 [0.15, 0.57]	Not estimable
Long 2020 (B)	21	0	46	0	CLIA	Bioscience Co (Chongqing)	0.31 [0.21, 0.44]	Not estimable
Lin 2020a [A]	10	0	2	0	CLIA	In-house	0.83 [0.52, 0.98]	Not estimable
Ma 2020a	11	0	6	0	CLIA	In-house	0.65 [0.38, 0.86]	Not estimable
Jin 2020	1	0	5	0	CLIA	Shenzhen YHLO	0.17 [0.00, 0.64]	Not estimable
Xiao 2020a	0	0	2	0	CLIA	Shenzhen YHLO	0.00 [0.00, 0.84]	Not estimable
Lippi 2020 [A]	1	0	29	0	CLIA	Snibe Diagnostic - MAGLUMI	0.03 [0.00, 0.17]	Not estimable
Padoan 2020	3	0	7	0	CLIA	Snibe Diagnostic - MAGLUMI	0.30 [0.07, 0.65]	Not estimable
Gao 2020b [C]	4	0	6	0	ELISA	Beijing Beier Bioengineering	0.40 [0.12, 0.74]	Not estimable
Liu 2020d [B]	8	0	14	0	ELISA	Beijing Hotgen	0.36 [0.17, 0.59]	Not estimable
Wang 2020a [A]	14	0	0	50	ELISA	Beijing Hotgen	1.00 [0.77, 1.00]	1.00 [0.93, 1.00]
Lou 2020 [A]	13	0	26	0	ELISA	Beijing Wantai	0.33 [0.19, 0.50]	Not estimable
Zhao 2020a	27	0	67	0	ELISA	Beijing Wantai	0.29 [0.20, 0.39]	Not estimable
Adams 2020 [A]	0	0	4	0	ELISA	In-house	0.00 [0.00, 0.60]	Not estimable
Guo 2020a	35	0	6	0	ELISA	In-house	0.85 [0.71, 0.94]	Not estimable
Liu 2020b	3	0	14	0	ELISA	Zhuhai Livzon	0.18 [0.04, 0.43]	Not estimable
Liu 2020d [A]	7	0	15	0	ELISA	Zhuhai Livzon	0.32 [0.14, 0.55]	Not estimable
Xiang 2020b	7	0	7	0	ELISA	Zhuhai Livzon	0.50 [0.23, 0.77]	Not estimable
Zeng 2020a	0	0	27	0	ELISA	Zhuhai Livzon	0.00 [0.00, 0.13]	Not estimable
Wan 2020 [A]	0	0	4	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [D]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [H]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [J]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable



IgM (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	5	0	8	0	CGIA	Beijing Beier Bioengineering	0.38 [0.14, 0.68]	Not estimable
Garcia 2020 (A)	3	0	21	0	CGIA	Hangzhou Alltest - IgG/IgM	0.13 [0.03, 0.32]	Not estimable
Garcia 2020 (B)	7	0	11	0	CGIA	Hangzhou Alltest - IgG/IgM	0.39 [0.17, 0.64]	Not estimable
Gao 2020a	4	0	4	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.50 [0.16, 0.84]	Not estimable
Liu 2020a	6	0	0	0	CGIA	Withheld	1.00 [0.54, 1.00]	Not estimable
Pan 2020a	24	0	10	0	CGIA	Zhuhai Livzon	0.71 [0.53, 0.85]	Not estimable
Gao 2020b [A]	4	0	9	0	CLIA	Beijing Beier Bioengineering	0.31 [0.09, 0.61]	Not estimable
Hu 2020a	78	0	48	0	CLIA	Bioscience Co (Chongqing)	0.62 [0.53, 0.70]	Not estimable
Long 2020 (B)	21	0	46	0	CLIA	Bioscience Co (Chongqing)	0.31 [0.21, 0.44]	Not estimable
Lin 2020a [A]	24	0	9	0	CLIA	In-house	0.73 [0.54, 0.87]	Not estimable
Ma 2020a	30	0	0	0	CLIA	In-house	1.00 [0.88, 1.00]	Not estimable
Jin 2020	12	0	15	0	CLIA	Shenzhen YHLO	0.44 [0.25, 0.65]	Not estimable
Xiao 2020a	2	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.16, 1.00]	Not estimable
Lippi 2020 [A]	5	0	13	0	CLIA	Snibe Diagnostic - MAGLUMI	0.28 [0.10, 0.53]	Not estimable
Padoan 2020	19	0	16	0	CLIA	Snibe Diagnostic - MAGLUMI	0.54 [0.37, 0.71]	Not estimable
Gao 2020b [C]	1	0	12	0	ELISA	Beijing Beier Bioengineering	0.08 [0.00, 0.36]	Not estimable
Liu 2020d [B]	64	0	28	0	ELISA	Beijing Hotgen	0.70 [0.59, 0.79]	Not estimable
Lou 2020 [A]	65	0	10	0	ELISA	Beijing Wantai	0.87 [0.77, 0.93]	Not estimable
Zhao 2020a	99	0	36	0	ELISA	Beijing Wantai	0.73 [0.65, 0.81]	Not estimable
Adams 2020 [A]	11	0	2	0	ELISA	In-house	0.85 [0.55, 0.98]	Not estimable
Liu 2020b	72	0	38	0	ELISA	Zhuhai Livzon	0.65 [0.56, 0.74]	Not estimable
Liu 2020d [A]	59	0	33	0	ELISA	Zhuhai Livzon	0.64 [0.53, 0.74]	Not estimable
Xiang 2020b	57	0	29	0	ELISA	Zhuhai Livzon	0.66 [0.55, 0.76]	Not estimable
Wan 2020 [A]	1	0	4	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.20 [0.01, 0.72]	Not estimable
Adams 2020 [D]	2	0	11	0	LFA (no details)	Withheld	0.15 [0.02, 0.45]	Not estimable
Adams 2020 [E]	1	0	12	0	LFA (no details)	Withheld	0.08 [0.00, 0.36]	Not estimable
Adams 2020 [F]	7	0	6	0	LFA (no details)	Withheld	0.54 [0.25, 0.81]	Not estimable
Adams 2020 [G]	7	0	6	0	LFA (no details)	Withheld	0.54 [0.25, 0.81]	Not estimable
Adams 2020 [H]	8	0	5	0	LFA (no details)	Withheld	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [I]	8	0	5	0	LFA (no details)	Withheld	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [J]	7	0	6	0	LFA (no details)	Withheld	0.54 [0.25, 0.81]	Not estimable




IgM (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020b [B]	9	0	5	0	CGIA	Beijing Beier Bioengineering	0.64 [0.35, 0.87]	Not estimable
Garcia 2020 (A)	9	0	14	0	CGIA	Hangzhou Alltest - IgG/IgM	0.39 [0.20, 0.61]	Not estimable
Garcia 2020 (B)	18	0	27	0	CGIA	Hangzhou Alltest - IgG/IgM	0.40 [0.26, 0.56]	Not estimable
Gao 2020a	12	0	11	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.52 [0.31, 0.73]	Not estimable
Liu 2020a	25	0	43	0	CGIA	Withheld	0.37 [0.25, 0.49]	Not estimable
Pan 2020a	27	0	11	0	CGIA	Zhuhai Livzon	0.71 [0.54, 0.86]	Not estimable

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.


Figure 5. (Continued)

Gao 2020a	12	0	11	0	CGIA	Innovita Biological - Ab test (IgM/IgG)	0.52 [0.31, 0.73]	Not estimable	
Liu 2020a	25	0	43	0	CGIA	Withheld	0.37 [0.25, 0.49]	Not estimable	
Pan 2020a	27	0	11	0	CGIA	Zhuhai Livzon	0.71 [0.54, 0.85]	Not estimable	
Gao 2020b [A]	6	0	8	0	CLIA	Beijing Beier Bioengineering	0.43 [0.18, 0.71]	Not estimable	
Hu 2020a	54	0	29	0	CLIA	Bioscience Co (Chongqing)	0.65 [0.54, 0.75]	Not estimable	
Long 2020 (B)	113	0	21	0	CLIA	Bioscience Co (Chongqing)	0.84 [0.77, 0.90]	Not estimable	
Lin 2020a [A]	31	0	3	0	CLIA	In-house	0.91 [0.76, 0.98]	Not estimable	
Ma 2020a	55	0	0	0	CLIA	In-house	1.00 [0.94, 1.00]	Not estimable	
Jin 2020	16	0	6	0	CLIA	Shenzhen YHLO	0.73 [0.50, 0.89]	Not estimable	
Xiao 2020a	4	0	0	0	CLIA	Shenzhen YHLO	1.00 [0.40, 1.00]	Not estimable	
Padoan 2020	22	0	3	0	CLIA	Snibe Diagnostic - MAGLUMI	0.88 [0.69, 0.97]	Not estimable	
Gao 2020b [C]	6	0	8	0	ELISA	Beijing Beier Bioengineering	0.43 [0.18, 0.71]	Not estimable	
Liu 2020d [B]	53	0	2	0	ELISA	Beijing Hotgen	0.96 [0.87, 1.00]	Not estimable	
Lou 2020 [A]	58	0	2	0	ELISA	Beijing Wantai	0.97 [0.88, 1.00]	Not estimable	
Zhao 2020a	83	0	5	0	ELISA	Beijing Wantai	0.94 [0.87, 0.98]	Not estimable	
Adams 2020 [A]	4	0	0	0	ELISA	In-house	1.00 [0.40, 1.00]	Not estimable	
Liu 2020b	92	0	19	0	ELISA	Zhuhai Livzon	0.83 [0.75, 0.89]	Not estimable	
Liu 2020d [A]	45	0	10	0	ELISA	Zhuhai Livzon	0.82 [0.69, 0.91]	Not estimable	
Xiang 2020b	45	0	12	0	ELISA	Zhuhai Livzon	0.79 [0.66, 0.89]	Not estimable	
Wan 2020 [A]	2	0	1	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.67 [0.09, 0.99]	Not estimable	
Adams 2020 [D]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable	
Adams 2020 [E]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable	
Adams 2020 [F]	2	0	2	0	LFA (no details)	Withheld	0.50 [0.07, 0.93]	Not estimable	
Adams 2020 [G]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable	
Adams 2020 [H]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable	
Adams 2020 [I]	2	0	2	0	LFA (no details)	Withheld	0.50 [0.07, 0.93]	Not estimable	
Adams 2020 [J]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable	

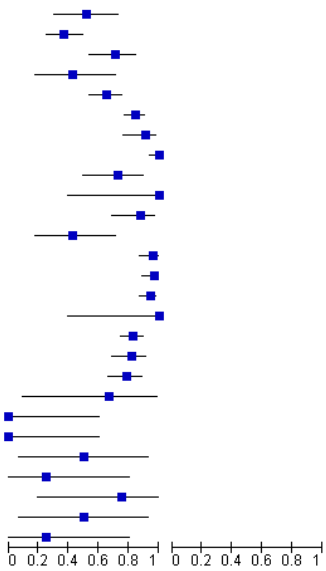


IgM (22 to 35 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Hu 2020a	85	0	66	0	CLIA	Bioscience Co (Chongqing)	0.56 [0.48, 0.64]	Not estimable
Long 2020 (B)	12	0	1	0	CLIA	Bioscience Co (Chongqing)	0.92 [0.64, 1.00]	Not estimable
Ma 2020a	91	0	0	0	CLIA	In-house	1.00 [0.96, 1.00]	Not estimable
Jin 2020	29	0	16	0	CLIA	Shenzhen YHLO	0.64 [0.49, 0.78]	Not estimable
Xiao 2020a	17	0	2	0	CLIA	Shenzhen YHLO	0.89 [0.67, 0.99]	Not estimable
Du 2020	7	0	0	0	CLIA	Withheld	1.00 [0.59, 1.00]	Not estimable
Liu 2020d [B]	40	0	5	0	ELISA	Beijing Hotgen	0.89 [0.76, 0.96]	Not estimable
Adams 2020 [A]	2	0	6	0	ELISA	In-house	0.25 [0.03, 0.65]	Not estimable
Liu 2020d [A]	35	0	10	0	ELISA	Zhuhai Livzon	0.78 [0.63, 0.89]	Not estimable
Xiang 2020b	43	0	16	0	ELISA	Zhuhai Livzon	0.73 [0.60, 0.84]	Not estimable
Wan 2020 [A]	0	0	1	0	IIFT	EUROIMMUN Anti-SARS-Cov	0.00 [0.00, 0.97]	Not estimable
Adams 2020 [D]	0	0	1	0	LFA (no details)	Withheld	0.00 [0.00, 0.97]	Not estimable
Adams 2020 [E]	0	0	1	0	LFA (no details)	Withheld	0.00 [0.00, 0.97]	Not estimable
Adams 2020 [F]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	1	0	1	0	LFA (no details)	Withheld	0.50 [0.01, 0.99]	Not estimable

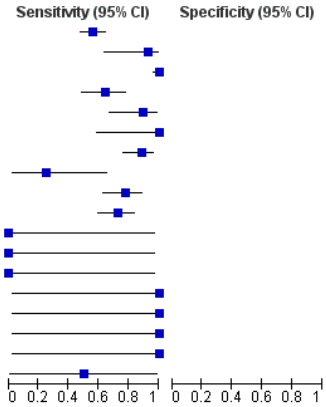

IgM (over 35 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Hu 2020a	24	0	25	0	CLIA	Bioscience Co (Chongqing)	0.49 [0.34, 0.64]	Not estimable
Ma 2020a	20	0	3	0	CLIA	In-house	0.87 [0.66, 0.97]	Not estimable
Xiao 2020a	5	0	2	0	CLIA	Shenzhen YHLO	0.71 [0.29, 0.96]	Not estimable
Du 2020	40	0	13	0	CLIA	Withheld	0.75 [0.62, 0.86]	Not estimable
Adams 2020 [A]	11	0	6	0	ELISA	In-house	0.65 [0.38, 0.86]	Not estimable
Adams 2020 [D]	1	0	10	0	LFA (no details)	Withheld	0.09 [0.00, 0.41]	Not estimable
Adams 2020 [E]	1	0	15	0	LFA (no details)	Withheld	0.06 [0.00, 0.30]	Not estimable
Adams 2020 [F]	5	0	4	0	LFA (no details)	Withheld	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [G]	5	0	4	0	LFA (no details)	Withheld	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [H]	5	0	6	0	LFA (no details)	Withheld	0.45 [0.17, 0.77]	Not estimable
Adams 2020 [I]	0	0	0	0	LFA (no details)	Withheld	Not estimable	Not estimable
Adams 2020 [J]	6	0	11	0	LFA (no details)	Withheld	0.35 [0.14, 0.62]	Not estimable

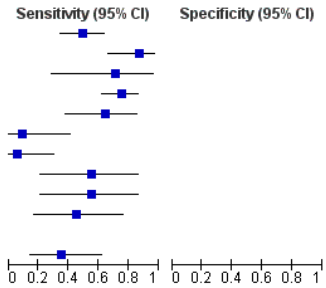


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 6. Forest plot of studies evaluating tests for detection of IgG/IgM according to week post-symptom onset and type of test


IgG/IgM (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (A)	1	0	7	0	CGIA	Hangzhou Alltest - IgG/IgM	0.13 [0.00, 0.53]	Not estimable
Liu 2020a	3	0	13	0	CGIA	Withheld	0.19 [0.04, 0.46]	Not estimable
Pan 2020a	7	0	29	0	CGIA	Zhuhai Livzon	0.19 [0.08, 0.36]	Not estimable
Long 2020 (B)	34	0	33	0	CLIA	Bioscience Co (Chongqing)	0.51 [0.38, 0.63]	Not estimable
Lin 2020a [A]	10	0	2	0	CLIA	In-house	0.83 [0.52, 0.98]	Not estimable
Liu 2020d [B]	10	0	12	0	ELISA	Beijing Hotgen	0.45 [0.24, 0.68]	Not estimable
Adams 2020 [A]	0	0	4	0	ELISA	In-house	0.00 [0.00, 0.60]	Not estimable
Liu 2020b	5	0	12	0	ELISA	Zhuhai Livzon	0.29 [0.10, 0.56]	Not estimable
Liu 2020d [A]	9	0	13	0	ELISA	Zhuhai Livzon	0.41 [0.21, 0.64]	Not estimable
Zeng 2020a	0	0	27	0	ELISA	Zhuhai Livzon	0.00 [0.00, 0.13]	Not estimable
Adams 2020 [D]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [H]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	1	0	3	0	LFA (no details)	Withheld	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [J]	0	0	4	0	LFA (no details)	Withheld	0.00 [0.00, 0.60]	Not estimable

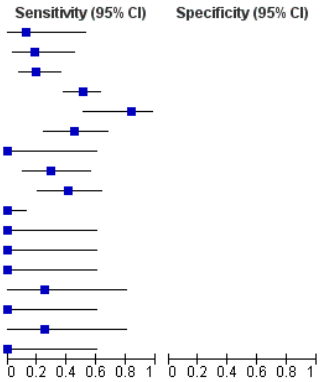


IgG/IgM (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [G]	5	0	2	0	CGIA	Artron Laboratories IgM/IgG	0.71 [0.29, 0.96]	Not estimable
Lassauniere 2020 [F]	6	0	1	0	CGIA	Autobio Diagnostics IgM/IgG	0.86 [0.42, 1.00]	Not estimable
Lassauniere 2020 [E]	5	0	2	0	CGIA	CTK Biotech OnSite IgG/IgM	0.71 [0.29, 0.96]	Not estimable
Lassauniere 2020 [D]	5	0	2	0	CGIA	Dynamiker Biotechnology IgG/IgM	0.71 [0.29, 0.96]	Not estimable
Garcia 2020 (A)	8	0	16	0	CGIA	Hangzhou Alltest - IgG/IgM	0.33 [0.16, 0.55]	Not estimable
Garcia 2020 (B)	15	0	3	0	CGIA	Hangzhou Alltest - IgG/IgM	0.83 [0.59, 0.96]	Not estimable
Liu 2020a	6	0	0	0	CGIA	Withheld	1.00 [0.54, 1.00]	Not estimable
Pan 2020a	31	0	3	0	CGIA	Zhuhai Livzon	0.91 [0.76, 0.98]	Not estimable
Long 2020 (B)	34	0	33	0	CLIA	Bioscience Co (Chongqing)	0.51 [0.38, 0.63]	Not estimable
Lin 2020a [A]	29	0	4	0	CLIA	In-house	0.88 [0.72, 0.97]	Not estimable
Liu 2020d [B]	72	0	20	0	ELISA	Beijing Hotgen	0.78 [0.68, 0.86]	Not estimable
Adams 2020 [A]	11	0	2	0	ELISA	In-house	0.85 [0.55, 0.98]	Not estimable
Liu 2020b	82	0	28	0	ELISA	Zhuhai Livzon	0.75 [0.65, 0.82]	Not estimable
Liu 2020d [A]	68	0	24	0	ELISA	Zhuhai Livzon	0.74 [0.64, 0.83]	Not estimable
Adams 2020 [D]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [E]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [F]	9	0	4	0	LFA (no details)	Withheld	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [G]	8	0	5	0	LFA (no details)	Withheld	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [H]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [I]	10	0	3	0	LFA (no details)	Withheld	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [J]	7	0	6	0	LFA (no details)	Withheld	0.54 [0.25, 0.81]	Not estimable

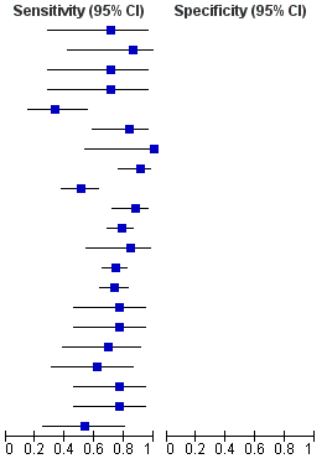


IgG/IgM (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [G]	12	0	3	0	CGIA	Artron Laboratories IgM/IgG	0.80 [0.52, 0.96]	Not estimable
Lassauniere 2020 [F]	14	0	1	0	CGIA	Autobio Diagnostics IgM/IgG	0.93 [0.68, 1.00]	Not estimable
Lassauniere 2020 [E]	14	0	1	0	CGIA	CTK Biotech OnSite IgG/IgM	0.93 [0.68, 1.00]	Not estimable
Lassauniere 2020 [D]	14	0	1	0	CGIA	Dynamiker Biotechnology IgG/IgM	0.93 [0.68, 1.00]	Not estimable
Garcia 2020 (A)	17	0	6	0	CGIA	Hangzhou Alltest - IgG/IgM	0.74 [0.52, 0.90]	Not estimable
Garcia 2020 (B)	41	0	4	0	CGIA	Hangzhou Alltest - IgG/IgM	0.91 [0.79, 0.98]	Not estimable
Liu 2020a	68	0	0	0	CGIA	Withheld	1.00 [0.95, 1.00]	Not estimable
Pan 2020a	35	0	3	0	CGIA	Zhuhai Livzon	0.92 [0.79, 0.98]	Not estimable
Long 2020 (B)	131	0	3	0	CLIA	Bioscience Co (Chongqing)	0.98 [0.94, 1.00]	Not estimable
Lin 2020a [A]	33	0	1	0	CLIA	In-house	0.97 [0.85, 1.00]	Not estimable
Liu 2020d [B]	72	0	20	0	ELISA	Beijing Hotgen	0.78 [0.68, 0.86]	Not estimable
Adams 2020 [A]	4	0	0	0	ELISA	In-house	1.00 [0.40, 1.00]	Not estimable
Liu 2020b	107	0	4	0	ELISA	Zhuhai Livzon	0.96 [0.91, 0.99]	Not estimable
Liu 2020d [A]	52	0	3	0	ELISA	Zhuhai Livzon	0.95 [0.85, 0.99]	Not estimable
Adams 2020 [D]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [E]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [F]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [G]	4	0	0	0	LFA (no details)	Withheld	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [H]	4	0	0	0	LFA (no details)	Withheld	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [I]	2	0	2	0	LFA (no details)	Withheld	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [J]	3	0	1	0	LFA (no details)	Withheld	0.75 [0.19, 0.99]	Not estimable

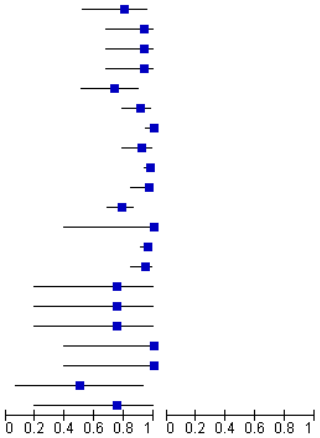

IgG/IgM (22 to 35 days)


Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [G]	8	0	0	0	CGIA	Artron Laboratories IgM/IgG	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [F]	8	0	0	0	CGIA	Autobio Diagnostics IgM/IgG	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [E]	8	0	0	0	CGIA	CTK Biotech OnSite IgG/IgM	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [D]	8	0	0	0	CGIA	Dynamiker Biotechnology IgG/IgM	1.00 [0.63, 1.00]	Not estimable
Long 2020 (B)	13	0	0	0	CLIA	Bioscience Co (Chongqing)	1.00 [0.75, 1.00]	Not estimable
Du 2020	7	0	0	0	CLIA	Withheld	1.00 [0.59, 1.00]	Not estimable
Liu 2020d [B]	41	0	4	0	ELISA	Beijing Hotgen	0.91 [0.79, 0.98]	Not estimable
Adams 2020 [A]	2	0	0	0	ELISA	In-house	1.00 [0.16, 1.00]	Not estimable
Liu 2020d [A]	43	0	2	0	ELISA	Zhuhai Livzon	0.96 [0.85, 0.99]	Not estimable

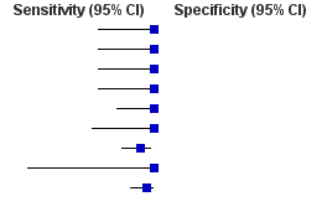

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.


Figure 6. (Continued)

Liu 2020d [B]	41	0	4	0	ELISA	Beijing Hotgen	0.91 [0.79, 0.98]	Not estimable
Adams 2020 [A]	2	0	0	0	ELISA	In-house	1.00 [0.16, 1.00]	Not estimable
Liu 2020d [A]	43	0	2	0	ELISA	Zhuhai Livzon	0.96 [0.85, 0.99]	Not estimable
Adams 2020 [D]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [E]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [F]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	LFA (no details)	Withheld	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	2	0	0	0	LFA (no details)	Withheld	1.00 [0.16, 1.00]	Not estimable

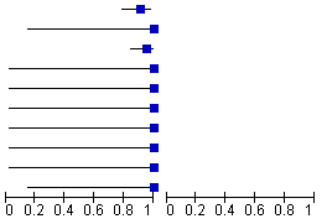

IgG/IgM (over 35 days)

Study	TP	FP	FN	TN	Test method	Test name	Sensitivity (95% CI)	Specificity (95% CI)
Du 2020	53	0	0	0	CLIA	Withheld	1.00 [0.93, 1.00]	Not estimable
Adams 2020 [A]	17	0	0	0	ELISA	In-house	1.00 [0.80, 1.00]	Not estimable
Adams 2020 [D]	7	0	4	0	LFA (no details)	Withheld	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [E]	11	0	5	0	LFA (no details)	Withheld	0.69 [0.41, 0.89]	Not estimable
Adams 2020 [F]	6	0	3	0	LFA (no details)	Withheld	0.67 [0.30, 0.93]	Not estimable
Adams 2020 [G]	6	0	3	0	LFA (no details)	Withheld	0.67 [0.30, 0.93]	Not estimable
Adams 2020 [H]	8	0	3	0	LFA (no details)	Withheld	0.73 [0.39, 0.94]	Not estimable
Adams 2020 [I]	4	0	6	0	LFA (no details)	Withheld	0.40 [0.12, 0.74]	Not estimable
Adams 2020 [J]	10	0	7	0	LFA (no details)	Withheld	0.59 [0.33, 0.82]	Not estimable

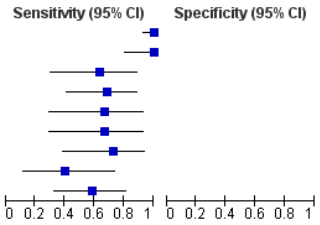

The numbers of individuals contributing data within each study within each week are very small, thus by pooling these data across studies these meta-analyses contribute clarity to the relationship between sensitivity and time, although the important limitations of these studies as described above should be considered when interpreting all findings.

Pooled results for IgG, IgM, IgA, total antibodies and IgG/IgM all show the same general pattern over the first three weeks, with sensitivity being low when tests were used in the first week since onset of symptoms, rising in the second week, and reaching their highest values in the third week. For IgG, sensitivity across the three weeks were 29.7% (95% confidence interval (CI) 22.1 to 38.6), 66.5% (95% CI 57.9 to 74.2) and 88.2% (95% CI 83.5 to 91.8); for IgM they were 23.2% (95% CI 14.9 to 34.2), 58.4% (95% CI 45.5 to 70.3) and 75.4% (95% CI 64.3 to 83.8); and for IgG/IgM they were 30.1% (95% CI 21.4 to 40.7), 72.2% (95% CI 63.5 to 79.5) and 91.4% (95% CI 87.0 to 94.4). Values for total antibodies and IgA are also given in Table 2.

It is important to note that these estimates are based on pooling multiple cross-sectional studies, and are not based on tracking the same groups of participants over time or even using the same tests. The reasons why individuals are included at some particular time points and not at others is mostly not reported.

Estimates of sensitivity beyond three weeks are based on smaller sample sizes, with a maximum of 12 studies contributing data in weeks 4 and 5, and only four studies providing any follow-up information beyond week 5. Estimates for IgA and total antibodies are based on fewer than 100 samples/participants and we will not comment upon them further. In weeks 4 and 5, pooled sensitivities of IgG were 80.3% (95% CI 72.4 to 86.4); IgM were 68.1% (95% CI 55.0 to 78.9); and for IgG/IgM were 96.0% (95% CI 90.6 to 98.3).

The data beyond week 5 gave sensitivity estimates of 86.7% (95% CI 79.6 to 91.7; IgG), 53.9% (95% CI 38.4 to 68.6; IgM) and 77.7% (95% CI 66.0 to 86.2; IgG/IgM). The expected decline in the sensitivity of IgM is evident.

Overall specificity

We estimated antibody test specificity from 35 studies. Specificity estimates for all studies are presented in Appendix 11 for IgG, IgM, IgG/IgM, IgA, total antibodies, and IgA/IgG. Results pooled across all studies are in Table 3 and show specificity exceeding 98% for all antibody types, with precise estimates (confidence intervals up to 2 percentage points wide), particularly for IgG, IgM, total antibodies and IgG/IgM, where estimates are based on several thousand non-COVID samples. Inspection of the figures shows low heterogeneity in study estimates of specificity across studies. Nine studies provided some information on the cross-reactivity of other infections, including other coronaviruses, with the SARS-CoV-2 antigens used in the assays (Table 4).

Impact of reference standard for COVID-19 cases on sensitivity

The majority of studies only included participants who were diagnosed with COVID-19 based upon observing a positive RT-PCR test. However, in clinical practice it is common to encounter patients from whom positive RT-PCR results are never obtained, but who demonstrate clinical and imaging features of COVID-19. Diagnostic criteria for COVID-19 produced by WHO and the China CDC include definitions for suspected COVID-19 in RT-PCR-negative patients. Twelve studies defined the presence of COVID-19 using these criteria, thus including RT-PCR-negative patients in the COVID-19 group as well as RT-PCR-positive patients. We compared estimates of sensitivity between studies using a RT-PCR-positive reference standard definition with a criteria-based reference standard (including both RT-PCR-positives and RT-PCR-negatives; Table 5). We stratified the analysis for weeks since onset of symptoms. All the observed differences were within magnitudes expected by chance.

In a further analysis, we separated COVID-19 participants who were RT-PCR-positive from those who were RT-PCR-negative, where studies allowed, and subgrouped the results to investigate whether there is a difference in accuracy according to RT-PCR status. Data from only three studies could be included in this analysis (Figure 7; Figure 8; Figure 9). Differences in estimates of sensitivity (pooled stratifying for weeks since onset of symptoms), varied in direction

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.


for IgG and IgM, and were very similar for IgG/IgM (Table 6). All differences were within magnitudes expected by chance. There was no consistent evidence that the accuracy of serology tests was lower in RT-PCR-positive patients, although there is high uncertainty in these findings.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 7. Sensitivity of IgG in PCR+ve and PCR-ve COVID-19 cases by week since onset of symptoms.


IgG in PCR-ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	28	0	2	0	CGIA	0.93 [0.78, 0.99]	Not estimable
Garcia 2020 (B)	56	0	7	0	CGIA	0.89 [0.78, 0.95]	Not estimable
Jia 2020	15	0	18	0	FIA	0.45 [0.28, 0.64]	Not estimable
Jin 2020	32	0	2	0	CLIA	0.94 [0.80, 0.99]	Not estimable
Qian 2020	45	0	7	0	CLIA	0.87 [0.74, 0.94]	Not estimable
Xie 2020a	40	0	0	0	CLIA	1.00 [0.91, 1.00]	Not estimable

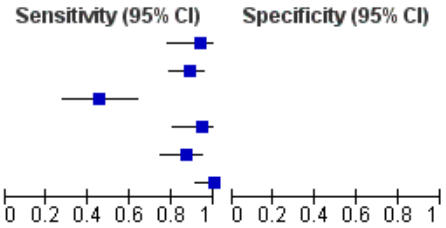


IgG in PCR+ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	14	0	1	0	CGIA	0.93 [0.68, 1.00]	Not estimable
Jia 2020	16	0	8	0	FIA	0.67 [0.45, 0.84]	Not estimable
Qian 2020	486	0	17	0	CLIA	0.97 [0.95, 0.98]	Not estimable
Xie 2020a	16	0	0	0	CLIA	1.00 [0.79, 1.00]	Not estimable

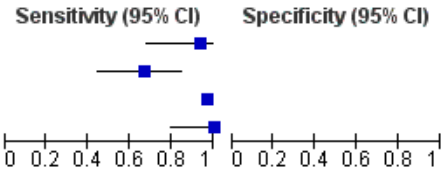


IgG in PCR +ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	0	0	1	0	CGIA	0.00 [0.00, 0.97]	Not estimable
Pan 2020a	1	0	26	0	CGIA	0.04 [0.00, 0.19]	Not estimable




IgG in PCR+ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	5	0	0	0	CGIA	1.00 [0.48, 1.00]	Not estimable
Pan 2020a	16	0	12	0	CGIA	0.57 [0.37, 0.76]	Not estimable




IgG in PCR+ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	9	0	0	0	CGIA	1.00 [0.66, 1.00]	Not estimable
Pan 2020a	30	0	1	0	CGIA	0.97 [0.83, 1.00]	Not estimable




IgG in PCR-ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	4	0	0	0	CGIA	1.00 [0.40, 1.00]	Not estimable
Pan 2020a	4	0	5	0	CGIA	0.44 [0.14, 0.79]	Not estimable




IgG in PCR-ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	6	0	0	0	CGIA	1.00 [0.54, 1.00]	Not estimable
Garcia 2020 (B)	15	0	3	0	CGIA	0.83 [0.59, 0.96]	Not estimable
Pan 2020a	4	0	2	0	CGIA	0.67 [0.22, 0.96]	Not estimable

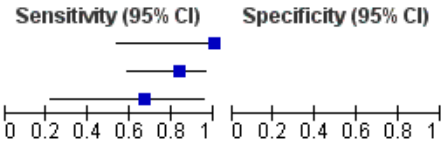

IgG in PCR-ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	18	0	2	0	CGIA	0.90 [0.68, 0.99]	Not estimable
Garcia 2020 (B)	41	0	4	0	CGIA	0.91 [0.79, 0.98]	Not estimable
Pan 2020a	5	0	2	0	CGIA	0.71 [0.29, 0.96]	Not estimable

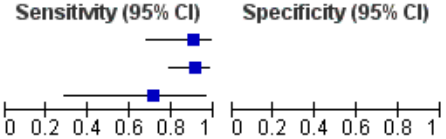


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 8. Sensitivity of IgM in PCR+ve and PCR-ve COVID-19 cases by week since onset of symptoms.


IgM in PCR+ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	7	0	8	0	CGIA	0.47 [0.21, 0.73]	Not estimable
Guo 2020a	62	0	20	0	ELISA	0.76 [0.65, 0.84]	Not estimable
Jia 2020	19	0	5	0	FIA	0.79 [0.58, 0.93]	Not estimable
Liu 2020c	74	0	17	0	CLIA	0.81 [0.72, 0.89]	Not estimable
Qian 2020	432	0	71	0	CLIA	0.86 [0.83, 0.89]	Not estimable
Xie 2020a	15	0	10	0	CLIA	0.60 [0.39, 0.79]	Not estimable

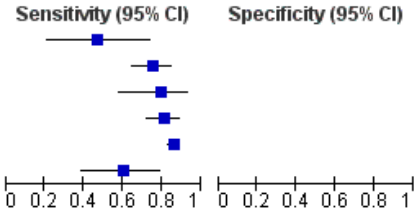


IgM in PCR-ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	13	0	17	0	CGIA	0.43 [0.25, 0.63]	Not estimable
Garcia 2020 (B)	25	0	38	0	CGIA	0.40 [0.28, 0.53]	Not estimable
Guo 2020a	54	0	4	0	ELISA	0.93 [0.83, 0.98]	Not estimable
Jia 2020	20	0	13	0	FIA	0.61 [0.42, 0.77]	Not estimable
Jin 2020	19	0	15	0	CLIA	0.56 [0.38, 0.73]	Not estimable
Liu 2020c	31	0	11	0	CLIA	0.74 [0.58, 0.86]	Not estimable
Qian 2020	38	0	14	0	CLIA	0.73 [0.59, 0.84]	Not estimable
Xie 2020a	34	0	6	0	CLIA	0.85 [0.70, 0.94]	Not estimable

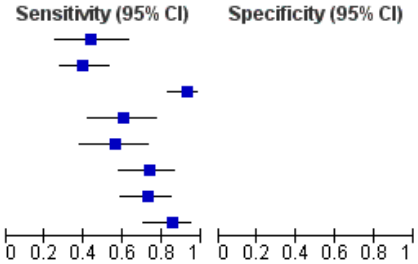


IgM in PCR+ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	0	0	1	0	CGIA	0.00 [0.00, 0.97]	Not estimable
Pan 2020a	3	0	24	0	CGIA	0.11 [0.02, 0.29]	Not estimable




IgM in PCR+ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	3	0	2	0	CGIA	0.60 [0.15, 0.95]	Not estimable
Pan 2020a	22	0	6	0	CGIA	0.79 [0.59, 0.92]	Not estimable




IgM in PCR+ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	4	0	5	0	CGIA	0.44 [0.14, 0.79]	Not estimable
Pan 2020a	4	0	3	0	CGIA	0.57 [0.18, 0.90]	Not estimable




IgM in PCR-ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	2	0	2	0	CGIA	0.50 [0.07, 0.93]	Not estimable
Pan 2020a	2	0	7	0	CGIA	0.22 [0.03, 0.60]	Not estimable



IgM in PCR-ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	2	0	4	0	CGIA	0.33 [0.04, 0.78]	Not estimable
Garcia 2020 (B)	7	0	11	0	CGIA	0.39 [0.17, 0.64]	Not estimable
Pan 2020a	2	0	4	0	CGIA	0.33 [0.04, 0.78]	Not estimable



IgM in PCR-ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	9	0	11	0	CGIA	0.45 [0.23, 0.68]	Not estimable
Garcia 2020 (B)	18	0	27	0	CGIA	0.40 [0.26, 0.56]	Not estimable
Pan 2020a	4	0	3	0	CGIA	0.57 [0.18, 0.90]	Not estimable



Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 9. Sensitivity of IgG/IgM in PCR+ve and PCR-ve COVID-19 cases by week since onset of symptoms.

IgG/IgM in PCR+ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Jia 2020	21	0	3	0	FIA	0.88 [0.68, 0.97]	Not estimable
Liu 2020b	127	0	26	0	ELISA	0.83 [0.76, 0.89]	Not estimable

IgG/IgM in PCR-ve (all time points)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	56	0	7	0	CGIA	0.89 [0.78, 0.95]	Not estimable
Jia 2020	24	0	9	0	FIA	0.73 [0.54, 0.87]	Not estimable
Jin 2020	32	0	2	0	CLIA	0.94 [0.80, 0.99]	Not estimable
Liu 2020b	67	0	18	0	ELISA	0.79 [0.69, 0.87]	Not estimable

IgG/IgM in PCR+ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	5	0	4	0	ELISA	0.56 [0.21, 0.86]	Not estimable
Pan 2020a	3	0	24	0	CGIA	0.11 [0.02, 0.29]	Not estimable

IgG/IgM in PCR+ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	11	0	14	0	ELISA	0.44 [0.24, 0.65]	Not estimable
Pan 2020a	26	0	2	0	CGIA	0.93 [0.76, 0.99]	Not estimable

IgG/IgM in PCR+ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	111	0	8	0	ELISA	0.93 [0.87, 0.97]	Not estimable
Pan 2020a	30	0	1	0	CGIA	0.97 [0.83, 1.00]	Not estimable

IgG/IgM in PCR-ve (1 to 7 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	0	0	8	0	ELISA	0.00 [0.00, 0.37]	Not estimable
Pan 2020a	4	0	5	0	CGIA	0.44 [0.14, 0.79]	Not estimable

IgG/IgM in PCR-ve (8 to 14 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	15	0	3	0	CGIA	0.83 [0.59, 0.96]	Not estimable
Liu 2020b	9	0	7	0	ELISA	0.56 [0.30, 0.80]	Not estimable
Pan 2020a	5	0	1	0	CGIA	0.83 [0.36, 1.00]	Not estimable

IgG/IgM in PCR-ve (15 to 21 days)

Study	TP	FP	FN	TN	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	41	0	4	0	CGIA	0.91 [0.79, 0.98]	Not estimable
Liu 2020b	58	0	3	0	ELISA	0.95 [0.86, 0.99]	Not estimable
Pan 2020a	5	0	2	0	CGIA	0.71 [0.29, 0.96]	Not estimable

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Impact of reference standard for non-COVID-19 cases on specificity

We classified the reference standard used to verify non-COVID cases into three main groups: pre-pandemic controls (both healthy and with other diseases) who underwent no RT-PCR testing, current controls from healthy or other disease groups (typically who also did not undergo RT-PCR testing), and individuals who were investigated for COVID-19 but deemed non-COVID cases. Whilst results were similar for IgG and IgM, we noted more false positives for the IgG/IgM outcome in the studies using a COVID suspect group than in other studies (Table 3).

Sensitivity and specificity by assay type

We further investigated the heterogeneity in sensitivity estimates at any time point according to test technology type. We considered differences between CGIA, CLIAs, ELISAs and tests we can only describe as lateral flow assays due to lack of any names or detail (this group originate from the UK National COVID Testing Scientific Advisory Panel, which withheld names of the tests evaluated due to confidentiality clauses in the legal contracts with the manufacturers Adams 2020 [A]). There were inadequate numbers of studies evaluating FIAs and indirect immunofluorescence tests, luciferase immunoprecipitation assays and 'S-flow' assays to analyse, and we were only able to assess IgG, IgM and IgG/IgM targets. In a sensitivity analysis we restricted the included studies to those that used commercial (rather than in-house) tests.

We obtained estimates from a model that included all data stratified by weeks since onset of symptoms. The results presented in Table 7 and below correspond to estimates from the model of performance in week 3 post-symptom onset.

For IgG, there were clear differences in the sensitivity of assays, with CLIA (94.6%), CGIA (87.3%) and ELISA (85.8%) all outperforming the unknown lateral flow assay tests (76.0%). The differences between the groups was beyond that expected by chance (P = 0.004), but largely driven by the low value for lateral flow tests (all of the data coming from 40 COVID-19 patients in the UK National COVID Testing Scientific Advisory Panel study tested multiple times).

For IgM, although laboratory-based ELISA (84.5%) and CLIA (80.9%) outranked lateral flow CGIA (69.5%) and the unknown lateral flow assays (51.4%), the differences observed were in the realms of those expected by chance (P = 0.11).

In the smaller subset of studies that evaluated tests combining IgM/IgG, the performance of laboratory CLIA tests (97.3%) ranked above those of CGIA (91.4%), ELISA (90.5%) and unknown lateral flow tests (85.8%). These differences were beyond those expected by chance (P = 0.01)

Excluding the in-house tests, and thus restricting the analysis to only commercial tests, made little difference to estimates of sensitivity.

Analyses of specificity presented by assay type are also given in Table 7. Differences in specificity of IgG and IgM between assay types were small, CLIA and CGIA tests showed lower specificity for IgG/IgM tests than ELISA and LFIA, but confidence intervals on all estimates are wide.

Sensitivity and specificity by brand

We have tabulated the results by brand for the 27 commercial tests: 15 tests for IgG Table 8; 14 tests for IgM Table 9; and nine tests for IgG/IgM Table 10. The study data for these estimates are provided in Figure 4, Figure 5 and Figure 6. Appendix 12 tabulates the information that we have been able to derive regarding the current availability of these commercially produced tests. Data for sensitivity are stratified by week of onset of symptoms and we present the numbers of studies and samples from which data are available for each time interval. Caution is required in the interpretation of these data as many are based only on single studies with small sample sizes. We present confidence intervals to quantify the uncertainty in the estimates. We would advise focusing on estimates based on at least 100 samples/participants per week further. Three tests have estimates of sensitivity based on more than 100 samples (Beijing Wantai ELISA, Bioscience Co. (Chongqing) CLIA, Zuhai Livzon ELISA). We evaluated the studies that we pooled to create these estimates as having multiple domains at risk of bias and having concerns about the applicability of the findings (all studies having at most 2 of the 7 ratings in the QUADAS-2 assessment described as low risk or low concern).

Eight tests have estimates of specificity based on more than 100 samples, with estimates over 98% for five tests (Bejing Hotgen ELISA, Beijing Wantai ELISA, Beijing Wantai CGIA, Xiamen InnodDx Biotech ELISA, Zhuhai Livzon ELISA). Again please note the concerns in the risk of bias and applicability of these findings.

Other sources of heterogeneity

Our protocol included additional planned analyses by:

- current infection or past infection;
- study design; and
- setting.

We could not investigate these sources because of lack of variability across the studies in these features. Only two studies explicitly stated that they recruited only convalescent patients, and 48 (85%) studies recruited hospital inpatients. For study design only five out of 54 (11%) studies recruited a single group of suspected COVID-19 patients, and did not use a 'COVID-19 cases only' study, or a 'two-group' study design.

Investigation of publication bias

We observed direct evidence of selective reporting through the withholding of names of the nine lateral flow assay testing brands from the UK National COVID Testing Scientific Advisory Panel study (Adams 2020 [A]). The paper states, "Individual manufacturers did not approve release of device-level data, so device names are anonymised" (Adams 2020 [A]). The sensitivity estimates for the lateral flow assays in this study (which are most likely to be CGIA) were noted to be lower than estimates for CGIA tests from other studies. Four other studies also did not identify the test that they were evaluating.

DISCUSSION

This is the first version of a Cochrane living review summarising the accuracy of antibody tests for detecting current or previous SARS-CoV-2infection. This version of the review is based on published studies or studies available as preprints up until the 27 April 2020.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

The speed of development and publication of studies for COVID-19 antibody tests is unprecedented, and the content of this review will always be out of date. We are continuously identifying new published studies, and plan to update this review several times during the next few months.

The studies included in this version are largely from China, evaluating tests from Chinese universities and manufacturers. Many of the studies are the first that have been published for each test, and thus are early-phase studies. Whilst there is no recognised stage classification of diagnostic studies, there are several common features of those undertaken during test development. These include multiple tests being described as 'in-house', that thresholds for tests are determined from the data collected during the study, that all tests are undertaken by technical experts in laboratories, that the samples used are from collections easily available to the research team, and that multiple samples are used from the same participants. These limitations explain much of the rating for high risk of bias and concerns about applicability in this review. Many of these issues make it likely that the accuracy of tests when used in clinical care will be lower than that observed here. We did locate six evaluations recruiting patients identified in clinical pathways before it was established whether they had COVID-19. This is more likely to produce results that reflect clinical practice, and we encourage future evaluations to consider this study design.

A concern with this review, and with its updates, is the high likelihood of selective reporting of results, particularly by manufacturers. We have already noted manufacturers being unwilling to be identified in the UK National COVID Testing Scientific Advisory Panel study (Adams 2020 [A]). Unlike randomised controlled trials of interventions, there are no requirements for test accuracy studies to be prospectively registered on study registers, nor to publish their findings. Many industry studies are only briefly described on 'Information for use' documents included with the tests, and study reports submitted to regulators are regarded as confidential. We are also aware that there are independent studies undertaken by National Public Health bodies, some of which have been submitted to FIND's data tracking tool for speedy data sharing. We plead for greater transparency and full publication in this field and continue to encourage laboratories to submit data and reports via FIND's portal. We request sharing of any unpublished reports for inclusion in future updates (please send to coviddta@contacts.bham.ac.uk). We have contacted test manufacturers to request full study reports which we will include in a future update of this review.

Summary of main results

We summarise 10 key findings from this review.

1. Evaluations of most antibody tests on the market are not available as publications or even as preprints. This review has evaluated data from 25 commercial tests and numerous in-house assays. These represent a small fraction of the antibody assays currently available. We have identified 66 additional studies of antibody tests published or available as preprints up until 25 May 2020, which we will appraise for inclusion in the review update, but there still remain no published data for the majority of tests on the current FIND list.
2. The design and execution of the current studies limits the strength of conclusions that we are currently able to draw. Nearly all studies sampled COVID-19 cases and non-COVID cases separately, and methods for selecting participants were not described. Only four studies reported blinding reference standard and index tests, and some reference standards may misclassify individuals.
3. Many studies only applied tests in laboratory settings on plasma or serum, whilst they are also approved for use as point-of-care tests using whole blood. From these data it is not possible to ascertain the clinical accuracy of these tests in lower resource and more accessible settings.
4. Sensitivity varies with the time since of onset of symptoms. Figures from the studies showed the ability of antibody tests to detect SARS-CoV-2infection is very low in the first week (average sensitivity 30.1%, 95% CI 21.4 to 40.7) and only moderate (average sensitivity 72.2%, 95% CI 63.5 to 79.5) in the second week post-symptom onset. These estimates are based on patients who have been hospitalised with COVID-19, and remain in hospital at the time of sampling, and thus are likely to represent the more severe end of the disease spectrum and are potentially individuals with higher antibody responses.
5. Tests have higher sensitivity when done later in the course of the disease. The average sensitivity across all the included studies for IgG/IgM tests was estimated from the included studies as 91.4% (95% CI 87.0 to 94.4) for 15 to 21 days, and 96.0% (95% CI 90.6 to 98.3) for 22 to 35 days. Too few studies had evaluated tests beyond 35 days to estimate accuracy. These findings are expected given the delayed rise of IgG antibodies.
6. Studies estimate the specificity of tests precisely, and it appears to be high. The average from the studies for IgG/IgM is 98.7% (95% CI 97.2% to 99.4%). However, estimates of specificity are mainly based on testing pre-pandemic, healthy people, or people known to have other disorders, and not those being investigated for possible COVID-19.
7. From the limited evaluations studied, some differences were noted by test technology, CLIA methods appearing more sensitive (97.5%, 95% CI 94.0 to 99.0) than ELISA (90.7%, 95% CI 83.3 to 95.0) or CGIA-based lateral flow assays (90.7%, 95% CI 82.7 to 95.2) for IgG/IgM, (there are also differences for IgG but no differences for IgM). There was little clear evidence of differences in specificity between technology types.
8. There is currently too little data on individual tests to be able to consider comparisons of their performance.
9. Study reports did not include many of the key items listed on the STARD reporting guideline for test accuracy studies (Bossuyt 2015), which has hindered assessment and data extraction. No study utilised a STARD participant flow diagram to enable identification of missing, indeterminate or unavailable test results.
10. We observed partial reporting (suppression of the identify of tests) in five studies, indicating the likelihood of publication bias.

Strengths and weaknesses of the review

Our review used a broad search screening all articles concerning COVID-19. We undertook all screening and eligibility assessments, QUADAS-2 assessments (Whiting 2011), and data extraction of study findings independently and in duplicate. Whilst we thus have reasonable confidence in the completeness and accuracy of the findings up until the search date, should errors be noted please inform us at coviddta@contacts.bham.ac.uk so that we can check and correct in our next update.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Weaknesses of the review primarily reflect the weaknesses in the primary studies and their reporting. Many studies omitted descriptions of sample recruitment, and key aspects of study design and execution. Some studies omit information that allows the tests to be identified. We have had to treat studies that describe their data as being based on 'samples' as if the samples were individual patients. We have been explicit about these issues where they arose.

More than half (28/54) of the studies we have included are currently only available as preprints, and as yet, have not undergone peer review. As published versions of these studies are identified in the future, we will double-check study descriptions, methods and findings, and update the review as required.

We also did not make within-study comparisons between tests. Two studies (Adams 2020 [A]; Lassauniere 2020 [A]), evaluated panels of nine or 10 tests, nine other studies evaluated two, three, or five tests. As we could not identify tests in Adams 2020 [A], and the sample of Lassauniere 2020 [A] was very small, it is not possible from the studies available at this time to make direct comparisons between alternative tests.

We identified only one study that included comparison of test results with a reference standard of a neutralisation assay in studies identified for inclusion in this first version of the review (Thompson 2020), but we did not include these data in this version of the review. We are aware of several more studies of these assays in more recent publications and will include this as a new target condition in the next update of the review.

In such a current and fast moving field searches will always be out of date. However we are committed to ongoing updates of this living review

Applicability of findings to the review question

In the background we outlined four main roles for antibody testing that would be addressed in this review.

1. In diagnosis of infection in patients presenting with symptoms of suspected COVID-19, particularly where molecular testing had failed to detect the virus. Most studies included in the review collected data from patients in the acute phase of disease in hospital settings and thus provide evidence to address this question amongst hospitalised patients. The review showed that antibody tests had very low sensitivity in the first week following onset of symptoms, but sensitivity rose in the second week, and only exceeded 90% in the third week. In addition we saw no difference in sensitivity of tests according to RT-PCR status. We had no data to inform the accuracy of the test in primary care and community settings for the purpose of diagnosis, where patients are likely to have milder symptoms.
2. In assessment of immune response in patients with severe disease. We stated in the Background that we would not cover this in this review. In any case, we found no studies that directly addressed this question. Assessment of the accuracy of a test used for assessment of immune response would involve comparison with a reference standard test of antibody response, rather than evidence of infection.
3. To assess whether individuals have had a SARS-CoV-2 infection. As above, we found no studies that directly addressed this question, and very few studies were undertaken in community settings in patients who had not undergone RT-PCR testing during their symptomatic period. Conclusions about the likely value of tests for this purpose rely on the sensitivity of the tests being no different in mild disease than in severe disease that requires hospital admission.
4. In seroprevalence surveys for public health management purposes. We also found no studies that directly addressed this question (although Bendavid 2020 is a seroprevalence study, it did not evaluate the accuracy of the test in the seroprevalence sample). High specificity of tests is essential in seroprevalence testing, which appears likely for many of the tests included in this review. However, the suitability of pre-pandemic samples to establish specificity requires further discussion. We found no difference in specificity between pre-pandemic and current non-COVID-19 samples, but lower specificity in those where COVID-19 was ruled out after initially being suspected. This either reflects misclassification, or a true lower specificity in those presenting with symptoms. As sensitivity of the tests was mainly evaluated in hospitalised patients it is also unclear whether the tests have the ability to detect lower antibody levels likely in non-hospitalised COVID-19 patients.

AUTHORS' CONCLUSIONS

Implications for practice

Diagnosis of acute suspected COVID-19 in symptomatic patients

Based on this analysis, in patients presenting with symptoms of acute suspected COVID-19, antibody tests have no role on their own as the primary test to use in the diagnosis of COVID-19 when patients present during the first week since onset of symptoms, as their sensitivity is too low.

A small number of studies showed that the sensitivity of antibody tests is no different in those who were reverse transcription polymerase chain reaction (RT-PCR)-negative rather than RT-PCR-positive. Thus in hospitalised patients where molecular tests have failed to detect virus, antibody tests have an increasing likelihood of detecting immune response to the infection as time since onset of symptoms progresses.

There may therefore be a role in using antibody tests in COVID-19 RT-PCR-negative but strongly suspected patients where patients are more than two weeks since the onset of symptoms. This is in line with the most recent version of the China CDC (National Health Commission of the People's Republic of China) COVID-19 case definition (Appendix 2).

Assessment of previous SARS-CoV-2 infection and immune response

The data analysed in the review suggest that antibody tests are likely to have a useful role for detecting previous SARS-CoV-2 infection if used at 15 days or more after the onset of symptoms. This conclusion needs to be cautioned by the poor study quality, the small sample sizes and restricted number of tests that have undergone evaluation. In addition, we have scant data to inform the accuracy of the test in non-hospitalised patients with milder disease, and too little data to comment on accuracy beyond 35 days.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Using, for illustration the overall IgG/IgM data at days 15 to 21 (sensitivity 91.4%, 95% CI 87.0 to 94.4 and specificity 98.7%, 93% CI 97.2 to 99.4), we have computed predictive values, and the numbers of true positives, false positives, false negatives and true negatives in a sample of 1000, at a prevalence of 50% (a value seen in healthcare worker populations who have suffered respiratory symptoms in the past months). In this scenario, the positive predictive value is estimated as 99% (95% CI 97 to 99), the negative predictive value as 92% (95% CI 88 to 95), and of 1000 people undergoing testing we would anticipate 7 (95% CI 3 to 14) false positives and 43 (95% CI 28 to 65) false negatives.

Please note that it is not certain whether a detectable immune response indicates that a patient is immune nor no longer infectious.

Seroprevalence surveys for public health management purposes

The duration of antibody rises is not yet known, and this review contains very little data beyond 35 days post-onset of symptoms. In the 'Summary of findings' table we present scenarios for the likely numbers of missed cases (false negatives) and false positive cases for prevalences of 2%, 5%, (likely values in national surveys), 10% and 20% (likely values in high-risk settings such as healthcare workers), presuming that the performance of an IgG/IgM test would continue at the same level as for 14-21 days. Again this conclusion needs to be cautioned by the poor study quality, the applicability of the study settings, the small sample sizes and restricted number of tests that have undergone evaluation. At a prevalence of 20%, a possible value in surveys in high-risk settings, 17 (95% CI 11 to 26) would be missed per 1000 people tested and 10 (95% CI 5 to 22) would be falsely positive. At a lower prevalence of 5%, a likely value in national surveys, 4 (95% CI 3 to 7) would be missed per 1000 tested, and 12 (95% CI 6 to 27) would be falsely positive.

Implications for research

Many more high-quality evaluation studies of COVID-19 antibody tests are needed in patients more than 21 days post-symptom onset, and in people in the community, particularly those who experience milder symptoms, or who are asymptomatic (but known to be infected).

Future studies must report data on sensitivity disaggregated by time since onset of symptoms. In future updates of this review we will not include studies for analysis of sensitivity where this has not been done. We would suggest that studies standardise how they define time since symptom onset (not, for example, using time since positive RT-PCR results since this has no biological basis) and present results using standard time groupings (we suggest initially by week up until 35 days and larger time intervals beyond). Studies that sample from the same patients at several time points over time are needed to fully understand how time since symptom onset directly affects performance – our current estimates are based on collation of multiple cross-sectional studies, which has limitations.

Primary studies need to be undertaken for the many tests that are on the market but as yet have no independent evaluations. Future studies should evaluate test performance in consecutive individuals who are recruited in clinical care with suspected COVID-19, to estimate both sensitivity and specificity, as this will estimate the likely performance of the tests in practice.

COVID-19-positive cases who are RT-PCR-negative should be included as well as those confirmed RT-PCR, in accordance with the World Health Organization (WHO) and China CDC case definitions.

Studies should ensure that the test is used as it is intended to be used in clinical practice (i.e. being undertaken at point-of-care rather than in laboratories (where appropriate) on the right specimens, by the intended healthcare worker). However, when validating people with suspected COVID-19 who do not have a positive identification of COVID-19 by RT-PCR, these studies need to take care to confirm or rule out COVID-19 by obtaining standardised evidence from other sources (e.g. repeat RT-PCR, CT scans, follow-up). Future studies need to recruit larger sample sizes and consider recruiting from multiple centres. We did not find any multicentre studies for this review.

We would also encourage investigators to utilise blinding in their study designs, such that index tests are undertaken without knowledge of the reference standard diagnosis, and likewise, reference standards are determined without knowledge of the index test findings.

We need good data upon which to compare tests. The strongest comparisons are made by testing the same participants multiple times with different tests. Whilst it is possible for this to be undertaken in prospective studies, it is easier to undertake in laboratory-based studies utilising serum banks, which will compromise on the applicability of the absolute estimates of test accuracy, but provide some information about comparability.

From these studies we can only draw limited conclusions about cross-reactivity of COVID-19 tests with other coronaviruses as these data are summarised in analytical accuracy studies. It would be of value for these results to be reviewed as well as clinical accuracy studies.

Study reporting requires substantial improvement. The STARD checklist outlines standard requirements for the reporting of a test accuracy study, which study investigators should take note of when planning their study to ensure the relevant information is collected and reported. No study was found that reported data using a STARD participant flow-diagram (Bossuyt 2015).

Due to the speed of new publications in this field, frequent updates of this review are required. Future updates will not include data on tests that are not (or not likely to become) commercially available (thus we will exclude all in-house assays).

ACKNOWLEDGEMENTS

Members of the Cochrane COVID-19 Diagnostic Test Accuracy Review Group include:

- the project team (Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Leeflang MMG, Spijker R, Hooft L, Van den Bruel A, McInnes MDF, Emperador D, Dittrich S);

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

- the systematic review teams for each review:
  * Molecular, antigen, and antibody tests (Adriano A, Beese S, Dretzke J, Ferrante di Ruffano L, Harris I, Price M, Taylor-Phillips S)
  * Signs and symptoms (Stuyf T, Domen J, Horn S)
  * Routine laboratory markers (Yang B, Langendam M, Ochodo E, Guleid F, Holtman G, Verbakel J, Wang J, Stegeman I)
  * Imaging tests (Salameh JP, McGrath TA, van der Pol CB, Frank RA, Prager R, Hare SS, Dennie C, Jenniskens K, Korevaar DA, Cohen JF, van de Wijgert J, Damen JAAG, Wang J);
- the wider team of systematic reviewers from University of Birmingham, UK who assisted with title and abstract screening across the entire suite of reviews for the diagnosis of COVID-19 (Agarwal R, Baldwin S, Berhane S, Herd C, Kristunas C, Quinn L, Scholefield B).

We thank Dr Jane Cunningham (World Health Organization) for participation in technical discussions and comments on the manuscript.

The editorial process for this review was managed by Cochrane's EMD Editorial Service in collaboration with Cochrane Infectious Diseases. We thank Helen Wakeford, Anne-Marie Stephani and Deirdre Walshe for their comments and editorial management. We thank Liz Bickerdike for comments on the Abstract. We thank Robin Featherstone for comments on the search and Mike Brown and Paul Garner for sign-off comments. We thank Denise Mitchell for her efforts in copy-editing this review.

Thank you also to peer referees Danny Altmann, Jessica Watson, Jeannette Guarner and Carlos Del Rio, consumer referee Dee Duckworth Shneiderman and methodological referees Danielle van der Windt and Matthew Grainge, for their insights.

The editorial base of Cochrane Infectious Diseases is funded by UK aid from the UK Government for the benefit of low- and middle-income countries (project number 300342-104). The views expressed do not necessarily reflect the UK Government's official policies.

Jonathan Deeks is a UK National Institute for Health Research (NIHR) Senior Investigator Emeritus. Yemisi Takwoingi is supported by a NIHR Postdoctoral Fellowship. Jonathan Deeks, Jacqueline Dinnes, Yemisi Takwoingi, Clare Davenport and Malcolm Price are supported by the NIHR Birmingham Biomedical Research Centre. This paper presents independent research supported by the NIHR Birmingham Biomedical Research Centre at the University Hospitals Birmingham NHS Foundation Trust and the University of Birmingham. The views expressed are those of the author(s) and not necessarily those of the NHS, the NIHR or the Department of Health and Social Care.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

REFERENCES

References to studies included in this review

Adams 2020 [A] *{published data only}*

Adams ER, Anand R, Andersson MI, Auckland K, Baillie JK, Barnes E, et al. Evaluation of antibody testing for SARS-Cov-2 using ELISA and lateral flow immunoassays. *medRxiv [Preprint]* 2020. [www.medrxiv.org/content/10.1101/2020.04.15.20066407v1.full.pdf]

Adams 2020 [B] *{published data only}*

Adams 2020 [C] *{published data only}*

Adams 2020 [D] *{published data only}*

Adams 2020 [E] *{published data only}*

Adams 2020 [F] *{published data only}*

Adams 2020 [G] *{published data only}*

Adams 2020 [H] *{published data only}*

Adams 2020 [I] *{published data only}*

Adams 2020 [J] *{published data only}*

Bendavid 2020 *{published data only}*

Bendavid E, Mulaney B, Sood N, Shah S, Ling E, Bromley-Dulfano R, et al. COVID-19 antibody seroprevalence in Santa Clara County, California. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.14.20062463]

Burbelo 2020 [A] *{published data only}*

Burbelo PD, Riedo FX, Morishima C, Rawlings S, Smith D, Das S, et al. Detection of nucleocapsid antibody to SARS-CoV-2 is more sensitive than antibody to spike protein in COVID-19 patients. *MedRxiv [Preprint]* 2020.

Burbelo 2020 [B] *{published data only}*

Cai 2020a *{published data only}*

Cai X, Chen J, Hu J, Long Q, Deng H, Fan K, et al. A peptide-based magnetic chemiluminescence enzyme immunoassay for serological diagnosis of corona virus disease 2019 (COVID-19). *MedRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.02.22.20026617]

Cassaniti 2020 (A) *{published data only}*

Cassaniti I, Novazzi F, Giardina F, Salivaro F, Sachs M, Perlini S, et al. Performance of VivaDiagTM COVID-19 IgM/IgG Rapid Test is inadequate for diagnosis of COVID-19 in acute patients referring to emergency room department. *Journal of Medical Virology* 2020 Mar 30 [Epub ahead of print]. [DOI: 10.1002/jmv.25800]

Cassaniti 2020 (B) *{published data only}*

Chen 2020a *{published data only}*

Chen Z, Zhang Z, Zhai X, Li Y, Lin L, Zhao H, et al. Rapid and sensitive detection of anti-SARS-CoV-2 IgG using lanthanide-doped nanoparticles-based lateral flow immunoassay. *Analytical Chemistry* 2020;**92**(10):7226-31.

Dohla 2020 *{published data only}*

Dohla M, Boesecke C, Schulte B, Diegmann C, Sib E, Richter E, et al. Rapid point-of-care testing for SARS-CoV-2 in a community screening setting shows low sensitivity. *Public Health* 2020;**182**:170-2.

Du 2020 *{published data only}*

Du Z, Zhu F, Guo F, Yang B, Wang T. Detection of antibodies against SARS-CoV-2 in patients with COVID-19. *Journal of Medical Virology* 2020 Apr 3 [Epub ahead of print]. [DOI: 10.1002/jmv.25820]

Freeman 2020 *{published data only}*

Freeman B, Lester S, Mills L, Rasheed MA, Moye S, Abiona O, et al. Validation of a SARS-CoV-2 spike ELISA for use in contact investigations and serosurveillance. *bioRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.24.057323]

Gao 2020a *{published data only}*

Gao Y, Yuan Y, Li T T, Wang W X, Li Y X, Li A, et al. Evaluation the auxiliary diagnosis value of antibodies assays for detection of novel coronavirus (SARS-Cov-2) causing an outbreak of pneumonia (COVID-19). *medRxiv [Preprint]* 2020.

* Gao Y, Yuan Y, Li TT, Wang WX, Li YX, Li A, et al. Evaluation of the auxiliary diagnostic value of antibody assays for the detection of novel coronavirus (SARS-CoV-2). *Journal of Medical Virology* 2020. [DOI: 10.1002/jmv.25919]

Gao 2020b [A] *{published data only}*

Gao HX, Li YN, Xu ZG, Wang YL, Wang HB, Cao JF, et al. Detection of serum immunoglobulin M and immunoglobulin G antibodies in 2019-novel coronavirus infected cases from different stages. *Chinese Medical Journal (Engl)* 2020 Mar 26 [Epub ahead of print]. [DOI: 10.1097/CM9.0000000000000820]

Gao 2020b [B] *{published data only}*

Gao 2020b [C] *{published data only}*

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (A) *{published data only}*

Garcia FP, Perez Tanoira R, Romanyk Cabrera JP, Arroyo Serrano T, Gomez Herruz P, Cuadros Gonzalez J. Rapid diagnosis of SARS-CoV-2 infection by detecting IgG and IgM antibodies with an immunochromatographic device: a prospective single-center study. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.11.20062158]

Garcia 2020 (B) *{published data only}*

Grzelak 2020 [A] *{published data only}*

Grzelak L, Temmam S, Planchais C, Demeret C, Huon C, Guivel F, et al. SARS-CoV-2 serological analysis of COVID-19 hospitalized patients, pauci-symptomatic individuals and blood donors. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.21.20068858]

Grzelak 2020 [B] *{published data only}*

Grzelak 2020 [C] *{published data only}*

Grzelak 2020 [D] *{published data only}*

Grzelak 2020 [E] *{published data only}*

Guo 2020a *{published data only}*

Guo L, Ren L, Yang S, Xiao M, Chang, Yang F, et al. Profiling early humoral response to diagnose novel coronavirus disease (COVID-19). *Clinical Infectious Diseases* 2020. [DOI: doi.org/10.1093/cid/ciaa310]

Hu 2020a *{published data only}*

Hu Q, Cui X, Liu X, Peng B, Jiang J, Wang X, et al. The production of antibodies for SARS-CoV-2 and its clinical implication. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.20.20065953]

Infantino 2020 *{published data only}*

Infantino M, Grossi V, Lari B, Bambi R, Perri A, Manneschi M, et al. Diagnostic accuracy of an automated chemiluminescent immunoassay for anti-SARS-CoV-2 IgM and IgG antibodies: an Italian experience. *Journal of Medical Virology* 2020 Apr 24 [Epub ahead of print]. [DOI: 10.1002/jmv.25932]

Jia 2020 *{published data only}*

Jia X, Zhang P, Tian Y, Wang J, Zeng H, Wang J, et al. Clinical significance of IgM and IgG test for diagnosis of highly suspected COVID-19 infection. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.02.28.20029025]

Jin 2020 *{published data only}*

Jin Y, Wang M, Zuo Z, Fan C, Ye F, Cai Z, et al. Diagnostic value and dynamic variance of serum antibody in coronavirus disease 2019. *International Journal of Infectious Diseases* 2020;**94**:49-52. [DOI: 10.1016/j.ijid.2020.03.065]

Lassauniere 2020 [A] *{published data only}*

Lassauniere R, Frische A, Harboe ZB, Nielsen AC, Fomsgaard A, Krogfelt KA, et al. Evaluation of nine commercial SARS-CoV-2 immunoassays. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.09.20056325]

Lassauniere 2020 [B] *{published data only}*

Lassauniere 2020 [C] *{published data only}*

Lassauniere 2020 [D] *{published data only}*

Lassauniere 2020 [E] *{published data only}*

Lassauniere 2020 [F] *{published data only}*

Lassauniere 2020 [G] *{published data only}*

Lassauniere 2020 [H] *{published data only}*

Lassauniere 2020 [I] *{published data only}*

Li 2020a *{published data only}*

Li Z, Yi Y, Luo X, Xiong N, Liu Y, Li S, et al. Development and clinical application of a rapid IgM-IgG combined antibody test for SARS-CoV-2 infection diagnosis. *Journal of Medical Virology* 2020 Feb 27 [Epub ahead of print]. [DOI: 10.1002/jmv.25727]

Lin 2020a [A] *{published data only}*

Lin D, Liu L, Zhang M, Hu Y, Yang Q, Guo J, et al. Evaluations of serological test in the diagnosis of 2019 novel coronavirus (SARS-CoV-2) infections during the COVID-19 outbreak. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.27.20045153]

Lin 2020a [B] *{published data only}*

Lippi 2020 [A] *{published data only}*

Lippi G, Salvagno GL, Pegoraro M, Militello V, Caloi C, Peretti A, et al. Assessment of immune response to SARS-CoV-2 with fully automated MAGLUMI 2019-nCoV IgG and IgM chemiluminescence immunoassays. *Clinical Chemistry and Laboratory Medicine* 2020 Apr 16 [Epub ahead of print]. [DOI: 10.1515/cclm-2020-0473]

Lippi 2020 [B] *{published data only}*

Liu 2020a *{published data only}*

Liu Y, Liu Y, Diao B, Ren F, Wang Y, Ding J, et al. Diagnostic indexes of a rapid IgG/IgM combined antibody test for SARS-CoV-2. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.26.20044883]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020b *{published data only}*

* Liu L, Liu W, Wang S, Zheng S. A preliminary study on serological assay for severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) in 238 admitted hospital patients. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.06.20031856]

Liu 2020c *{published data only}*

Liu R, Liu X, Han H, Shereen MA, Niu Z, Li D, et al. The comparative superiority of IgM-IgG antibody test to real-time reverse transcriptase PCR detection for SARS-CoV-2 infection diagnosis. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.28.20045765]

Liu 2020d [A] *{published data only}*

* Liu W, Liu L, Kou G, Zheng Y, Ding Y, Ni W, et al. Evaluation of nucleocapsid and spike protein-based ELISAs for detecting antibodies against SARS-CoV-2. *Journal of Clinical Microbiology* 2020. [DOI: 10.1128/JCM.00461-20]

Liu W, Liu L, Kou G, Zheng Y, Ding Y, Ni W, et al. Evaluation of nucleocapsid and spike protein-based ELISAs for detecting antibodies against SARS-CoV-2. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.16.20035014]

Liu 2020d [B] *{published data only}*

Long 2020 (A) *{published data only}*

Long Q, Deng H, Chen J, Hu J, Liu B, Liao P, et al. Antibody responses to SARS-CoV-2 in COVID-19 patients: the perspective application of serological tests in clinical practice. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.18.20038018]

Long 2020 (B) *{published data only}*

Lou 2020 [A] *{published data only}*

Lou B, Li T, Zheng S, Su Y, Li Z, Liu W, et al. Serology characteristics of SARS-CoV-2 infection since the exposure and post symptoms onset. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.23.20041707]

Lou 2020 [B] *{published data only}*

Lou 2020 [C] *{published data only}*

Ma 2020a *{published data only}*

Ma H, Zeng W, He H, Zhao D, Yang Y, Jiang D, et al. COVID-19 diagnosis and study of serum SARS-CoV-2 specific IgA, IgM and IgG by a quantitative and sensitive immunoassay. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.17.20064907]

Okba 2020a *{published data only}*

* Okba NM, Muller MA, Li W, Wang C, GeurtsvanKessel CH, Corman VM, et al. Severe acute respiratory syndrome coronavirus 2-specific antibody responses in coronavirus disease 2019 patients. *Emerging Infectious Diseases* 2020 Apr 8 [Epub ahead of print];**26**(7).

Woelfel R, Corman VM, Guggemos W, Seilmaier M, Zange S, Muller MA, et al. Virological assessment of hospitalized patients with COVID-2019. *Nature* 2020;**581**:465-9.

Padoan 2020 *{published data only}*

Padoan A, Cosma C, Sciacovelli L, Faggian D, Plebani M. Analytical performances of a chemiluminescence immunoassay for SARS-CoV-2 IgM/IgG and antibody kinetics. *Clinical Chemistry and Laboratory Medicine* 2020. [DOI: doi.org/10.1515/cclm-2020-0443]

Pan 2020a *{published data only}*

* Pan Y, Li X, Yang G, Fan J, Tang Y, Zhao J, et al. Serological immunochromatographic approach in diagnosis with SARS-CoV-2 infected COVID-19 patients. *Journal of Infection* (in press).

Pan Y, Li X, Yang G, Fan J, Tang Y, Zhao J, et al. Serological immunochromatographic approach in diagnosis with SARS-CoV-2 infected COVID-19 patients. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.13.20035428]

Paradiso 2020a *{published data only}*

Paradiso AV, De Summa S, Loconsole D, Procacci V, Sallustio A, Centrone F, et al. Clinical meanings of rapid serological assay in patients tested for SARS-Co2 RT-PCR. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.03.20052183]

Qian 2020 *{published data only}*

Qian C, Zhou M, Cheng F, Lin X, Gong Y, Xie X, et al. Development and multicenter performance evaluation of the first fully automated SARS-CoV-2 IgM and IgG immunoassays. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.04.16.20067231]

To 2020a [A] *{published data only}*

To KK, Tsang OT, Leung WS, Tam AR, Wu TC, Lung DC, et al. Temporal profiles of viral load in posterior oropharyngeal saliva samples and serum antibody responses during infection by SARS-CoV-2: an observational cohort study. *Lancet Infectious Diseases* 2020;**20**(5):565-74.

To 2020a [B] *{published data only}*

Wan 2020 [A] *{published data only}*

Wan W Y, Lim S H, Seng E H. Cross-reaction of sera from COVID-19 patients with SARS-CoV assays. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.17.20034454]

Wan 2020 [B] *{published data only}*

Wang 2020a [A] *{published data only}*

Wang Q, Du Q, Guo B, Guo Y, Fang L, X Guo. Performance of urea-mediated dissociation in reducing false-positive of 2019-nCoV IgM test. *Chinese Journal of Laboratory Medicine* 2020. [DOI: 10.3760/cma.j.cn114452-20200219-00091]

* Wang Q, Du Q, Guo B, Mu D, Lu X, Ma Q, et al. A method to prevent SARS-CoV-2 IgM false positives in gold immunochromatography and enzyme-linked immunosorbent assays. *Journal of Clinjcal Microbiology* 2020. [DOI: 10.1128/JCM.00375-20]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wang 2020a [B] *{published data only}*

Xiang 2020a [A] *{published data only}*

Xiang J, Yan M, Li H, Liu T, Lin C, Huang S, et al. Evaluation of enzyme-linked immunoassay and colloidal gold-immunochromatographic assay kit for detection of novel coronavirus (SARS-Cov-2) causing an outbreak of pneumonia (COVID-19). *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.02.27.20028787]

Xiang 2020a [B] *{published data only}*

Xiang 2020b *{published data only}*

Xiang F, Wang X, He X, Peng Z, Yang B, Zhang J, et al. Antibody detection and dynamic characteristics in patients with COVID-19. *Clinical Infectious Diseases* 2020;**ciaa461**. [DOI: doi.org/10.1093/cid/ciaa461]

Xiao 2020a *{published data only}*

Xiao DA, Gao DC, Zhang DS. Profile of specific antibodies to SARS-CoV-2: the first report. *Journal of Infection* 2020. [DOI: doi.org/10.1016/j.jinf.2020.03.012]

Xie 2020a *{published data only}*

Xie J, Ding C, Li J, Wang Y, Guo H, Lu Z, et al. Characteristics of patients with coronavirus disease (COVID-19) confirmed using an IgM-IgG antibody test. *Journal of Medical Virology* 2020. [DOI: doi.org/10.1002/jmv.25930]

Xu 2020a *{published data only}*

Xu Y. Dynamic profile of severe or critical COVID-19 cases. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.18.20038513]

Yongchen 2020 *{published data only}*

Yongchen Z, Shen H, Wang X, Shi X, Li Y, Yan J, et al. Different longitudinal patterns of nucleic acid and serology testing results based on disease severity of COVID-19 patients. *Emerging Microbes and Infections* 2020;**9**(1):833-6.

Zeng 2020a *{published data only}*

Zeng Z, Chen L, Pan Y, Deng Q, Ye G, Li Y, et al. Re: Profile of specific antibodies to SARS-CoV-2: the first report. *Journal of Infection* 2020. [DOI: doi.org/10.1016/j.jinf.2020.03.052]

Zhang 2020a *{published data only}*

Zhang B, Zhou X, Zhu C, Feng F, Qiu Y, Feng J, et al. Immune phenotyping based on neutrophil-to-lymphocyte ratio and IgG predicts disease severity and outcome for patients with COVID-19. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.12.20035048]

Zhang 2020b *{published data only}*

Zhang J, Liu J, Li N, Liu Y, Ye R, Qin X, et al. Serological detection of 2019-nCoV respond to the epidemic: a useful complement to nucleic acid testing. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.04.20030916]

Zhang 2020c *{published data only}*

Zhang W, Du RH, Li B, Zheng XS, Yang X L, Hu B, et al. Molecular and serological investigation of 2019-nCoV infected patients: implication of multiple shedding routes. *Emerging Microbes and Infections* 2020;**9**(1):386-9.

Zhang 2020d *{published data only}*

Zhang P, Gao Q, Wang T, Ke Y, Mo F, Jia R, et al. Evaluation of recombinant nucleocapsid and spike proteins for serological diagnosis of novel coronavirus disease 2019 (COVID-19). *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.17.20036954]

Zhao 2020a *{published data only}*

* Zhao J, Yuan Q, Wang H, Liu W, Liao X, Su Y, et al. Antibody responses to SARS-CoV-2 in patients of novel coronavirus disease 2019. *Clinical Infectious Diseases* 2020;**ciaa344**. [DOI: doi.org/10.1093/cid/ciaa344]

Zhao J, Yuan Q, Wang H, Liu W, Liao X, Su Y, et al. Antibody responses to SARS-CoV-2 in patients of novel coronavirus disease 2019. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.02.20030189]

Zhao 2020b *{published data only}*

Zhao R, Li M, Song H, Chen J, Ren W, Feng Y, et al. Serological diagnostic kit of SARS-CoV-2 antibodies using CHO-expressed full-length SARS-CoV-2 S1 proteins. *medRxiv [Preprint]* 2020. [DOI: doi.org/10.1101/2020.03.26.20042184]

Zhong 2020 [A] *{published data only}*

Zhong L, Chuan J, Gong BO, Shuai P, Zhou Y, Zhang Y, et al. Detection of serum IgM and IgG for COVID-19 diagnosis. *Science China. Life Sciences* 2020;**63**(5):777-80. [DOI: 10.1007/s11427-020-1688-9]

Zhong 2020 [B] *{published data only}*

Zhong 2020 [C] *{published data only}*

References to studies excluded from this review

Ai 2020 *{published data only}*

Ai T, Yang Z, Hou H, Zhan C, Chen C, Lv W, et al. Correlation of Chest CT and RT-PCR testing in coronavirus disease 2019 (COVID-19) in China: a report of 1014 cases. *Radiology* 2020. [DOI: 10.1148/radiol.2020200642 10.1148/radiol.2020200642]

Aitken 2020 *{published data only}*

Aitken J, Ambrose K, Barrell S, Beale R, Bineva-Todd G, Biswas D, et al. Scalable and resilient SARS-CoV2 testing in an academic centre. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.19.20071373]

Amanat 2020 *{published data only}*

Amanat F, Nguyen T, Chromikova V, Strohmeier S, Stadlbauer D, Javier A, et al. A serological assay to detect SARS-CoV-2

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

seroconversion in humans. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.17.20037713]

Annamalai 2020 *{published data only}*

Annamalai P, Kanta M, Ramu P, Ravi B, Veerapandian K, Srinivasan R. A simple colorimetric molecular detection of novel coronavirus (COVID-19), an essential diagnostic tool for pandemic screening. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.10.20060293]

Argenziano 2020 *{published data only}*

Argenziano MG, Bruce SL, Slater CL, Tiao JR, Baldwin MR, Barr RG. Characterization and clinical course of 1000 patients with COVID-19 in New York: retrospective case series. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.20.20072116]

Arons 2020 *{published data only}*

Arons MM, Hatfield KM, Reddy SC, Kimball A, James A, Jacobs JR. Presymptomatic SARS-CoV-2 infections and transmission in a skilled nursing facility. *New England Journal of Medicine* 2020. [DOI: 10.1056/NEJMoa2008457]

Arumugam 2020 *{published data only}*

Arumugam A, Wong SS. The potential use of unprocessed sample for RT-qPCR detection of COVID-19 without an RNA extraction step. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.06.028811]

Baggett 2020 *{published data only}*

Baggett TP, Keyes H, Sporn N, Gaeta JM. COVID-19 outbreak at a large homeless shelter in Boston: implications for universal testing. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.12.20059618]

Bai 2020 *{published data only}*

Bai SL, Wang JY, Zhou YQ, Yu DS, Gao XM, Li LL, et al. Analysis of the first cluster of cases in a family of novel coronavirus pneumonia in Gansu Province. *Zhonghua Yu Fang Yi Xue Za Zhi* 2020;**54**(0):E005. [DOI: 10.3760/cma.j.issn.0253-9624.2020.0005 10.3760/cma.j.issn.0253-9624.2020.0005.]

Bajema 2020 *{published data only}*

Bajema KL, Oster AM, McGovern OL, Lindstrom S, Stenger MR, Anderson TC, et al. Persons evaluated for 2019 novel coronavirus - United States, January 2020. *MMWR. Morbidity and Mortality Weekly Report* 2020;**69**(6):166-70. [DOI: 10.15585/mmwr.mm6906e1 10.15585/mmwr.mm6906e1]

Barra 2020 *{published data only}*

Barra GB, Santa Rita TH, Mesquita PG, Jacomo RH, Nery LF. Analytical sensibility and specificity of two RT-qPCR protocols for SARS-CoV-2 detection performed in an automated workflow. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.07.20032326]

Batista 2020 *{published data only}*

Batista, AF, Miraglia JL, Donato TH, Chiavegatto Filho AD. COVID-19 diagnosis prediction in emergency care patients: a machine learning approach. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.04.20052092]

Beltran Corbellini 2020 *{published data only}*

Beltran-Corbellini NA, Chico-Garcia JL, Martinez-Poles J, Rodriguez-Jorge F, Natera-Villalba E, Gomez-Corral J, et al. Acute-onset smell and taste disorders in the context of COVID-19: a pilot multicenter PCR-based case-control study. *European Journal of Neurology* 2020 Apr 22 [Epub ahead of print]. [DOI: 10.1111/ene.14273]

Beltran Pavez 2020 *{published data only}*

Beltran-Pavez C, Marquez CL, Munoz G, Valiente-Echeverria F, Gaggero A, Soto-Rifo R, et al. SARS-CoV-2 detection from nasopharyngeal swab samples without RNA extraction. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.28.013508]

Ben Ami 2020 *{published data only}*

Ben-Ami R, Klochendler A, Seidel M, Sido T, Gurel-Gurevich O, Yassour M, et al. Pooled RNA extraction and PCR assay for efficient SARS-CoV-2 detection. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.17.20069062]

Bhadra 2020 *{published data only}*

Bhadra S, Maranhao AC, Ellington AD. A one-enzyme RT-qPCR assay for SARS-CoV-2, and procedures for reagent production. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.29.013342]

Bordi 2020 *{published data only}*

Bordi L, Nicastri E, Scorzolini L, Di Caro A, Capobianchi MR, Castilletti C, et al, on behalf of Inmi COVID-Study Group Collaborating Centers. Differential diagnosis of illness in patients under investigation for the novel coronavirus (SARS-CoV-2), Italy, February 2020. *Eurosurveillance* 2020;**25**(8):pii=2000170. [DOI: 10.2807/1560-7917.Es.2020.25.8.2000170 10.2807/1560-7917.ES.2020.25.8.2000170]

Burhan 2020 *{published data only}*

Burhan E, Prasenohadi P, Rogayah R, Isbaniyah F, Reisa T, Dharmawan I. Clinical progression of COVID-19 patient with extended incubation period, delayed RT-PCR time-to-positivity, and potential role of chest CT-scan. *Acta Medica Indonesiana* 2020;**52**(1):80-3.

Cai 2020 *{published data only}*

Cai J, Xu J, Lin D, Yang Z, Xu L, Qu Z, et al. A case series of children with 2019 novel coronavirus infection: clinical and epidemiological features. *Clinical Infectious Diseases* 2020. [DOI: 10.1093/cid/ciaa198 10.1093/cid/ciaa198]

Callahan 2020 *{published data only}*

Callahan CJ, Lee R, Zulauf K, Tamburello L, Smith KP, Previtera J, et al. Rapid open development and clinical validation of multiple new 3D-printed nasopharyngeal swabs in response to the COVID-19 pandemic. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.14.20065094]

Chan 2020 *{published data only}*

Chan JF, Yuan S, Kok KH, To KK, Chu H, Yang J, et al. A familial cluster of pneumonia associated with the 2019 novel coronavirus indicating person-to-person transmission: a study of a family cluster. *Lancet* 2020;**395**(10223):514-23.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

[DOI: 10.1016/s0140-6736(20)30154-9 10.1016/S0140-6736(20)30154-9. Epub 2020 Jan 24.]

Chandler Brown 2020 *{published data only}*

Chandler-Brown D, Bueno AM, Atay O, Tsao DS. A highly scalable and rapidly deployable RNA extraction-free COVID-19 assay by quantitative Sanger sequencing. *BioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.07.029199]

Chen 2020b *{published data only}*

Chen X, Ling J, Mo P, Zhang Y, Jiang Q, Ma Z, et al. Restoration of leukomonocyte counts is associated with viral clearance in COVID-19 hospitalized patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.03.20030437]

Chen 2020c *{published data only}*

Chen C, Li J, Di L, Jing Q, Du P, Song C, et al. MINERVA: A facile strategy for SARS-CoV-2 whole genome deep sequencing of clinical samples. *BioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.25.060947]

Cheng 2020a *{published data only}*

Cheng Z, Lu Y, Cao Q, Qin L, Pan Z, Yan F, et al. Clinical features and chest CT manifestations of coronavirus disease 2019 (COVID-19) in a single-center study in Shanghai, China. *American Journal of Roentgenology* 2020:1-6. [DOI: 10.2214/ajr.20.22959 10.2214/AJR.20.22959]

Chu 2020 *{published data only}*

Chu DK, Pan Y, Cheng SM, Hui KP, Krishnan P, Liu Y, et al. Molecular diagnosis of a novel coronavirus (2019-nCoV) causing an outbreak of pneumonia. *Clinical Chemistry* 2020. [DOI: 10.1093/clinchem/hvaa029 10.1093/clinchem/hvaa029.]

Colson 2020 *{published data only}*

Colson P, Lagier JC, Baudoin JP, Bou Khalil J, La Scola B, Raoult D. Ultrarapid diagnosis, microscope imaging, genome sequencing, and culture isolation of SARS-CoV-2. *European Journal of Clinical Microbiology & Infectious Diseases* 2020. [DOI: 10.1007/s10096-020-03869-w]

Comar 2020 *{published data only}*

Comar M, Brumat M, Concas MP, Argentini G, Bianco A, Bicego L, et al. COVID-19 experience: first Italian survey on healthcare staff members from a mother-child research hospital using combined molecular and rapid immunoassays test. *MedRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.19.20071563]

Corman 2020 *{published data only}*

Corman VM, Landt O, Kaiser M, Molenkamp R, Meijer A, Chu DK, et al. Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. *Eurosurveillance* 2020;**25**(3). [DOI: 10.2807/1560-7917.Es.2020.25.3.2000045 10.2807/1560-7917.ES.2020.25.3.2000045.]

Cui 2020 *{published data only}*

Cui P, Chen Z, Wang T, Dai J, Zhang J, Ding T, et al. Clinical features and sexual transmission potential of SARS-CoV-2 infected female patients: a descriptive study in Wuhan, China. *medRxiv [preprint]* 2020. [DOI: 10.1101/2020.02.26.20028225]

Curti 2020 *{published data only}*

Curti L, Pereyra-Bonnet F, Gimenez C. An ultrasensitive, rapid, and portable coronavirus SARS-CoV-2 sequence detection method based on CRISPR-Cas12. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.29.971127]

Dahlke 2020 *{published data only}*

Dahlke C, Heidepriem J, Kobbe R, Santer R, Koch T, Fathi A. Distinct early IgA profile may determine severity of COVID-19 symptoms: an immunological case series. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.14.20059733]

Ding 2020 *{published data only}*

Ding X, Yin K, Li Z, Liu C. All-in- one dual CRISPR-Cas12a (AIOD-CRISPR) assay: a case for rapid, ultrasensitive and visual detection of novel coronavirus SARS-CoV-2 and HIV virus. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.19.998724]

Fang 2020z *{published data only}*

Fang D, Ma J, Guan J, Wang M, Song Y, Tian D, et al. Manifestations of digestive system in hospitalized patients with novel coronavirus pneumonia in Wuhan, China: a single-center, descriptive study. *Chinese Journal of Digestion* 2020. [DOI: 10.3760/cma.j.issn. 0254-1432.2020.03.000]

Farfan 2020 *{published data only}*

Farfan MJ, Torres JP, Oryan M, Olivares M, Gallardo P, Salas C. Optimizing RT-PCR detection of SARS-CoV-2 for developing countries using pool testing. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.15.20067199]

Feng 2020 *{published data only}*

Feng K, Yun YX, Wang XF, Yang GD, Zheng YJ, Lin CM, et al. Analysis of CT features of 15 children with 2019 novel coronavirus infection. *Zhonghua Er Ke Za Zhi* 2020;**58**(0):E007. [DOI: 10.3760/cma.j.issn.0578-1310.2020.0007 10.3760/cma.j.issn.0578-1310.2020.0007.]

Fontanet 2020 *{published data only}*

Fontanet A, Tondeur L, Madec Y, Grant R, Besombes C, Jolly N, et al. Cluster of COVID-19 in northern France: a retrospective closed cohort study. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.18.20071134]

Fu 2020a *{published data only}*

Fu H, Xu H, Zhang N, Xu H, Li Z, Chen H, et al. Association between clinical, laboratory and CT characteristics and RT-PCR results in the follow-up of COVID-19 patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.19.20038315]

Fu 2020b *{published data only}*

Fu YQ, Sun YL, Lu SW, Yang Y, Wang Y, Xu F. Impact of blood analysis and immune function on the prognosis of patients with COVID-19. *medRxiv [preprint]* 2020. [DOI: 10.1101/2020.04.16.20067587]

Fumeaux 2020 *{published data only}*

Fumeaux T. COVID-19: Que sait-on des patients admis en soins intensifs? *Revue Medicale Suisse* 2020;**16**(690):756.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020 *{published data only}*

Gao Y, Li T, Han M, Li X, Wu D, Xu Y, et al. Diagnostic utility of clinical laboratory data determinations for patients with the severe COVID-19. *Journal of Medical Virology* 2020. [DOI: 10.1002/jmv.25770 10.1002/jmv.25770]

Giamarellos Bourboulis 2020 *{published data only}*

Giamarellos-Bourboulis EJ, Netea MG, Rovina N, Akinosoglou K, Antoniadou A, Antonakos N, et al. Complex immune dysregulation in COVID-19 patients with severe respiratory failure. *Cell Host & Microbe* 2020. [DOI: S1931-3128(20)30236-5]

Gietema 2020 *{published data only}*

Gietema HA, Zelis N, Nobel JM, Lambriks LJ, Van Alphen LB, Oude Lashof AM, et al. CT in relation to RT-PCR in diagnosing COVID-19 in the Netherlands: a prospective study. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.22.20070441]

Gonzalez Gonzalez 2020a *{published data only}*

Gonzalez-Gonzalez E, Lara-Mayorga IM, Garcia-Rubio A, Garciamendez-Mijares CE, Guerra-Alvarez GE, Garcia-Martinez G, et al. Scaling diagnostics in times of COVID-19: rapid prototyping of 3D-printed water circulators for loop-mediated isothermal amplification (LAMP) and detection of SARS-CoV-2 virus. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.09.20058651]

Gonzalez Gonzalez 2020b *{published data only}*

Gonzalez-Gonzalez E, Trujillo-de Santiago G, Lara-Mayorga IM, Martinez-Chapa SO, Alvarez MM. Portable and accurate diagnostics for COVID-19: combined use of the miniPCR thermocycler and a well-plate reader for SARS-Co2 virus detection. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.03.20052860]

Guan 2020 *{published data only}*

Guan WD, Chen LP, Ye F, Ye D, Wu SG, Zhou HX, et al. High-throughput sequencing for confirmation of suspected 2019-nCoV infection identified by fluorescence quantitative polymerase chain reaction. *Chinese Medical Journal* 2020. [DOI: 10.1097/cm9.0000000000000792 10.1097/CM9.0000000000000792.]

Guo 2020b *{published data only}*

Guo L, Sun X, Wang X, Liang C, Jiang H, Gao Q, et al. SARS-CoV-2 detection with CRISPR diagnostics. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.10.023358]

Guo 2020c *{published data only}*

Guo X, Guo Z, Duan C, Chen Z, Wang G, Lu Y, et al. Long-term persistence of IgG antibodies in SARS-CoV infected healthcare workers. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.12.20021386]

Han 2020 *{published data only}*

Han R, Huang L, Jiang H, Dong J, Peng H, Zhang D. Early clinical and CT manifestations of coronavirus disease 2019 (COVID-19) pneumonia. *American Journal of Roentgenology* 2020:1-6. [DOI: 10.2214/ajr.20.22961 10.2214/AJR.20.22961.]

Hao 2020 *{published data only}*

Hao W, Li M. Clinical diagnostic value of CT imaging in COVID-19 with multiple negative RT-PCR testing. *Travel Medicine and Infectious Disease* 2020:101627. [DOI: 10.1016/j.tmaid.2020.101627]

Hass 2020 *{published data only}*

Hass K, Bao M, He Q, Park M, Qin P, Du K. Integrated micropillar polydimethylsiloxane accurate CRISPR detection (IMPACT) system for rapid viral DNA sensing. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.17.994137]

Hirotsu 2020 *{published data only}*

Hirotsu Y, Mochizuki H, Omata M. Double- quencher probes improved the detection sensitivity of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) by One-Step RT-PCR. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.17.20037903]

Hogan 2020 *{published data only}*

Hogan CA, Sahoo MK, Pinsky BA. Sample pooling as a strategy to detect community transmission of SARS-CoV-2. *JAMA* 2020. [DOI: 10.1001/jama.2020.5445]

Holland 2020 *{published data only}*

Holland M, Negron D, Mitchell S, Dellinger N, Ivancich M, Barrus T, et al. BioLaboro: a bioinformatics system for detecting molecular assay signature erosion and designing new assays in response to emerging and reemerging pathogens. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.08.031963]

Hu 2020b *{published data only}*

Hu F, Chen F, Wang Y, Xu T, Tang X, Li F. Failed detection of the full-length genome of SARS-CoV-2 by ultra-deep sequencing from the recovered and discharged patients retested viral PCR positive. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.27.20043299]

Hu 2020c *{published data only}*

Hu, X, An, T, Situ, B, Hu, Y, Ou, Z, Li, Q, et al. Heat inactivation of serum interferes with the immunoanalysis of antibodies to SARS-CoV-2. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.12.20034231]

Hu 2020d *{published data only}*

Hu Z, Song C, Xu C, Jin G, Chen Y, Xu X, et al. Clinical characteristics of 24 asymptomatic infections with COVID-19 screened among close contacts in Nanjing, China. *Science China. Life Sciences* 2020 Mar 4 [Epub ahead of print]. [DOI: 10.1007/s11427-020-1661-4]

Huang 2020a *{published data only}*

Huang WH, Teng LC, Yeh TK, Chen YJ, Lo WJ, Wu MJ, et al. 2019 novel coronavirus disease (COVID-19) in Taiwan: reports of two cases from Wuhan, China. *Journal of Microbiology, Immunology and Infection* 2020;**53**(3):481-4. [DOI: 10.1016/j.jmii.2020.02.009 10.1016/j.jmii.2020.02.009.]

Jenkins 2020 *{published data only}*

Jenkins C, Orsburn B. In silico approach to accelerate the development of mass spectrometry-based proteomics methods

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

for detection of viral proteins: application to COVID-19. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.08.980383]

Jiang 2020a *{published data only}*

Jiang DM. Recurrent PCR positivity after hospital discharge of people with coronavirus disease 2019 (COVID-19). *Journal of Infection* 2020. [DOI: S0163-4453(20)30152-3]

Jiang 2020b *{published data only}*

Jiang HW, Li Y, Zhang HN, Wang W, Men D, Yang X, et al. Global profiling of SARS-CoV-2 specific IgG/ IgM responses of convalescents using a proteome microarray. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.20.20039495]

Jung 2020 *{published data only}*

Jung YJ, Park GS, Moon JH, Ku K, Beak SH, Kim S, et al. Comparative analysis of primer-probe sets for the laboratory confirmation of SARS-CoV-2. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.25.964775]

Khan 2020 *{published data only}*

Khan S, Nakajima R, Jain A, de Assis RR, Jasinskas A, Obiero JM, et al. Analysis of serologic cross-reactivity between common human coronaviruses and SARS-CoV-2 using coronavirus antigen microarray. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.24.006544]

Kim 2019 *{published data only}*

Kim JH, Kang M, Park E, Chung DR, Kim J, Hwang ES. A simple and multiplex loop-mediated isothermal amplification (LAMP) assay for rapid detection of SARS-CoV. *BioChip Journal* 2019;**13**(4):341-51. [DOI: 10.1007/s13206-019-3404-3]

Kong 2020 *{published data only}*

Kong WH, Li Y, Peng MW, Kong DG, Yang XB, Wang L, Liu MQ. SARS-CoV-2 detection in patients with influenza-like illness. *Nature Microbiology* 2020;**5**:675-8. [DOI: 10.1038/s41564-020-0713-1]

Konrad 2020 *{published data only}*

Konrad R, Eberle U, Dangel A, Treis B, Berger A, Bengs K, et al. Rapid establishment of laboratory diagnostics for the novel coronavirus SARS-CoV-2 in Bavaria, Germany, February 2020. *Eurosurveillance* 2020;**25**(9). [DOI: 10.2807/1560-7917.Es.2020.25.9.2000173 10.2807/1560-7917.ES.2020.25.9.2000173.]

Kurstjens 2020 *{published data only}*

Kurstjens S, Van der Horst A, Herpers R, Geerits MW, Kluiters-de Hingh YC, Göttgens EL, et al. Rapid identification of SARS-CoV-2-infected patients at the emergency department using routine testing. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.20.20067512]

Lamb 2020 *{published data only}*

Lamb LE, Bartolone SN, Ward E, Chancellor MB. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.19.20025155]

Lan 2020 *{published data only}*

Lan L, Xu D, Ye G, Xia C, Wang S, Li Y, et al. Positive RT-PCR test results in patients recovered from COVID-19. *JAMA* 2020. [DOI: 10.1001/jama.2020.2783 10.1001/jama.2020.2783.]

Lechien 2020 *{published data only}*

Lechien J, Cabaraux P, Chiesa-Estomba C, Khalife M, Plzak J, Hans S, et al. Objective olfactory testing in patients presenting with sudden onset olfactory dysfunction as the first manifestation of confirmed COVID-19 infection. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.15.20066472]

Lei 2020 *{published data only}*

Lei Z, Cao H, Jie Y, Huang Z, Guo X, Chen J, et al. A cross-sectional comparison of epidemiological and clinical features of patients with coronavirus disease (COVID-19) in Wuhan and outside Wuhan, China. *Travel Medicine and Infectious Disease* 2020:101664. [DOI: S1477-8939(20)30132-0]

Li 2020c *{published data only}*

Li Y, Hu Y, Zhang X, Yu Y, Li B, Wu J, et al. Follow-up testing of viral nucleic acid in discharged patients with moderate type of 2019 coronavirus disease (COVID-19). *Zhejiang Da Xue Xue Bao Yi Xue Ban* 2020;**49**(1):0. [DOI: 10.3785/j.issn.1008-9292.2020.03.11]

Li 2020d *{published data only}*

Li C, Debruyne D, Spencer J, Kapoor V, Liu LY, Zhang B, et al. High sensitivity detection of SARS-CoV-2 using multiplex PCR and a multiplex-PCR-based metagenomic method. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.12.988246]

Li 2020e *{published data only}*

Li Y, Xia L. Coronavirus disease 2019 (COVID-19): role of chest CT in diagnosis and management. *American Journal of Roentgenology* 2020:1-7. [DOI: 10.2214/ajr.20.22954 10.2214/AJR.20.22954.]

Li 2020f *{published data only}*

Li D, Wang D, Dong J, Wang N, Huang H, Xu H, et al. False-negative results of real-time reverse-transcriptase polymerase chain reaction for severe acute respiratory syndrome coronavirus 2: role of deep-learning-based CT diagnosis and insights from two cases. *Korean Journal of Radiology* 2020. [DOI: 10.3348/kjr.2020.0146 10.3348/kjr.2020.0146.]

Li 2020g *{published data only}*

Li YY, Wang WN, Lei Y, Zhang B, Yang J, Hu JW, et al. Comparison of the clinical characteristics between RNA positive and negative patients clinically diagnosed with 2019 novel coronavirus pneumonia. *Zhonghua Jie He He Hu Xi Za Zhi* 2020;**43**(0):E023. [DOI: 10.3760/cma.j.cn112147-20200214-00095 10.3760/cma.j.cn112147-20200214-00095.]

Liang 2020a *{published data only}*

Liang Y, Liang J, Zhou Q, Li X, Lin F, Deng Z, et al. Prevalence and clinical features of 2019 novel coronavirus disease (COVID-19) in the fever clinic of a teaching hospital in Beijing: a single-center, retrospective study. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.25.20027763]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liang 2020b *{published data only}*

Liang C, Cao J, Liu Z, Ge F, Cang J, Miao C, et al. Positive RT-PCR test results after consecutively negative results in patients with COVID-19. *Infectious Diseases* 2020;**52**(7):517-9. [DOI: 10.1080/23744235.2020.1755447]

Ling 2020 *{published data only}*

Ling Y, Xu SB, Lin YX, Tian D, Zhu ZQ, Dai FH, et al. Persistence and clearance of viral RNA in 2019 novel coronavirus disease rehabilitation patients. *Chinese Medical Journal* 2020. [DOI: 10.1097/cm9.0000000000000774 10.1097/CM9.0000000000000774.]

Liu 2020e *{published data only}*

Liu J, Li S, Liu J, Liang B, Wang X, Wang H, et al. Longitudinal characteristics of lymphocyte responses and cytokine profiles in the peripheral blood of SARS-CoV-2 infected patients. *EbioMedicine* 2020;**55**:102763. [DOI: 10.1016/j.ebiom.2020.102763]

Liu 2020f *{published data only}*

Liu W, Tao ZW, Lei W, Ming-Li Y, Kui L, Ling Z, et al. Analysis of factors associated with disease outcomes in hospitalized patients with 2019 novel coronavirus disease. *Chinese Medical Journal* 2020. [DOI: 10.1097/cm9.0000000000000775 10.1097/CM9.0000000000000775.]

Liu 2020g *{published data only}*

Liu R, Han H, Liu F, Lv Z, Wu K, Liu Y, et al. Positive rate of RT-PCR detection of SARS-CoV-2 infection in 4880 cases from one hospital in Wuhan, China, from Jan to Feb 2020. *Clinica Chimica Acta; International Journal of Clinical Chemistry* 2020;**505**:172-5. [DOI: 10.1016/j.cca.2020.03.009 10.1016/j.cca.2020.03.009.]

Liu 2020h *{published data only}*

Liu J, Xiao Y, Shen Y, Shi C, Chen Y, Shi P, et al. Detection of SARS-CoV-2 by RT-PCR in anal from patients who have recovered from coronavirus disease 2019. *Journal of Medical Virology* 2020. [DOI: 10.1002/jmv.25875]

Lo 2020 *{published data only}*

Lo IL, Lio CF, Cheong HH, Lei CI, Cheong TH, Zhong X, et al. Evaluation of SARS-CoV-2 RNA shedding in clinical specimens and clinical characteristics of 10 patients with COVID-19 in Macau. *International Journal of Biological Sciences* 2020;**16**(10):1698-707. [DOI: 10.7150/ijbs.45357]

Lopez-Rincon 2020 *{published data only}*

Lopez-Rincon A, Tonda A, Mendoza-Maldonado L, Claassen E, Garssen J, Kraneveld AD. Accurate identification of SARS-CoV-2 from viral genome sequences using deep learning. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.13.990242]

Lu 2020 *{published data only}*

Lu R, Wu X, Wan Z, Li Y, Zuo L, Qin J, et al. Development of a novel reverse transcription loop-mediated isothermal amplification method for rapid detection of SARS-CoV-2. *Virologica Sinica* 2020. [DOI: 10.1007/s12250-020-00218-1]

Ma 2020b *{published data only}*

Ma SY, Luo YM, Hu TY, You ZC, Sun JG, Yu SY, et al. Clinical application effect of modified nasopharyngeal swab sampling for 2019 novel coronavirus nucleic acid detection. *Zhonghua Shao Shang Za Zhi* 2020;**36**(0):E009. [DOI: 10.3760/cma.j.cn501120-20200312-00153]

Mahari 2020 *{published data only}*

Mahari S, Roberts A, Shahdeo D, Gandhi S. eCovSens-ultrasensitive novel in-house built printed circuit board based electrochemical device for rapid detection of nCOVID-19. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.24.059204]

Mardani 2020 *{published data only}*

Mardani R, Ahmadi Vasmehjani A, Zali F, Gholami A, Mousavi Nasab SD, Kaghazian H, et al. Laboratory parameters in detection of COVID-19 patients with positive RT-PCR; a diagnostic accuracy study. *Archives of Academic Emergency Medicine* 2020;**8**(1):e43.

Marzinotto 2020 *{published data only}*

Marzinotto S, Mio C, Cifu A, Verardo R, Pipan C, Schneider C, et al. A streamlined approach to rapidly detect SARS-CoV-2 infection, avoiding RNA extraction. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.06.20054114]

McKay 2020 *{published data only}*

McKay PF, Hu K, Blakney AK, Samnuan K, Bouton CR, Rogers P, et al. Self-amplifying RNA SARS-CoV-2 lipid nanoparticle vaccine induces equivalent preclinical antibody titers and viral neutralization to recovered COVID-19 patients. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.22.055608]

McRae 2020 *{published data only}*

McRae MP, Simmons GW, Christodoulides NJ, Lu Z, Kang SK, Fenyo D, et al. Clinical decision support tool and rapid point-of-care platform for determining disease severity in patients with COVID-19. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.16.20068411]

Mei 2020 *{published data only}*

Mei X, Lee HC, Diao K, Huang M, Lin B, Liu C, et al. Artificial intelligence for rapid identification of the coronavirus disease 2019 (COVID-19). *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.12.20062661]

Meng 2020 *{published data only}*

Meng Z, Wang M, Song H, Guo S, Zhou Y, Li W, et al. Development and utilization of an intelligent application for aiding COVID-19 diagnosis. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.18.20035816]

Mercurio 2020 *{published data only}*

Mercurio I, Tragni V, Busto F, De Grassi A, Pierri CL. Protein structure analysis of the interactions between SARS-CoV-2 spike protein and the human ACE2 receptor: from conformational changes to novel neutralizing antibodies. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.17.046185]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Metsky 2020 *{published data only}*

Metsky HC, Freije CA, Kosoko-Thoroddsen TS, Sabeti PC, Myhrvold C. CRISPR-based COVID-19 surveillance using a genomically-comprehensive machine learning approach. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.26.967026]

Nelson 2020 *{published data only}*

Nelson AC, Auch B, Schomaker M, Gohl DM, Grady P, Johnson D, et al. Analytical validation of a COVID-19 qRT-PCR detection assay using a 384-well format and three extraction methods. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.02.022186]

Nemati 2020 *{published data only}*

Nemati S, Najari HR, Eftekharzadeh A, Kazemifar AM, Qandian A, Fattahi P, et al. Association between rRT-PCR test results upon admission and outcome in hospitalized chest CT-Positive COVID-19 patients; a provincial retrospective cohort with active follow-up. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.21.20074641]

Nie 2020 *{published data only}*

Nie J, Li Q, Wu J, Zhao C, Hao H, Liu H, et al. Establishment and validation of a pseudovirus neutralization assay for SARS-CoV-2. *Emerging Microbes and Infections* 2020;**9**(1):680-6. [DOI: 10.1080/22221751.2020.1743767 10.1080/22221751.2020.1743767.]

Nunez Bajo 2020 *{published data only}*

Nunez-Bajo E, Kasimatis M, Cotur Y, Asfour T, Collins A, Tanriverdi U, et al. Ultra-low-cost integrated silicon-based transducer for on-site, genetic detection of pathogens. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.23.002931]

Okba 2020b *{published data only}*

Okba N, Muller MA, Li W, Wang C, GeurtsvanKessel CH, Corman VM, et al. SARS-CoV-2 specific antibody responses in COVID-19 patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.18.20038059]

Paden 2020 *{published data only}*

Paden CR, Tao Y, Queen K, Zhang J, Li Y, Uehara A, et al. Rapid, sensitive, full genome sequencing of severe acute respiratory syndrome virus coronavirus 2 (SARS-CoV-2). *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.22.055897]

Pan 2020b *{published data only}*

Pan Y, Yu X, Du X, Li Q, Li X, Qin T, et al. Epidemiological and clinical characteristics of 26 asymptomatic SARS-CoV-2 carriers. *Journal of Infectious Diseases* 2020. [DOI: jiaa205]

Pan 2020c *{published data only}*

Pan Y, Zhang D, Yang P, Poon LL, Wang Q. Viral load of SARS-CoV-2 in clinical samples. *Lancet Infectious Diseases* 2020. [DOI: 10.1016/S1473-3099(20)30113-4]

Pan 2020d *{published data only}*

Pan F, Ye T, Sun P, Gui S, Liang B, Li L, et al. Time course of lung changes on chest CT during recovery from 2019 novel coronavirus (COVID-19) pneumonia. *Radiology* 2020:200370. [DOI: 10.1148/radiol.2020200370 10.1148/radiol.2020200370.]

Pan 2020e *{published data only}*

Pan Y, Long L, Zhang D, Yan T, Cui S, Yang P, et al. Potential false-negative nucleic acid testing results for severe acute respiratory syndrome coronavirus 2 from thermal inactivation of samples with low viral loads. *Clinical Chemistry* 2020. [DOI: hvaa091]

Paradiso 2020b *{published data only}*

Paradiso AV, De Summa S, Silvestris N, Tommasi S, Tufaro A, De Palma G, et al. Rapid serological tests have a role in asymptomatic health workers COVID-19 screening. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.15.20057786]

Park 2020 *{published data only}*

* Park GS, Ku K, Baek SH, Kim SJ, Kim SI, Kim BT, et al. Development of reverse transcription loop-mediated isothermal amplification (RT-LAMP) assays targeting SARS-CoV-2. *Journal of Molecular Diagnostics* 2020;**22**(6):729-35. [DOI: 10.1016/j.jmoldx.2020.03.006]

Park GS, Ku K, Beak SH, Kim SJ, Kim SI, Kim BT, et al. Development of reverse transcription loop-mediated isothermal amplification (RT-LAMP) assays targeting SARS-CoV-2. *bioRxiv [Preprint]* 2020.

Peng 2020 *{published data only}*

Peng L, Liu J, Xu W, Luo Q, Deng K, Lin B, et al. 2019 novel coronavirus can be detected in urine, blood, anal swabs and oropharyngeal swabs samples. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.21.20026179]

Pfefferle 2020 *{published data only}*

Pfefferle S, Reucher S, Nörz D, Lütgehetmann M. Evaluation of a quantitative RT-PCR assay for the detection of the emerging coronavirus SARS-CoV-2 using a high throughput system. *Eurosurveillance* 2020;**25**(9). [DOI: 10.2807/1560-7917.ES.2020.25.9.2000152]

Rauch 2020 *{published data only}*

Rauch JN, Valois E, Solley SC, Braig F, Lach RS, Baxter NJ, et al. A scalable, easy-to-deploy, protocol for Cas13-based detection of SARS-CoV-2 genetic material. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.20.052159]

Scallan 2020 *{published data only}*

Scallan MF, Dempsey C, MacSharry J, O'Callaghan I, O'Connor PM, Hogan CP, et al. Validation of a lysis buffer containing 4 M guanidinium thiocyanate (GITC)/ Triton X-100 for extraction of SARS-CoV-2 RNA for COVID-19 testing: comparison of formulated lysis buffers containing 4 to 6 M GITC, Roche external lysis buffer and Qiagen RTL lysis buffer. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.05.026435]

Seo 2020 *{published data only}*

Seo G, Lee G, Kim MJ, Baek SH, Choi M, Ku KB, et al. Rapid detection of COVID-19 causative virus (SARS-CoV-2) in human nasopharyngeal swab specimens using field-effect transistor-based biosensor. *ACS Nano* 2020. [DOI: 10.1021/acsnano.0c02823]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Shental 2020 *{published data only}*

Shental N, Levy S, Skorniakov S, Wuvshet V, Shemer-Avni Y, Porgador A, et al. Efficient high throughput SARS-CoV-2 testing to detect asymptomatic carriers. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.14.20064618]

Shi 2020 *{published data only}*

Shi Y, Wang X, Liu G, Zhu Q, Wang J, Yu H, et al. A quickly, effectively screening process of novel corona virus disease 2019 (COVID-19) in children in Shanghai, China. *Annals of Translational Medicine* 2020;**8**(5). [DOI: 10.21037/atm.2020.03.22]

Shirato 2020 *{published data only}*

Shirato K, Nao N, Katano H, Takayama I, Saito S, Kato F, et al. Development of genetic diagnostic methods for novel coronavirus 2019 (nCoV-2019) in Japan. *Japanese Journal of Infectious Diseases* 2020. [DOI: 10.7883/yoken.JJID.2020.061 10.7883/yoken.JJID.2020.061.]

Song 2020 *{published data only}*

Song C, Wang Y, Li W, Hu B, Chen G, Xia P, et al. Detection of 2019 novel coronavirus in semen and testicular biopsy specimen of COVID-19 patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.31.20042333]

Su 2020 *{published data only}*

Su L, Ma X, Yu H, Zhang Z, Bian P, Han Y, et al. The different clinical characteristics of corona virus disease cases between children and their families in China - the character of children with COVID-19. *Emerging Microbes and Infections* 2020;**9**(1):707-13. [DOI: 10.1080/22221751.2020.1744483 10.1080/22221751.2020.1744483.]

Sun 2020a *{published data only}*

Sun X, Zhang X, Chen X, Chen L, Deng C, Zou X, et al. The infection evidence of SARS-COV-2 in ocular surface: a single-center cross-sectional study. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.26.20027938]

Sun 2020b *{published data only}*

Sun Y, Koh V, Marimuthu K, Ng OT, Young B, Vasoo S, et al. Epidemiological and clinical predictors of COVID-19. *Clinical Infectious Diseases* 2020. [DOI: 10.1093/cid/ciaa322 10.1093/cid/ciaa322.]

Sun 2020c *{published data only}*

Sun F, Ganguli A, Nguyen J, Brisbin R, Shanmugam K, Hirschberg DL, et al. Smartphone-based multiplex 30-minute nucleic acid test of live virus from nasal swab extract. *Lab on a Chip* 2020. [DOI: 10.1039/d0lc00304b]

Tagarro 2020 *{published data only}*

Tagarro A, Epalza C, Santos M, Sanz-Santaeufemia FJ, Otheo E, Moraleda C, et al. Screening and severity of coronavirus disease 2019 (COVID-19) in children in Madrid, Spain. *JAMA Pediatrics* 2020. [DOI: 10.1001/jamapediatrics.2020.1346]

Tan 2020a *{published data only}*

Tan W, Lu Y, Zhang J, Wang J, Dan Y, Tan Z, et al. Viral kinetics and antibody responses in patients with COVID-19. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.24.20042382]

Tan 2020b *{published data only}*

Tan X, Huang J, Zhao F, Zhou Y, Li JQ, Wang XY. Clinical features of children with SARS-CoV-2 infection: an analysis of 13 cases from Changsha, China. *Zhongguo Dang Dai Er Ke Za Zhi* 2020;**22**(4):294-8. [DOI: 10.7499/j.issn.1008-8830.2003199]

Tan 2020c *{published data only}*

Tan X, Lin C, Zhang J, Khaing Oo MK, Fan X. Rapid and quantitative detection of COVID-19 markers in micro-liter sized samples. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.20.052233]

Toptan 2020 *{published data only}*

Toptan T, Hoehl S, Westhaus S, Bojkova D, Berger A, Rotter B, et al. Optimized qRT-PCR approach for the detection of intra- and extracellular SARS-CoV-2 RNAs. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.20.052258]

Tsang 2003 *{published data only}*

Tsang OT, Chau TN, Choi KW, Tso EY, Lim W, Chiu MC, et al. Coronavirus-positive nasopharyngeal aspirate as predictor for severe acute respiratory syndrome mortality. *Emerging Infectious Diseases* 2003;**9**(11):1381-7. [DOI: 10.3201/eid0911.030400 10.3201/eid0911.030400.]

Vermeiren 2020 *{published data only}*

Vermeiren C, Marchand-Senécal X, Sheldrake E, Bulir D, Smieja M, Chong S, et al. Comparison of Copan Eswab and FLOQswab for COVID-19 PCR diagnosis: working around a supply shortage. *Journal of Clinical Microbiology* 2020. [DOI: 10.1128/JCM.00669-20]

Viehweger 2020 *{published data only}*

Viehweger A, Kühnl F, Brandt C, König B. Increased PCR screening capacity using a multi-replicate pooling scheme. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.16.20067603]

Vogels 2020 *{published data only}*

Vogels CB, Brito AF, Wyllie AL, Fauver JR, Ott IM, Kalinich CC, et al. Analytical sensitivity and efficiency comparisons of SARS-COV-2 qRT-PCR assays. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.30.20048108]

Waghmare 2020 *{published data only}*

Waghmare A, Krantz EM, Baral S, Vasquez E, Loeffelholz T, Chung EL, et al. Reliability of self-sampling for accurate assessment of respiratory virus viral and immunologic kinetics. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.03.20051706]

Wang 2020b *{published data only}*

Wang F, Hou H, Luo Y, Tang G, Wu S, Huang M, et al. The laboratory tests and host immunity of COVID-19 patients with different severity of illness. *JCI Insight* 2020. [DOI: 10.1172/jci.insight.137799]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wang 2020c *{published data only}*

Wang Z, Li H, Li J, Yang C, Guo X, Hu Z, et al. Elevated serum IgM levels indicate poor outcome in patients with coronavirus disease 2019 pneumonia: a retrospective case-control study. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.22.20041285]

Wang 2020d *{published data only}*

Wang X, Guo X, Xin Q, Chu Y, Li J, Pan Y, et al. Neutralizing antibodies responses to SARS-CoV-2 in COVID-19 inpatients and convalescent patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.15.20065623]

Wang 2020e *{published data only}*

Wang B, Wang L, Kong X, Geng J, Xiao D, Ma C. Long-term co-existence of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) with antibody response in non-severe coronavirus disease 2019 (COVID-19) patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.13.20040980]

Wang 2020f *{published data only}*

Wang X, Yao H, Xu X, Zhang P, Zhang M, Shao J, et al. Limits of detection of six approved RT-PCR kits for the novel SARS-coronavirus-2 (SARS-CoV-2). *Clinical Chemistry* 2020. [DOI: 10.1093/clinchem/hvaa099]

Wang 2020g *{published data only}*

Wang XF, Yuan J, Zheng YJ, Chen J, Bao YM, Wang YR, et al. Retracted: Clinical and epidemiological characteristics of 34 children with 2019 novel coronavirus infection in Shenzhen. *Zhonghua Er Ke Za Zhi* 2020;**58**(0):E008. [DOI: 10.3760/cma.j.issn.0578-1310.2020.0008 10.3760/cma.j.issn.0578-1310.2020.0008.]

Wang 2020h *{published data only}*

Wang QX, Zeng XH, Zheng SL. The nucleic acid test of induced sputum should be used for estimation of patients cure with 2019-nCov. *European Review for Medical and Pharmacological Sciences* 2020;**24**(7):3437. [DOI: 20795]

Wang 2020i *{published data only}*

Wang Z, Weng J, Li Z, Hou R, Zhou L, Ye H, et al. Development and validation of a diagnostic nomogram to predict COVID-19 pneumonia. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.03.20052068]

Wee 2020 *{published data only}*

Wee SK, Sivalingam SP, Yap EP. Rapid direct nucleic acid amplification test without RNA extraction for SARS-CoV-2 using a portable PCR thermocycler. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.17.042366]

Weiss 2020 *{published data only}*

Weiss S, Klingler J, Hioe C, Amanat F, Baine I, Kojic EM, et al. A high through-put assay for circulating antibodies directed against the S protein of severe acute respiratory syndrome corona virus 2. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.14.20059501]

Woelfel 2020 *{published data only}*

Woelfel R, Corman VM, Guggemos W, Seilmaier M, Zange S, Mueller MA, et al. Clinical presentation and virological assessment of hospitalized cases of coronavirus disease 2019 in a travel-associated transmission cluster. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.05.20030502]

Won 2020 *{published data only}*

Won J, Lee S, Park M, Kim TY, Park MG, Choi BY, et al. Development of a laboratory-safe and low-cost detection protocol for SARS-CoV-2 of the coronavirus disease 2019 (COVID-19). *Experimental Neurobiology* 2020. [DOI: 10.5607/en20009 10.5607/en20009.]

Woo 2020 *{published data only}*

Woo CH, Jang S, Shin G, Jung GY, Lee JW. Sensitive one-step isothermal detection of pathogen-derived RNAs. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.05.20031971]

Wu 2020a *{published data only}*

Wu F, Wang A, Liu M, Wang Q, Chen J, Xia S, et al. Neutralizing antibody responses to SARS-CoV-2 in a COVID-19 recovered patient cohort and their implications. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.30.20047365]

Wu 2020b *{published data only}*

Wu Q, Xing Y, Shi L, Li W, Gao Y, Pan S, et al. Epidemiological and clinical characteristics of children with coronavirus disease 2019. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.19.20027078]

Wu 2020c *{published data only}*

Wu X, Fu B, Chen L, Feng Y. Serological tests facilitate identification of asymptomatic SARS-CoV-2 infection in Wuhan, China. *Journal of Medical Virology* 2020. [DOI: 10.1002/jmv.25904]

Xia 2020a *{published data only}*

Xia J, Tong J, Liu M, Shen Y, Guo D. Evaluation of coronavirus in tears and conjunctival secretions of patients with SARS-CoV-2 infection. *Journal of Medical Virology* 2020. [DOI: 10.1002/jmv.25725 10.1002/jmv.25725.]

Xia 2020b *{published data only}*

Xia XY, Wu J, Liu HL, Xia H, Jia B, Huang WX. Epidemiological and initial clinical characteristics of patients with family aggregation of COVID-19. *Journal of Clinical Virology* 2020;**127**:104360. [DOI: 10.1016/j.jcv.2020.104360]

Xie 2020b *{published data only}*

Xie X, Zhong Z, Zhao W, Zheng C, Wang F, Liu J. Chest CT for typical 2019-nCoV pneumonia: relationship to negative RT-PCR testing. *Radiology* 2020:200343. [DOI: 10.1148/radiol.2020200343 10.1148/radiol.2020200343]

Xie 2020c *{published data only}*

Xie C, Lu J, Wu D, Zhang L, Zhao H, Rao B, et al. False negative rate of COVID-19 is eliminated by using nasal swab test. *Travel Medicine and Infectious Disease* 2020. [DOI: S1477-8939(20)30136-8]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xing 2020a *{published data only}*

Xing Y, Ni W, Wu Q, Li W, Li G, Wang W, et al. Dynamics of faecal SARS-CoV-2 in infected children during the convalescent phase. *Journal of Infection* 2020. [DOI: S0163-4453(20)30177-8]

Xing 2020b *{published data only}*

Xing Y, Ni W, Wu Q, Li W, Li G, Tong J, et al. Prolonged presence of SARS-CoV-2 in feces of pediatric patients during the convalescent phase. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.11.20033159]

Xu 2020b *{published data only}*

Xu SP, Kuang D, Hu Y, Liu C, Duan YQ, Wang GP. Detection of 2019-nCoV in the pathological paraffin embedded tissue. *Zhonghua Bing Li Xue Za Zhi* 2020;**49**(0):E004. [DOI: 10.3760/cma.j.cn112151.20200219.00001 10.3760/cma.j.cn112151.20200219.00001.]

Xu 2020c *{published data only}*

Xu Y, Xiao M, Liu X, Xu S, Du T, Xu J, et al. Significance of serology testing to assist timely diagnosis of SARS-CoV-2 infections: implication from a family cluster. *Emerging Microbes and Infection* 2020:01/Dec. [DOI: 10.1080/22221751.2020.1752610]

Xu 2020d *{published data only}*

Xu K, Chen Y, Yuan J, Yi P, Ding C, Wu W, et al. Factors associated with prolonged viral RNA shedding in patients with COVID-19. *Clinical Infectious Diseases* 2020. [DOI: ciaa351]

Yan 2020 *{published data only}*

Yan S, Song X, Lin F, Zhu H, Wang X, Li M, et al. Clinical characteristics of coronavirus disease 2019 in Hainan, China. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.19.20038539]

Yang 2020a *{published data only}*

Yang Y, Yang M, Shen C, Wang F, Yuan J, Li J, et al. Evaluating the accuracy of different respiratory specimens in the laboratory diagnosis and monitoring the viral shedding of 2019-nCoV infections. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.11.20021493]

Yang 2020b *{published data only}*

Yang P, Shao FL, Wang GJ. Clinical observation on increasing the positive rate of novel coronavirus nucleic acid tests by sputum excretion induced by nebulizer therapy. *Zhonghua Jie He He Hu Xi Za Zhi* 2020;**43**(4):335-6. [DOI: 10.3760/cma.j.cn112147-20200212-00076]

Yelin 2020 *{published data only}*

Yelin I, Aharony N, Shaer-Tamar E, Argoetti A, Messer E, Berenbaum D, et al. Evaluation of COVID-19 RT-qPCR test in multi-sample pools. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.26.20039438]

Yuan 2020 *{published data only}*

Yuan J, Zou R, Zeng L, Kou S, Lan J, Li X, et al. The correlation between viral clearance and biochemical outcomes of 94 COVID-19 infected discharged patients. *Inflammation Research* 2020. [DOI: 10.1007/s00011-020-01342-0]

Yun 2020 *{published data only}*

Yun H, Sun Z, Wu J, Tang A, Hu M, Xiang Z. Laboratory data analysis of novel coronavirus (COVID-19) screening in 2510 patients. *Clinica Chimica Acta* 2020. [DOI: S0009-8981(20)30173-X]

Zeng 2020b *{published data only}*

Zeng F, Dai C, Cai P, Wang J, Xu L, Li J, et al. A comparison study of SARS-CoV-2 IgG antibody between male and female COVID-19 patients: a possible reason underlying different outcome between gender. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.26.20040709]

Zhang 2020e *{published data only}*

Zhang X, Wu X, Wang D, Lu M, Hou X, Wang H, et al. Proteome-wide analysis of differentially-expressed SARS-CoV-2 antibodies in early COVID-19 infection. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.14.20064535]

Zhang 2020f *{published data only}*

Zhang G, Zhang J, Wang B, Zhu X, Wang Q, Qiu S. Analysis of clinical characteristics and laboratory findings of 95 cases of 2019 novel coronavirus pneumonia in Wuhan, China: a retrospective analysis. *Respiratory Research* 2020;**21**(1):74. [DOI: 10.1186/s12931-020-01338-8]

Zhang 2020g *{published data only}*

Zhang L, Pang R, Xue X, Bao J, Ye S, Dai Y, et al. Anti-SARS-CoV-2 virus antibody levels in convalescent plasma of six donors who have recovered from COVID-19. *Aging (Albany NY)* 2020;**12**. [DOI: 10.18632/aging.103102]

Zhang 2020h *{published data only}*

Zhang N, Gong Y, Meng F, Bi Y, Yang P, Wang F. Virus shedding patterns in nasopharyngeal and fecal specimens of COVID-19 patients. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.28.20043059]

Zhao 2020c *{published data only}*

Zhao D, Yao F, Wang L, Zheng L, Gao Y, Ye J, et al. A comparative study on the clinical features of COVID-19 pneumonia to other pneumonias. *Clinical Infectious Diseases* 2020. [DOI: 10.1093/cid/ciaa247 10.1093/cid/ciaa247]

Zhao 2020d *{published data only}*

Zhao Z, Cui H, Song W, Ru X, Zhou W, Yu X. A simple magnetic nanoparticles-based viral RNA extraction method for efficient detection of SARS-CoV-2. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.02.22.961268]

Zhifeng 2020 *{published data only}*

Zhifeng J, Feng A, Li T. Consistency analysis of COVID-19 nucleic acid tests and the changes of lung CT. *Journal of Clinical Virology* 2020;**127**:104359. [DOI: 10.1016/j.jcv.2020.104359]

Zhou 2020 *{published data only}*

Zhou J, Bai Z, Liu X, Guo Y, Jiang N, Li X, et al. Flocked swab might be one main reason causing the high false-negative rate in COVID-19 screening----the advantages of a novel silicone swab. *bioRxiv [Preprint]* 2020. [DOI: 10.1101/2020.03.29.014415]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhuang 2020 *{published data only}*

Zhuang GH, Shen MW, Zeng LX, Mi BB, Chen FY, Liu WJ, et al. Potential false-positive rate among the 'asymptomatic infected individuals' in close contacts of COVID-19 patients. *Zhonghua Liu Xing Bing Xue Za Zhi* 2020;**41**(4):485-8. [DOI: 10.3760/cma.j.cn112338-20200221-00144 10.3760/cma.j.cn112338-20200221-00144.]

References to studies awaiting assessment

Li 2020b *{published data only}*

Li H, Li Y, Zhang Z, Lu Z, Wang Y, Lin G, et al. Establishment and clinical performance evaluation of 2019 novel coronavirus antibody colloidal gold detection method. *Chinese Journal of Infectious Diseases* 2020.

Thompson 2020 *{published data only}*

Thompson C, Grayson N, Paton R, Lourenco J, Penman B, Lee LN, et al. Neutralising antibodies to SARS coronavirus 2 in Scottish blood donors - a pilot study of the value of serology to determine population exposure. *medRxiv [Preprint]* 2020. [DOI: 10.1101/2020.04.13.20060467]

Xiong 2020 *{published data only}*

Xiong Z, Fu L, Zhou H, Liu JK, Wang AM, Huang, Y, et al. Construction and evaluation of a novel diagnosis process for 2019-corona virus disease. *Zhonghua Yi Xue Za Zhi* 2020;**100**(0):E019. [DOI: 10.3760/cma.j.cn112137-20200228-00499 10.3760/cma.j.cn112137-20200228-00499.]

References to ongoing studies

ChiCTR2000029625 *{published data only}*

ChiCTR2000029625. Construction of early warning and prediction system for patients with severe / critical novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029625 (first received 27 April 2020).

ChiCTR2000029695 *{published data only}*

ChiCTR2000029695. Early detection of novel coronavirus pneumonia (COVID-19) based on a novel high-throughput mass spectrometry analysis with exhaled breath. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029695 (first received 27 April 2020).

ChiCTR2000029810 *{published data only}*

ChiCTR2000029810. Clinical study of a novel high sensitivity nucleic acid assay for novel coronavirus pneumonia (COVID-19) based on CRISPR-cas protein. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029810 (first received 27 April 2020).

ChiCTR2000029870 *{published data only}*

ChiCTR2000029870. Evaluation of rapid diagnostic kit (IgM/IgG) for novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029870 (first received 27 April 2020).

ChiCTR2000029883 *{published data only}*

ChiCTR2000029883. A comparative study on the sensitivity of nasopharyngeal and oropharyngeal swabbing for the detection of SARS-CoV-2 by real-time PCR. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029883 (first received 27 April 2020).

ChiCTR2000029982 *{published data only}*

ChiCTR2000029982. Study for using multiomics in the diagnosis and treatment of novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000029982 (first received 27 April 2020).

ChiCTR2000030005 *{published data only}*

ChiCTR2000030005. Nucleic acid analysis of novel coronavirus pneumonia (COVID-19) in morning sputum samples and pharyngeal swabs-a prospectively diagnostic test. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030005 (first received 27 April 2020).

ChiCTR2000030085 *{published data only}*

ChiCTR2000030085. Cancelled by the investigator Study for the false positive rate of IgM / IgG antibody test kit for novel coronavirus pneumonia (COVID-19) in different inpatients. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030085 (first received 27 April 2020).

ChiCTR2000030185 *{published data only}*

ChiCTR2000030185. The value of critical care ultrasound in rapid screening, diagnosis, evaluation of effectiveness and intensive prevention of novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030185 (first received 27 April 2020).

ChiCTR2000030253 *{published data only}*

ChiCTR2000030253. Exploration and research for a new method for detection of novel coronavirus (COVID-19) nucleic acid. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030253 (first received 27 April 2020).

ChiCTR2000030334 *{published data only}*

ChiCTR2000030334. MicroRNA as a marker for early diagnosis of novel coronavirus infection (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030334 (first received 27 April 2020).

ChiCTR2000030542 *{published data only}*

ChiCTR2000030542. A clinical study about the diagnosis and prognosis evaluation of novel coronavirus pneumonia (COVID-19) based on viral genome, host genomic sequencing, relative cytokines and other laboratory indexes. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030542 (first received 27 April 2020).

ChiCTR2000030543 *{published data only}*

ChiCTR2000030543. Detection of coronavirus in simultaneously collecting tears and throat swab samples collected from the patients with novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030543 (first received 27 April 2020).

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030558 *{published data only}*

ChiCTR2000030558. Cancelled by the investigator Epidemiological research of novel coronavirus pneumonia (COVID-19) suspected cases based on virus nucleic acid test combined with low-dose chest CT screening in primary hospital. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030558 (first received 27 April 2020).

ChiCTR2000030706 *{published data only}*

ChiCTR2000030706. Cancelled by the investigator Application of cas13a-mediated RNA detection in the assay of novel coronavirus nucleic acid (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030706 (first received 27 April 2020).

ChiCTR2000030721 *{published and unpublished data}*

ChiCTR2000030721. A comparative study for the sensitivity of induced sputum and throat swabs for the detection of SARS-CoV-2 by real-time PCR in patients with novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030721 (first received 27 April 2020).

ChiCTR2000030754 *{published data only}*

ChiCTR2000030754. Medical records based study for the accuracy of SARS-CoV-2 IgM antibody screening for diagnosis of novel coronavirus pneumonia (COVID-19). apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030754 (first received 27 April 2020).

ChiCTR2000030833 *{published data only}*

ChiCTR2000030833. Clinical validation and application of high-throughput novel coronavirus (2019-nCoV) screening detection kit. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030833 (first received 27 April 2020).

ChiCTR2000030834 *{published data only}*

ChiCTR2000030834. Epidemiological characteristics and antibody levels of novel coronavirus pneumonia (COVID-19) of pediatric medical staff working in quarantine area. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030834 (first received 27 April 2020).

ChiCTR2000030838 *{published data only}*

ChiCTR2000030838. Development of warning system with clinical differential diagnosis and prediction for severe type of novel coronavirus pneumonia (COVID-19) patients based on artificial intelligence and CT images. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030838 (first received 27 April 2020).

ChiCTR2000030856 *{published data only}*

ChiCTR2000030856. An artificial intelligence assistant system for suspected novel coronavirus pneumonia (COVID-19) based on chest CT. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030856 (first received 27 April 2020).

ChiCTR2000030859 *{published data only}*

ChiCTR2000030859. A medical based analysis for influencing factors of death of novel coronavirus pneumonia (COVID-19) patients in Wuhan Third Hospital. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030859 (first received 27 April 2020).

ChiCTR2000030860 *{published data only}*

ChiCTR2000030860. A medical records based study for investigation of dynamic profile of RT-PCR test for SARS-CoV-2 nucleic acid of novel coronavirus pneumonia (COVID-19) patients. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030860 (first received 27 April 2020).

ChiCTR2000030862 *{published data only}*

ChiCTR2000030862. Correlation analysis of blood eosinophil cell levels and clinical type category of novel coronavirus pneumonia (COVID-19): a medical records based retrospective study. apps.who.int/trialsearch/Trial2.aspx?TrialID=ChiCTR2000030862 (first received 27 April 2020).

NCT04245631 *{published data only}*

NCT04245631. Development of a simple, fast and portable recombinase aided amplification assay for 2019-nCoV. clinicaltrials.gov/ct2/show/NCT04245631 (first received 27 April 2020).

NCT04259892 *{published data only}*

NCT04259892. Viral excretion in contact subjects at high/moderate risk of coronavirus 2019-nCoV infection. ClinicalTrials.gov/show/NCT04259892 (first received 27 April 2020).

NCT04279795 *{published data only}*

NCT04279795. Detection of 2019 novel coronavirus in multiple organ system and its relationship with clinical manifestations. ClinicalTrials.gov/show/NCT04279795 (first received 27 April 2020).

NCT04304690 *{published data only}*

NCT04304690. SARS-CoV2 seroconversion among front line medical and paramedical staff in emergency, intensive care units and infectious disease departments during the 2020 epidemic. clinicaltrials.gov/ct2/show/NCT04304690 (first received 27 April 2020).

NCT04311398 *{published data only}*

NCT04311398. Development and verification of a new coronavirus multiplex nucleic acid detection system. ClinicalTrials.gov/show/NCT04311398 (first received 27 April 2020).

NCT04316728 *{published data only}*

NCT04316728. Clinical performance of the VivaDiag ™ COVID-19 IgM IgG rapid test in early detecting the infection of COVID-19. ClinicalTrials.gov/show/NCT04316728 (first received 27 April 2020).

NCT04321369 *{published data only}*

NCT04321369. Impact of swab site and sample collector on testing sensitivity for SARS-CoV-2 virus in symptomatic individuals. clinicaltrials.gov/ct2/show/NCT04321369 (first received 27 April 2020).

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

NCT04322279 *{published data only}*

NCT04322279. Factors associated with a positive SARS-CoV-2 serology in contact subjects at high/moderate risk of coronavirus SARS-CoV-2 infection (CoV-CONTACT-SERO). clinicaltrials.gov/ct2/show/NCT04322279 (first received 27 April 2020).

NCT04322513 *{published data only}*

NCT04322513. Biomarkers for identification of SARS-COV-2 infection. clinicaltrials.gov/ct2/show/NCT04322513 (first received 27 April 2020).

Sullivan 2020 *{published data only}*

Sullivan PS, Sailey C, Guest JL, Guarner J, Siegler AJ, Valentine-Graves, et al. Detection of SARS-CoV-2 RNA and antibodies in diverse samples: protocol to validate the sufficiency of provider-observed home-collected blood, saliva and oropharyngeal samples. *JMIR Public Health and Surveillance* 2020. [DOI: 10.2196/19054]

Additional references

Bossuyt 2015

Bossuyt PM, Reitsma JB, Bruns DE, Gatsonis CA, Glasziou PP, Irwig L, et al. STARD 2015: an updated list of essential items for reporting diagnostic accuracy studies. *BMJ* 2015;**351**:h5527. [DOI: 10.1136/bmj.h5527] [PMID: 26511519]

CDC China 2020

National Health Commission of the People's Republic of China. Release of 7th edition of case definitions. www.nhc.gov.cn/yzygj/s7653p/202003/46c9294a7dfe4cef80dc7f5912eb1989.shtml (accessed prior to 23 June 2020).

Cheng 2020b

Cheng MP, Yansouni CP, Basta NE, Desjardins M, Kanjilal S, Paquette K, et al. Serodiagnostics for severe acute respiratory syndrome-related coronavirus-2: a narrative review. *Annals of Internal Medicine* (in press).

Covidence [Computer program]

Veritas Health Innovation Covidence. Version accessed 27 April 2020. Melbourne, Australia: Veritas Health Innovation.Available at covidence.org.

Macaskill 2010

Macaskill P, Gatsonis C, Deeks JJ, Harbord RM, Takwoingi Y. Chapter 10: analysing and presenting results. In: Deeks JJ, Bossuyt PM, Gatsonis C editor(s). Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0. The Cochrane Collaboration, 2010. Available from methods.cochrane.org/sdt/handbook-dta-reviews.

McInnes 2018

McInnes MDF, Moher D, Thombs BD, McGrath TA, Bossuyt PM and the PRISMA-DTA Group. Preferred Reporting Items for a Systematic Review and Meta-analysis of Diagnostic Test Accuracy Studies: The PRISMA-DTA Statement. *JAMA* 2018;**319**(4):388-396. [DOI: 10.1001/jama.2017.19163] [PMID: 29362800]

McInnes 2020

McInnes M, Leeflang MM, Salameh J-P, McGrath T, Van der Pol CB, Frank RA, et al. Imaging tests for the diagnosis of COVID-19. *Cochrane Database of Systematic Reviews* 2020, Issue 4. [DOI: 10.1002/14651858.CD013639]

Moher 2009

Moher D, Liberati A, Tetzlaff J, Altman DG, The PRISMA Group (2009). Preferred reporting items for systematic reviews and meta-analyses: the PRISMA Statement. *PLoS Medicine* 6;**7**:1000097. [DOI: 10.1371/journal.pmed1000097]

Review Manager 2014 [Computer program]

Nordic Cochrane Centre, The Cochrane Collaboration Review Manager 5 (RevMan 5). Version 5.3. Copenhagen: Nordic Cochrane Centre, The Cochrane Collaboration, 2014.

Stata [Computer program]

Stata. Version 15. College Station, TX, USA: StataCorp, 2017.Available at www.stata.com.

Takwoingi 2017

Takwoingi Y, Guo B, Riley RD, Deeks JJ. Performance of methods for meta-analysis of diagnostic test accuracy with few studies or sparse data. *Statistical Methods in Medical Research* 2017;**26**(4):1896-911.

Whiting 2011

Whiting PF, Rutjes AW, Westwood ME, Mallett S, Deeks JJ, Reitsma JB, et al. QUADAS-2: a revised tool for the quality assessment of diagnostic accuracy studies. *Annals of Internal Medicine* 2011;**155**(8):529-36.

WHO 2020

World Health Organization (WHO). Global surveillance for COVID-19 caused by human infection with COVID-19 virus Interim guidance. www.who.int/publications/i/item/global-surveillance-for-human-infection-with-novel-coronavirus-(2019-ncov) (accessed prior to 23 June 2020). [https://www.who.int/publications/i/item/global-surveillance-for-human-infection-with-novel-coronavirus-(2019-ncov)]

References to other published versions of this review

Deeks 2020

Deeks JJ, Dinnes J, Takwoingi Y, Davenport C, Leeflang MM, Spijker R, et al. Diagnosis of SARS-CoV-2 infection and COVID-19: accuracy of signs and symptoms; molecular, antigen, and antibody tests; and routine laboratory markers. *Cochrane Database of Systematic Reviews* 2020, Issue 4. [DOI: 10.1002/14651858.CD013596]

* Indicates the major publication for the study

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

CHARACTERISTICS OF STUDIES

Characteristics of included studies *[ordered by study ID]*

Adams 2020 [A]

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] Rt-PCR confirmed COVID-19 cases (n = 40) [2] Pre-pandemic controls (n = 142) Recruitment: unclear Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 182 (40) Inclusion and exclusion criteria: none stated
Patient characteristics and setting	Setting [1] Acute hospital samples (n = 16), recovering healthcare workers (n = 6), convalescent patients (n = 18) [2] Health blood donors (n = 60); organ donor samples (n = 50); pertussis vaccine study (BERT) (n = 32) Location [1] Acute hospital patients from Oxford University Hospitals NHS Foundation Trust (location of other groups NR) [2] National Health Service Blood and Transplant, UK National Quality in Organ Donation (QUOD) study, the 'BERT' study (A Study Exploring Whooping Cough Protection in Children and Adults), UK Country: UK Dates: [1] NR; [2] before December 2019 Symptoms and severity: [1] asymptomatic (n = 1); mild (n = 26); severe (n = 4); critical (n = 9) Sex: NR Age: [1] Median (range): 57 (22-95) years; [2] NR Exposure history: NR
Index tests	Adams 2020 [A] is test [A] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	Reference standard for cases: RT-PCR Samples used: nose or throat swabs Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: pre-pandemic
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: computed from analysis of individual participant data

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [A] *(Continued)*

	All participants received the same reference standard: no Missing data: different tests were evaluted in different numbers of samples, no information on how sampling decisions were made Uninterpretable results: not mentioned Indeterminate results: not mentioned Unit of analysis: per patient
Comparative	
Notes	Funding: NIHR, Oxford Biomedical Research Centre, the UK Government Department of Health and Social Care and grants from NIHR and the Medical Research Council Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: several authors declared relationships with companies for other work; funders were co-authors

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [A] *(Continued)*

Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Adams 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [B] is test [B] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [B] *(Continued)*

	Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Adams 2020 [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [C] is test [C] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [D]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [D] is test [D] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Adams 2020 [E]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [E] is test [E] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [E] *(Continued)*

	Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Adams 2020 [F]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [F] is test [F] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [G]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [G] is test [G] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Adams 2020 [H]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [H] is test [H] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [H] *(Continued)*

	Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Adams 2020 [I]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [I] is test [I] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Adams 2020 [J]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Index tests	Adams 2020 [J] is test [J] from the following entry: Test name: [A] ELISA test [B]-[J] LFIA names withheld Manufacturer: [A] in-house [B]-[J] manufacturer name withheld Ab targets: [A] IgG and IgM [B]-[C] total antibodies [D]-[J] IgG and IgM Antigens used: [A] SARS-CoV-2 trimeric S protein [B]-[J] details withheld Test method: [A] ELISA [B]-[J] LFIA further details withheld Timing of samples: 4-62 days after onset of symptoms Samples used: plasma Test operators: laboratory staff Definition of test positivity: [A]-[J] NR Blinded to reference standard: NR Threshold predefined: no for [A], unclear for [B] to [J]
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Adams 2020 [A])
Comparative	
Notes	

Bendavid 2020

Study characteristics	
Patient Sampling	Multiple-group study recruiting patients estimating sensitivity and specificity [1] Specimens from COVID-19 cases recruited from 3 different sources (n = 157 specimens) [2] Specimens from non-cases recruited from 13 different sources (n = 3308 specimens) Recruitment: unclear Prospective or retrospective recruitment of cases: unclear Sample size (virus/COVID cases): 3481 (3324) specimens Inclusion and exclusion criteria: none stated
Patient characteristics and setting	Setting: not described for most sample sets Location: not described for most sample sets Country: USA, China, but not described for most sample sets Dates: not described Symptoms and severity: not described Sex: not described Age: not described

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Bendavid 2020 *(Continued)*

	Exposure history: not described
Index tests	Test name: unnamed test Manufacturer: Premier Biotech, Minneapolis, USA (may be Hangzhou All-test) Ab targets: IgG, IgM Antigens used: NR Test method: NR Timing of samples: NR Samples used: serum, plasma, fingerstick blood, venous whole blood (may be blood for majority of cases) Test operators: NR Definition of test positivity: NR Blinded to reference standard: no Threshold predefined: NR
Target condition and reference standard(s)	Reference standard for cases: various unclear, includes RT-PCR-pos Samples used: NR Timing of reference standard: NR Blinded to index test: yes Incorporated index test: serology tests were included in 1 cohort Reference standard for non-cases: pre-pandemic, RT-PCR-neg, healthy volunteers
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no All participants received the same reference standard: no Missing data: none mentioned Uninterpretable results: none mentioned Indeterminate results: none mentioned Unit of analysis: specimens
Comparative	
Notes	Funding: individual donors Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Bendavid 2020 *(Continued)*

Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Unclear
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Unclear		
Were results presented per patient?	No		
Could the patient flow have introduced bias?		High risk	

Burbelo 2020 [A]

Study characteristics

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Burbelo 2020 [A] *(Continued)*

Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] 35 patients with COVID-19 symptoms and RT-PCR-positive [2] 32 pre-pandemic blood donors Recruitment: unclear Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 67 (35) Inclusion and exclusion criteria: nothing additional The study included a 3rd group on COVID-19 suspects (n = 10) who were not included as they had no reference standard diagnosis
Patient characteristics and setting	Setting [1] Hospital patients [2] Blood donors Location [1] University of California, San Diego; University of Washington, Seattle; EvergreenHealth, Kirkland, Washington; NIH Clinical Center, NIH [2] NIH Clinical Center, NIH Country: USA Dates: NR Symptoms and severity: [1] 37% (13/35) were on a ventilator Sex: [1] 87% (30/35) male [2] NR Age: [1] median age 44 years (range 32-50 years) [2] NR Exposure history: NR
Index tests	This entry (Burbelo 2020 [A]) refers to the LIPS assay to detect antibodies to the nucleocapsid (N) protein Test name: LIPS Manufacturer: in-house Ab targets: antibodies for the nucleocapsid and S proteins Antigens used: nucleocapsid and S proteins Test method: LIPS Timing of samples: 2-50 days pso Samples used: plasma or serum Test operators: presumed laboratory researchers Definition of test positivity: 125,000 LU for nucleocapsid and 45,000 LU for S proteins Blinded to reference standard: unclear Threshold predefined: no, derived from analysis of group [2] to achieve 100% specificity
Target condition and reference standard(s)	Reference standard for cases: RT-PCR Samples used: nasal or throat swabs Timing of reference standard: unclear Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: pre-pandemic controls (no testing)
Flow and timing	Time interval between index and reference tests: unclear Results presented by time period: ≤ 14 days; > 14 days All participants received the same reference standard: no Missing data: yes - unclear why there are different numbers for spike and nucleocapsid tests Uninterpretable results: not mentioned Indeterminate results: not mentioned

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Burbelo 2020 [A] *(Continued)*

Comparative	
Notes	Funding: intramural research programmes of the National Institute of Dental and Craniofacial Research, the National Institute of Allergy and Infectious Diseases, and the National Institute of Health Clinical Center Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Burbelo 2020 [A] *(Continued)*

The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Unclear		
Were results presented per patient?	No		
Could the patient flow have introduced bias?		High risk	

Burbelo 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Burbelo 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Burbelo 2020 [A])
Index tests	This entry (Burbelo 2020 [B]) refers to the LIPS assay to detect antibodies to the spike (S) protein; see (Burbelo 2020 [A] for further study characteristics and QUADAS-2 assessments) Test name: LIPS Manufacturer: in-house Ab targets: antibodies for the nucleocapsid and S proteins Antigens used: nucleocapsid and S proteins Test method: LIPS Timing of samples: 2-50 days pso Samples used: plasma or serum Test operators: presumed laboratory researchers Definition of test positivity: 125,000 LU for nucleocapsid and 45,000 LU for S proteins Blinded to reference standard: unclear Threshold predefined: no - derived from analysis of group [2] to achieve 100% specificity
Target condition and ref-	See main entry for this study for characteristics and QUADAS-2 assessment (Burbelo 2020 [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Burbelo 2020 [B] *(Continued)*

erence standard(s)	
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Burbelo 2020 [A])
Comparative	
Notes	

Cai 2020a

Study characteristics	
Patient Sampling	2-group study to estimate sensitivity and specificity for detection of active disease [1] Laboratory-confirmed COVID-19 patients (n = 276) [2] Controls with other infections (n = 167). A third group of healthy controls was used to set thresholds (n = 200) but not estimate accuracy. Recruitment method: NR if patients were consecutive Sample size (viral/COVID cases): 443 (276) Exclusion criteria: none stated
Patient characteristics and setting	[1] Hospital (inpatients); Chongqing Three Gorges Central Hospital, Yongchuan Hospital Affiliated to Chongqing Medical University (CQMU), and The Public Health Center, in Chongqing, China (recruitment dates NR). 168/276 (61%) had fever. Median age 48 (IQR 37-56; range 0-84) years, 151/276 (55%) male. 99/276 (36%) reported known exposure [2] Controls with other infection (n = 167); Second Hospital Affiliated to CQMU and Children's Hospital Affiliated to CQMU; time NR. Other infections included: influenza A virus (25), respiratory syncytial virus (7), parainfluenza 111 virus (8), influenza B virus (5), adenovirus (6), *Klebsiella pneumoniae* (8), *Streptococcus pneumoniae* (3), Mycoplasma (5), *Acinetobacter baumannii* (10), *Candida albicans* (2), *Staphylococcus aureus* (3), *Mycobacterium tuberculosis* (4), Hepatitis B virus (33), Hepatitis C virus (22), Syphilis (23) and Saccharomycopsis (3) [3] Healthy controls (n = 200), source NR; recruited > 1 year before the outbreak. No further details
Index tests	1 Ab test, blinding NR Laboratory-based in-house luminescent immunoassay (CLIA) using serum samples Measured IgM +IgG. Antigen: peptide from SARS-CoV-2 S protein Test threshold: determined as the mean luminescence (CL) value of the 200 normal sera plus 5 folds of SD; cut-off used ≥ 0.7 CL (for both IgG and IgM). (Determined in the healthy control group) Samples acquired day 2-day 27 after symptoms. Person applying the test NR.
Target condition and reference standard(s)	1. Real time RT-PCR detection of virus RNA, samples not described. Reference threshold and timing NR. Blinded to index test 2. Healthy controls, pre-December 2019
Flow and timing	Time interval between index and reference: NR. Accuracy results were not disaggregated by time period since point of symptom onset. No missing data, uninterpretable or indeterminate results described Analysis participant-based

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cai 2020a *(Continued)*

Comparative	
Notes	Funded by Emergency Project from the Science & Technology Commission of Chongqing; Major National S&T program grant from Science & Technology Commission of China; Grant from the National Natural Science Foundation of China, Grant from the Science & Technology Commission of Yuzhong district, Chongqing. COI (reported or derived): study author employed by BioScience Co. LTD, Tianjin, China Publication status (source): preprint (not peer reviewed) (medRxiv) NOTE: Study author institution reported as BioScience Co. LTD, Tianjin, China (www.bio-science-tj.com/en/about.php)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cai 2020a *(Continued)*

Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Cassaniti 2020 (A)

Study characteristics	
Patient Sampling	The report contains 3 different groups that fit with 2 different comparisons. 2-group design with separate estimates of sensitivity and specificity [1] COVID-19-positive patients in ICU (n = 30) [2] Healthy volunteers with negative RT-PCR results (n = 30) Recruitment: unclear Sample size (virus/COVID cases): 60 (30) Inclusion and exclusion criteria: not further described (Single group recruiting individuals presenting with symptoms extracted as Cassaniti 2020 (B))
Patient characteristics and setting	Setting: hospital inpatients (Infectious Diseases Unit or ICU, Tertiary hospital) Location: Fondazione IRCCS Policlinico San Matteo, Pavia Country: Italy Dates: NR Symptoms and severity: [1] NR [2] NR Sex: [1] 83% male (25/30); [2] 55% Male (11/30)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cassaniti 2020 (A) *(Continued)*

	Age: [1] median age, 73.5; range 38-86 years; [2] median age, 38.5; range 25-69 years) Exposure history: [1] NR; [2] 10 (33.3%) previously infected with common OC43, 229E, HKU1, and NL63 coronavirus
Index tests	Test name: VivaDiag COVID-19 IgM/IgG Manufacturer: VivaChek Ab targets: IgM, IgG Antigens used: NR Test method: LFIA Timing of samples: [1] median 7 days (IQR 4-11) after first test; [2] NR Samples used: serum or blood Test operators: NR Definition of test positivity: visible line Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: RT-PCR targeting RNA-dependent RNA polymerase and E genes were used to detect the presence of SARS-CoV-2 according to the WHO guidelines (2 negatives required for non-cases) Samples used: respiratory samples Timing of reference standard: [1] during patient care [2] unclear Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: no information Results presented by time period: no information All participants received the same reference standard: yes Missing data: none mentioned Uninterpretable results: none mentioned Indeterminate results: none mentioned Unit of analysis: participants
Comparative	
Notes	Funding: VivaDiag COVID-19 IgM/IgG Rapid Test provided free of charge by the Italian Chinese community. Regional Health Authority of Lombardy, Milan, Italy and Italian Ministry of Health, Ricerca Finalizzata Publication status: published letter Source: academic journal Study author COI: none mentioned

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cassaniti 2020 (A) *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cassaniti 2020 (B)

Study characteristics	
Patient Sampling	Single-group study estimating sensitivity and specificity Patients presenting to A&E with fever and respiratory symptoms indicative of COVID-19 infection. 2 additional cohorts extracted as separate 2-group study (Cassaniti 2020 (A)) Recruitment: unclear Sample size (virus/COVID cases): 50 (38) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: A&E Location: Fondazione IRCCS Policlinico San Matteo, Pavia Country: Italy Dates: NR Symptoms and severity: NR Sex: 68% male 34 male/16 female Age: median age, 61.50; range 33-97 years Exposure history: NR
Index tests	Test name: VivaDiag COVID-19 IgM/IgG Manufacturer: VivaChek Ab targets: IgM, IgG Antigens used: NR Test method: LFIA Timing of samples: on presentation at A&E Samples used: serum or blood Test operators: NR Definition of test positivity: visible line Blinded to reference standard: yes on presentation Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: RT-PCR targeting RNA-dependent RNA polymerase and E genes were used to detect the presence of SARS-CoV-2 according to the WHO guidelines Samples used: nasal swab Timing of reference standard: on presentation Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: single negative RT-PCR result
Flow and timing	Time interval between index and reference tests: done at the same time Results presented by time period: no (likely to be short as on admission) All participants received the same reference standard: yes Missing data: none mentioned Uninterpretable results: none mentioned Indeterminate results: not mentioned Unit of analysis: participants
Comparative	
Notes	Funding: VivaDiag COVID-19 IgM/IgG Rapid Test provided free of charge by the Italian Chinese community. Regional Health Authority of Lombardy, Milan, Italy and Italian Ministry of Health, Ricerca Finalizzata Publication status: published letter Source:Academic journal

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cassaniti 2020 (B) *(Continued)*

Study author COI: none mentioned

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Low risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Cassaniti 2020 (B) *(Continued)*

DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Unclear
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Unclear risk

Chen 2020a

Study characteristics	
Patient Sampling	Unclear whether study recruited as 1 or 2 groups (we describe it as a 2-group study), estimating sensitivity and specificity [1] RT–PCR-positive samples, n = 7 samples [2] RT–PCR-negative samples, but clinically suspicious for COVID-19, n = 12 samples A 3rd group of 'normal' samples (n = 51), were used to derive test threshold and not included in the accuracy evaluation. Recruitment: unclear Prospective or retrospective recruitment of cases: unclear Sample size (virus/COVID cases): 19 (7) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: hospital samples Location: Guangzhou Eighth People's Hospital and Nanfang Hospital, Guangzhou province Country: China Dates: NR Symptoms and severity: [1] NR; [2] fever: 12/12 (100%) Sex: NR Age: NR Exposure history: NR
Index tests	Test name: no name. LFIA that uses lanthanide-doped polystyrene nanoparticles (LNPs) Manufacturer: in–house Ab targets: IgG Antigens used: recombinant nucleocapsid phosphoprotein of SARS-CoV-2 Test method: LFIA that uses lanthanide-doped polystyrene nanoparticles (LNPs) Timing of samples: NR Samples used: serum Test operators: NR Definition of test positivity: At/Ac ratio (R) > 0.0666 Blinded to reference standard: NR Threshold predefined: defined from control samples
Target condition and reference standard(s)	Reference standard for cases: RT–PCR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Chen 2020a *(Continued)*

	Samples used: NR Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: RT–PCR single negative
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: NR All participants received the same reference standard: yes Missing data: none reported Uninterpretable results: none reported Indeterminate results: none reported Unit of analysis: sample
Comparative	
Notes	Funding: National Natural Science Foundation of China and China Postdoctoral Science Foundation Publication status: peer–reviewed early online Source: academic journal Study author COI: study authors state no competing financial interests

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Chen 2020a *(Continued)*

DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	No		
Could the patient flow have introduced bias?		High risk	

Dohla 2020

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] COVID-19 suspects attending community screening (n = 39) [2] Confirmed COVID-19 cases (n = 10) Recruitment: [1] random selection (no random sampling method stated); [2] unclear Prospective or retrospective recruitment of cases: [1] prospective; [2]retrospective Sample size (virus/COVID cases): 49 (22) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: [1] community screening centre; [2] NR Location: [1] German Red Cross COVID-19 testing centre; [2] NR Country: Germany Dates: NR Symptoms and severity: (71%) with dry cough; (65%) with fatigue; (46%) with runny nose (only %s reported). 5/49 (10%) were asymptomatic Sex: 25/49 (51%) male Age: median 46 (IQR 28–72) years

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Dohla 2020 *(Continued)*

	Exposure history: identified in 22/49 (45%): median time exposure–to–test of 18.5 days (IQR 15–24)
Index tests	Test name: NR Manufacturer: NR Ab targets: IgM and IgG Antigens used: SARS-CoV-2 antigen (not further described) Test method: CGIA Threshold: visible line - weak and strong responses counted as positive Timing of median time exposure–to–test = 18.5 days (IQR 15–24) known (45%) for samples Samples used: [1] fingerprick blood [2] stored serum Test operators: NR Definition of test positivity: weakly clearly visible line Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: [1] RT–qPCR (Altona Diagnostics), threshold NR; [2] RT–qPCR (unknown if same kit), threshold NR Samples used: [1] throat swab; [2] NR Timing of reference standard: [1] same time as index test. [2] NR. For 22 participants (unclear how many in group 1 or 2): median time exposure–to–test of 18.5 days (IQR 15–24) Blinded to index test: NR - presumed Incorporated index test: no Reference standard for non-cases: single negative RT-qPCR
Flow and timing	Time interval between index and reference tests: simultaneous Results presented by time period: no All participants received the same reference standard: yes Missing data: none reported Uninterpretable results: reporting that there were none Indeterminate results: weak lines considered as test positive Unit of analysis: participant
Comparative	
Notes	Funding: none declared Publication status: published paper (proof) Source: academic journal Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Dohla 2020 *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Unclear
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Yes		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Low risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Du 2020

Study characteristics	
Patient Sampling	Single group estimating sensitivity in convalescent patients [1] Hospital COVID-19 convalescent patients (n = 60) Recruitment: unclear Sample size (virus/COVID cases): 60 (60) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: hospital inpatients (convalescent) Location: Wuhan Tongji Hospital Country: China Dates: admitted 12 January 2020-5 February 2020 Symptoms and severity: no information Sex: no information Age: no information Exposure history: no information
Index tests	Test name: NR Manufacturer: NR Ab targets: IgM, IgG Antigens used: NR Test method: NR but presumed to be CLIA based on reported threshold in AU/mL Timing of samples: during hospital stay (between 3 March 2020 and 14 March 2020) Samples used: NR Test operators: unclear Definition of test positivity: > 10 AU/mL Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases (including threshold): method NR Samples used: NR Timing of reference standard: diagnosed during initial hospital stay (6-7 weeks previously) Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: 6-7 weeks Results presented by time period: results presented by day since onset All participants received the same reference standard: presumed Missing data: none mentioned Uninterpretable results: none mentioned Indeterminate results: none mentioned Unit of analysis: participant
Comparative	
Notes	Funding: Beijing Natural Science Foundation Publication status: published letter Source: academic journal Study author COI: none mentioned
Methodological quality	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Du 2020 *(Continued)*

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Unclear
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Du 2020 *(Continued)*

Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Freeman 2020

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] confirmed COVID-19 cases (n = 99) [2] Healthy adults (n = 377) or with other infections (n = 142) Additionally reports a separate cross-reactivity study using acute and convalescent paired sera from PCR confirmed commonly circulating coronavirus (229E, NL63, OC43, and HKU1)- infected patients Recruitment: unclear Prospective or retrospective recruitment of cases: unclear Sample size (virus/COVID cases): 618 (99) Inclusion and exclusion criteria: [1] convalescent PCR+ COVID-19 cases sera collected at day 10 pso or later
Patient characteristics and setting	Setting: NR Location: NR Country: USA Dates: NR Symptoms and severity: [1] NR [2] healthy controls (n = 377); suspected hantavirus (n = 101); HIV (n = 21); hepatitis B virus (n = 10); hepatitis C virus-positive (n = 10) Sex: NR Age: NR Exposure history: NR
Index tests	Test name: SARS-CoV-2 S protein ELISA Manufacturer: in-house Ab targets: IgG, IGM and total antibodies Antigens used: pre-fusion stabilised ectodomain of SARS-CoV-2 spike (S) Test method: ELISA Timing of samples: at day 10 pso or later Samples used: serum Test operators: laboratory staff Definition of test positivity: based on optical density signal Blinded to reference standard: NR Threshold predefined: NR
Target condition and reference standard(s)	Reference standard for cases: PCR Samples used: NR Timing of reference standard: NR Blinded to index test: yes, PCR was performed before index test (inferred) Incorporated index test: no Reference standard for non-cases: pre-pandemic (healthy controls or with other diseases)
Flow and timing	Time interval between index and reference tests: not clear Results presented by time period: no

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Freeman 2020 *(Continued)*

	All participants received the same reference standard: no Missing data: not mentioned Uninterpretable results: not mentioned Indeterminate results: not mentioned Unit of analysis: per participant
Comparative	
Notes	Funding: intramural funding from the National Institute of Allergy and Infectious Diseases Publication status: preprint (not peer-reviewed) Source: bioRxiv Study author COI: NR

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Freeman 2020 *(Continued)*

Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Gao 2020a

Study characteristics	
Patient Sampling	Single-group study estimating sensitivity [1] Patients with confirmed COVID-19 (n = 38) Recruitment: unclear Sample size (virus/COVID cases): 38 (38) Inclusion and exclusion criteria: COVID-19 confirmed by New Coronavirus Pneumonia Prevention and Control Program (5th edition) published by the National Health Commission of China.
Patient characteristics and setting	Setting: hospital inpatient Location: Second People's Hospital of Fuyang Country: China Dates: 22 January 2020-28 February 2020 Symptoms and severity: 3/38 described as in severe or critical conditions; 35/38 described as mild cases Sex: 55.3% (21/38) male Age: median age 40.5 years (IQR 31.0-49.5years), range 15-75 years Exposure history: NR
Index tests	Test name: Colloidal Gold Antibodies Test Manufacturer: Innovita Biological Technology Co., Ltd Ab targets: IgM, IgG Antigens used: NR Test method: CGIA

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020a *(Continued)*

	Timing of samples: days 0-15+ Samples used: serum Test operators: NR Definition of test positivity: visible line Blinded to reference standard: NR Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: participants met the criteria of the New Coronavirus Pneumonia Prevention and Control Program (5th edition) published by the National Health Commission of China Samples used: NR Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes: 0-7 days (n = 13), 8-14 days (n = 8) and ≥ 15 days (n = 23) after onset of symptoms All participants received the same reference standard: yes Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: results reported for participants. 38 participants included and 76 serum samples collected in total from these 38 participants. Median number of samples collected from each participant was 8
Comparative	
Notes	Funding: The Science and Technology Bureau of Fuyang Publication status: accepted manuscript (peer reviewed) Source: Journal of Medical Virology Study author COI: none reported

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020a *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Gao 2020b [A]

Study characteristics	
Patient Sampling	Single-group study recruiting patients estimating sensitivity [1] confirmed COVID-19 cases Recruitment: consecutive (inferred). From all confirmed cases admitted to hospital Prospective or retrospective recruitment of cases: retrospectively (appears) Sample size (virus/COVID cases): 22 participants (corresponding to 37 samples) Inclusion and exclusion criteria: not clearly defined; describes all participants having typical ground-glass opacity of the lung on CT but not clear if this was part of eligibility

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020b [A] *(Continued)*

Patient characteristics and setting	Setting: hospital inpatient Location: Fifth Hospital of Shijiazhuang Country: China Dates: from 21 January-24 February 2020 Symptoms and severity: typical ground-glass opacity in lung was observed in CT scan results of all participants. At the time the paper was written all participants had recovered and been discharged from hospital. Sex: 14/22 male (64%) Age: 40 (4-72) years Exposure history: 11 participants had recent history of travel to epidemic areas, and the remaining 10 had close contacts with their family members, who were confirmed to be infected by 2019-nCoV
Index tests	Gao 2020b [A] is test [A] from the following entry: Test name: [A] CLIA; [B] GICA; [C] ELISA Manufacturer: Beier Bioengineering Company (Beijing, China) Ab targets: IgG and IgM Antigens used: spike (S) and nucleocapsid (N) proteins of 2019-nCoV Test method: [A] CLIA; [B] GICA; [C] ELISA Timing of samples: [1] early stage (1-7 days pso) 10/37 samples (27%), [2] middle stage (8-14 days pso) 13/37 samples (35%); [3] late stage (14-24 days pso) 14/37 samples (38%) Samples used: serum Test operators: laboratory staff Definition of test positivity: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Visible line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result. Blinded to reference standard: NR Threshold predefined: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Positive results showed the appearance of both control line and testing line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result.
Target condition and reference standard(s)	Reference standard for cases: RT-PCR assay (2019-nCoV RNA Test Kit, Daan Gene Company, China) Samples used: nasal and pharyngeal swab specimens Timing of reference standard: on admission (most likely) Blinded to index test: yes, index tests performed on already-confirmed cases (inferred) Incorporated index test: no Reference standard for non-cases: N/A
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: yes Missing data: timing of reference standard test Uninterpretable results: Indeterminate results: Unit of analysis: samples
Comparative	
Notes	Funding: NR Publication status: published letter Source: Chinese Medical Journal Study author COI: none
Methodological quality	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020b [A] *(Continued)*

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference			High

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020b [A] *(Continued)*

standard does not match the question?	
DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Unclear
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	No
Could the patient flow have introduced bias?	High risk

Gao 2020b [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Index tests	Gao 2020b [B] is test [B] from the following entry: Test name: [A] CLIA; [B] GICA; [C] ELISA Manufacturer: Beier Bioengineering Company (Beijing, China) Ab targets: IgG and IgM Antigens used: spike (S) and nucleocapsid (N) proteins of 2019-nCoV Test method: [A] CLIA; [B] GICA; [C] ELISA Timing of samples: [1] early stage (1-7 days pso) 10/37 samples (27%), [2] middle stage (8-14 days pso) 13/37 samples (35%); [3] late stage (14-24 days pso) 14/37 samples (38%) Samples used: serum Test operators: laboratory staff Definition of test positivity: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Visible line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result. Blinded to reference standard: NR Threshold predefined: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Positive results showed the appearance of both control line and testing line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result.
Target condition and ref-	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Gao 2020b [B] *(Continued)*

erence standard(s)	
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Comparative	
Notes	

Gao 2020b [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Index tests	Gao 2020b [C] is test [C] from the following entry: Test name: [A] CLIA; [B] GICA; [C] ELISA Manufacturer: Beier Bioengineering Company (Beijing, China) Ab targets: IgG and IgM Antigens used: spike (S) and nucleocapsid (N) proteins of 2019-nCoV Test method: [A] CLIA; [B] GICA; [C] ELISA Timing of samples: [1] early stage (1-7 days pso) 10/37 samples (27%), [2] middle stage (8-14 days pso) 13/37 samples (35%); [3] late stage (14-24 days pso) 14/37 samples (38%) Samples used: serum Test operators: laboratory staff Definition of test positivity: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Visible line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result. Blinded to reference standard: NR Threshold predefined: [A] samples with an concentration ≥ 8 arbitrary unit (AU)/mL were considered positive. [B] Positive results showed the appearance of both control line and testing line. [C] The absorbance at 450 nm (A450 nm) of each well was determined and the cut-off value was 0.10+Anegative control. A value > cut-off value was considered a positive result.
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Gao 2020b [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (A)

Study characteristics	
Patient Sampling	3-group study estimating sensitivity and specificity [1] COVID-19 patients (n = 55) [2] Pre-pandemic healthy controls (n = 45) Third group of patients admitted with a clinical and radiological diagnosis of pneumonia of unknown etiology but RT-PCR-negative reported as Garcia 2020 (B) Recruitment: NR Sample size (virus/COVID cases): 100 (55) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: [1] hospital inpatient [2] pre-pandemic controls Location: [1] Hospital Universitario Príncipe de Asturias, Madrid [2] Hospital Universitario Príncipe de Asturias Country: Spain Dates: [1] 1 March-6 April 2020 [2] 1 October-30 November 2019 Symptoms and severity: NR Sex: [1] male n = 33, 60% [2] male n = 27, 60% Age: [1] median age 63, IQR 50-79 [2] median age 55, IQR 34-66 Exposure history: NR
Index tests	Test name: AllTest COV-19 IgG / IgM kit Manufacturer: AllTest Biotech, Hangzhou, China Ab targets: IgM, IgG Antigens used: NR Test method: immunochromatography Timing of samples: days 0-14+ pso Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: RT-PCR Samples used: NR Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes: < 7 days 15% (n = 8); 7-13 days 44% (n = 24); ≥ 14 days 42% (n = 23) All participants received the same reference standard: no Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participants
Comparative	
Notes	Funding: no funding received Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared
Methodological quality	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (A) *(Continued)*

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Unclear		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (A) *(Continued)*

Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Yes	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Low risk

Garcia 2020 (B)

Study characteristics	
Patient Sampling	3-group study estimating sensitivity and specificity [3] Patients admitted with a clinical and radiological diagnosis of pneumonia of unknown etiology but RT-PCR-negative (n = 63) 2 additional cohorts extracted as separate 2-group study (Garcia 2020 (A)) Recruitment: NR Sample size (virus/COVID cases): 100 (55) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: hospital inpatient Location: Hospital Universitario Príncipe de Asturias, Madrid Country: Spain Dates: 9 February-2 April 2020 Symptoms and severity: NR Sex: male n = 47, 74% Age: median age 67, IQR 57-74 Exposure history: NR
Index tests	Test name: AllTest COV-19 IgG / IgM kit Manufacturer: AllTest Biotech, Hangzhou, China Ab targets: IgM, IgG. Antigens used: NR Test method: immunochromatography Timing of samples: days 0-14+ pso Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: clinical diagnosis of COVID-19 Criteria NR Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes: 7-13 days 29% (n = 18); ≥ 14 days 71% (n = 45) All participants received the same reference standard: yes Missing data: NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (B) *(Continued)*

	Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participants
Comparative	
Notes	Funding: no funding received Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Garcia 2020 (B) *(Continued)*

Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk
Are there concerns that the target condition as defined by the reference standard does not match the question?		Unclear
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Unclear	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Grzelak 2020 [A]

Study characteristics	
Patient Sampling	4-group study to estimate sensitivity and specificity for diagnosing active disease. [1] Hospitalised COVID-19 patients (51; 161 samples) [2] Pre-pandemic sera (491) Recruitment: NR (appears retrospective); consecutive or otherwise NR Review team excluded: [3] Blood donors during pandemic (200) [4] Cohort of 209 pauci-symptomatic suspected cases (mild signs compatible with COVID-19 -fever, cough or dyspnea) who had been in contact with a confirmed case as no reference standard reported
Patient characteristics and setting	Setting: inpatient Location: Hôpital Bichat, Paris Country: France Dates: NR
Index tests	This entry (Grzelak 2020 [A]) refers to test [A] in the list below: 5 tests evaluated: A. LIPS (S1 protein) B. LIPS (N protein) C. ELISA (N protein) D. S-Flow (unknown) E. ELISA tri-S (S protein) Manufacturer: in-house Ab targets: A. total Ab; B. total Ab; C. IgG; D IgM or IgG; E. total Ab

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Grzelak 2020 [A] *(Continued)*

	Antigens used: A. S1; B. N-based; C. full-length SARS-CoV-2 N protein; D. S at the cell surface; E. trimeric S (recombinant S glycoprotein ectodomain)
Target condition and reference standard(s)	Reference standard for cases: NR. Described as confirmed COVID-19 hospitalised cases only Samples used: not described Timing of reference standard: not described Was it blind to index test: not described
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no All participants received the same reference standard: no Missing data: pre-pandemic sera are missing from the evaluations of ELISA tri-S (n = 391), S-flow (n = 357) and LIPS S1 and N (n = 2) Sample-based analysis
Comparative	
Notes	Funding: OS lab is funded by Institut Pasteur, ANRS, Sidaction, the Vaccine Research Institute (ANR- 10-LABX-77), Labex IBEID (ANR-10-LABX-62 IBEID), "TIMTAMDEN" ANR-14-CE14-0029, "CHIKV-Viro- Immuno" ANR-14-CE14-0015-01 and the Gilead HIV cure program. LG is supported by the French Ministry of Higher Education, Research and Innovation.ME lab is funded by Institut Pasteur, Labex IBEID (ANR-10-LABX-62-IBEID), Reacting, EU grant Recover, ANR Oh'ticks. HM received core grants from the G5 Institut Pasteur Program, the Milieu Intérieur Program (ANR-10-LABX-69-01) and INSERM. C.P. is supported by a fellowship from the Agence Nationale de Recherches sur le Sida et les Hépatites Virales (ANRS). SVDW lab is funded by Institut Pasteur, CNRS, Université de Paris, Santé publique France, Labex IBEID (ANR-10-LABX-62-IBEID), REACTing, EU grant Recover. Publication status: preprint Source: medRxiv Study author COI: PC is the founder and CSO of TheraVectys

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Grzelak 2020 [A] *(Continued)*

DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	No		
Could the patient flow have introduced bias?		High risk	

Grzelak 2020 [B]

Study characteristics			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Grzelak 2020 [B] *(Continued)*

Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Index tests	This entry (Grzelak 2020 [B]) refers to test [B] in the list below; see Grzelak 2020 [A] for further study characteristics and QUADAS-2 assessments) 5 tests evaluated: A. LIPS (S1 protein) B. LIPS (N protein) C. ELISA (N protein) D. S-Flow (unknown) E. ELISA tri-S (S protein) Manufacturer: in-house Ab targets: A. total Ab; B. total Ab; C. IgG; D IgM or IgG; E. total Ab Antigens used: A. S1; B. N-based; C. full-length SARS-CoV-2 N protein; D. S at the cell surface; E. trimeric S (recombinant S glycoprotein ectodomain)
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Comparative	
Notes	

Grzelak 2020 [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Index tests	This entry (Grzelak 2020 [C]) refers to test [C] in the list below; see Grzelak 2020 [A] for further study characteristics and QUADAS-2 assessments) 5 tests evaluated: A. LIPS (S1 protein) B. LIPS (N protein) C. ELISA (N protein)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Grzelak 2020 [C] *(Continued)*

	D. S-Flow (unknown) E. ELISA tri-S (S protein) Manufacturer: in-house Ab targets: A. total Ab; B. total Ab; C. IgG; D IgM or IgG; E. total Ab Antigens used: A. S1; B. N-based; C. full-length SARS-CoV-2 N protein; D. S at the cell surface; E. trimeric S (recombinant S glycoprotein ectodomain)
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Comparative	
Notes	

Grzelak 2020 [D]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Index tests	This entry (Grzelak 2020 [D]) refers to test [D] in the list below; see Grzelak 2020 [A] for further study characteristics and QUADAS-2 assessments) 5 tests evaluated: A. LIPS (S1 protein) B. LIPS (N protein) C. ELISA (N protein) D. S-Flow (unknown) E. ELISA tri-S (S protein) Manufacturer: in-house Ab targets: A. total Ab; B. total Ab; C. IgG; D IgM or IgG; E. total Ab Antigens used: A. S1; B. N-based; C. full-length SARS-CoV-2 N protein; D. S at the cell surface; E. trimeric S (recombinant S glycoprotein ectodomain)
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Comparative	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Grzelak 2020 [D] *(Continued)*

Notes

Grzelak 2020 [E]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Index tests	This entry (Grzelak 2020 [E]) refers to test [E] in the list below; see Grzelak 2020 [A] for further study characteristics and QUADAS-2 assessments) 5 tests evaluated: A. LIPS (S1 protein) B. LIPS (N protein) C. ELISA (N protein) D. S-Flow (unknown) E. ELISA tri-S (S protein) Manufacturer: in-house Ab targets: A. total Ab; B. total Ab; C. IgG; D IgM or IgG; E. total Ab Antigens used: A. S1; B. N-based; C. full-length SARS-CoV-2 N protein; D. S at the cell surface; E. trimeric S (recombinant S glycoprotein ectodomain)
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Grzelak 2020 [A])
Comparative	
Notes	

Guo 2020a

Study characteristics	
Patient Sampling	2-group study estimating sensitivity and specificity for detection of active disease in people with suspected or confirmed SARS-Cov-2 infection and other infection controls. 1. Cases - 101 inpatients from Wuhan (43 PCR confirmed and 58 probable) provided 169 paired throat and blood samples (69 from confirmed and 100 from probable) 2. Cases - 39 inpatient confirmed cases from Beijing provided 39 samples (total of 208 samples) 3. Control samples provided by people with acute LRTI (135)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Guo 2020a *(Continued)*

	Family cluster also recruited but does not contribute data. Healthy individuals (150) used to define threshold. Additional plasma samples positive for human CoV-229E, -NL63, -OC43, -HKU1, and SARS-CoV previously obtained were included for Western Blot cross-reactivity analysis. Recruitment method NR
Patient characteristics and setting	1. Inpatients at Wuhan hospitals. 43 confirmed cases (PCR or deep sequencing): 20 severe; 23 mild to moderate; 58 possible cases (test-negative but with clinical signs, X-ray evidence): 5 severe, 53 mild to moderate. Exposure history NR 2. Beijing hospitals, China (recruitment dates January 2020); 8 severe and 31 mild to moderate. No further details 3. Acute LRTI infection controls: 135 samples from adult patients. No further detail (Family cluster of 6; aged 2-64, 3 male 3 female. Healthy control samples from Wuhan City adult health check-ups, 2018-19)
Index tests	3 ELISA assays, blinding NR In-house ELISA (indirect, laboratory-based, using blood/plasma samples. Measured IgM, IgA, IgG. Antigen: rNPs (recombinant N protein) from SARS-CoV-2 virus Test threshold determined from mean values and SD of healthy individual plasma (calculated the mean absorbance at 450 nm (A450) of the negative sera plus 3 folds of the SD values which were 0.13, 0.1 and 0.30 for IgM, IgA, and IgG, respectively. Samples acquired 1-39 days after disease onset (41/208 at 1-7 days; 84/208 at 8-14 days; 83 > 14 days pso). Person applying the test not described
Target condition and reference standard(s)	1. and 2. Confirmed cases - deep sequencing or a qPCR assay with a detection limit of 1 copy/µL, using throat swabs samples. Positivity threshold: NR. Probable cases - clinical manifestation, chest radiography imaging and epidemiology but no virus detected by deep sequencing or qPCR. Timing NR. Not blinded to index test. 3. LRTI controls: pre-pandemic samples (2018-2019)
Flow and timing	Differential verification: all cases had RT-PCR but some were negative, plus controls did not have RT-PCR. Time interval between index and reference: presumed short. There are multiple samples for some participants (cases) but others contribute only sample with a range of days pso; only data for 1-7 days pso can be disaggregated from the rest. Missing data, uninterpretable and indeterminate results not described Per participant and per sample data can be extracted
Comparative	
Notes	Funded by Chinese Academy of Medical Sciences (CAMS) Innovation Fund for Medical Sciences, Non-profit Central Research Institute Fund of CAMS, National Major Science & Technology Project for Control and Prevention of Major Infectious Diseases in China. No conflicts of interest reported Publication status: preprint

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Guo 2020a *(Continued)*

Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Guo 2020a *(Continued)*

Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Unclear risk

Hu 2020a

Study characteristics	
Patient Sampling	Single-group study to estimate sensitivity for detecting active or prior infection Confirmed COVID-19 patients (211) Recruitment: NR; likely retrospective. Consecutive or otherwise NR
Patient characteristics and setting	Setting: inpatient Location: Chongqing Three Gorges Central Hospital, Chongqing. Country: China Dates: 23 January-3 March
Index tests	Test name: Magnetic Chemiluminescence Enzyme Immunoassay (MCLIA) kit Manufacturer: Bioscience Co., Ltd (Chongqing, China) Ab targets: IgM, IgG Antigens used: N and S (nucleoprotein and a peptide from the SARS SARS-CoVCoV-2 S protein)
Target condition and reference standard(s)	Reference standard for cases: Chinese CDC guidelines (Trial Version 6); included RT-PCR Samples used: NR Timing of reference standard: unclear; appears that repeat PCR undertaken during hospitalisation; 74/211 met discharge criteria during study period (normal temperature, significantly improving respiratory symptoms and chest radiology plus 2 repeat negative PCRs with ≥ 1-day interval) Was it blind to index test: unclear
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: yes Missing data: none described; however text states 993 samples but only 409 reported for IgM and 507 for IgG Uninterpretable results: none described
Comparative	
Notes	Funding: funded by Chongqing Education Board “new coronavirus infection and prevention” emergency scientific research project

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Hu 2020a *(Continued)*

(KYYJ202006YYJ202006). Chongqing Science and Technology Bureau "new crown pneumonia epidemic emergency science and technology special" the fourth batch of projects. Famous teacher project of Chongqing talent plan
Publication status: preprint
Source: medRxiv
Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Hu 2020a *(Continued)*

Are there concerns that the target condition as defined by the reference standard does not match the question?		Low concern
DOMAIN 4: Flow and Timing		
Was there an appropriate interval between index test and reference standard?	Unclear	
Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Infantino 2020

Study characteristics	
Patient Sampling	3-group study recruiting patients estimating sensitivity and specificity [1] COVID-19 confirmed [2] Rheumatic disease or infectious disease control group (2018-19; pre COVID-19 era) [3] Blood donor control group (November/December 2019) Recruitment: unclear Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 125 (51 COVID cases) Inclusion and exclusion criteria: COVID-19 cases were confirmed by RT-PCR
Patient characteristics and setting	Setting: hospital inpatient Location: San Giovanni di Dio Hospital, Florence Country: Italy Dates: NR Symptoms and severity: 30/61 (49%) mild to moderate symptoms 31/61 (51%) with severe pneumonia required admission to the ICU Sex: [1] 26/61 (43%) male [2] 26/61 (43%) male [3] 12/20 (60%) male Age: [1] mean 59 ± 23 years; [2] mean 49 ± 17 years; [3] 44 ± 11 years Exposure history: NR
Index tests	Test name: SARS CoV-2 antibodies IgM and IgG CLIA kits (analysed with iFlash1800 fully automatic CLIA) Manufacturer: Shenzhen YHLO Biotech Co., Ltd (China) Ab targets: IgM or IgG Antigens used: N protein and S protein Test method: CLIA Timing of samples: NR Samples used: blood (discussion mentions serum) Test operators: NR Definition of test positivity: ≥ 10 AU/mL Blinded to reference standard: NR Threshold predefined: yes

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Infantino 2020 *(Continued)*

Target condition and reference standard(s)	Reference standard for cases: RT-PCR Samples used: OP and NP swabs Timing of reference standard: NR Blinded to index test: NR Incorporated index test: no Reference standard for non-cases: [2] pre-pandemic; [2] NR (contemporaneous blood donors)
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no All participants received the same reference standard: no Missing data: no Uninterpretable results: no Indeterminate results: no Unit of analysis: participant
Comparative	
Notes	Funding: NR Publication status: accepted Source: Journal of Medical Virology Study author COI: NR

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Infantino 2020 *(Continued)*

Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Unclear		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Jia 2020

Study characteristics	
Patient Sampling	Single-group study estimating sensitivity for detection of active or recent infection in people with suspected COVID-19. Patients with highly suspected COVID-19 (n = 57; 24 PCR-positive) defined by exposure history, one of: 1. the patient has a history of travel or resident in Wuhan or surrounding area, or communities with COVID-19 patients within 14 days before onset; 2. has a contact history with people infected with COVID-19 (positive NAAT) within 14 days before onset; 3. has a contact history with patients from Wuhan and surrounding areas, or has a contact history with patients who have fever or respiratory symptoms from communities with COVID-19; 4. cluster onset; and by clinical manifestations, 2 of:

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Jia 2020 *(Continued)*

	1. fever and (or) respiratory symptoms; 2. conforming to the imaging features; 3. white blood cells are normal or reduced in early stage of disease, and lymphocyte count is reduced. Second, if there is no clear epidemiological history, it meets the above 3 clinical manifestations
Patient characteristics and setting	Inpatients at > 20 hospitals of ShenZhen, China (recruitment dates NR). Sample characteristics and exposure history not described
Index tests	1 Ab test, blinding NR LFA. Time-Resolved Immunofluorescence assay (needs fluorescence analyser); Beijing Diagreat Biotechnologies Co., Ltd, Lot: 20200214). Samples and timing of sampling not described. Measured IgM and IgG; antigen not described. Threshold (Flu) for IgM ≥ 0.88 Flu and IgG ≥ 1.02 Flu. Estimated from 242 healthy people without related diseases (95% of the values were negative) Person applying the test not described
Target condition and reference standard(s)	RT-PCR using 2 kits from one of 6 companies (DAAN, Sansure Biotech, BGI, ShangHai ZJ Biotech, Geneodx, Biogerm) across 20 different hospitals. Each participant tested 3 times at different time points (24 positive on first test, all negative on 2nd and 3rd tests), using pharyngeal swabs (acquired 1-34 days from exposure to first test). Negative on all PCR tests classed as D- for purposes of this review For PCR-negative, clinical diagnosis criteria required exposure history plus 2 (1) fever and (or) respiratory symptoms; (2) conforming to the imaging features; (3) white blood cells are normal or reduced in early stage of disease, and lymphocyte count is reduced. If there was no clear epidemiological history, 3 clinical manifestations required. No guideline cited but criteria clearly defined. Blinding to index test NR
Flow and timing	All received same reference standard but not all PCR-positive; Time interval between index and reference not described. (Serology sample timing NR; PCR was 1-34 days from exposure to confirmed case. Time pso NR) No missing data, uninterpretable or indeterminate results reported Participant-based analysis
Comparative	
Notes	No funding sources described COI: none described Publication status: preprint (not peer reviewed)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Jia 2020 *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Jia 2020 *(Continued)*

Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Unclear risk

Jin 2020

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] Laboratory-confirmed COVID-19 patients (n = 43); reported separately for 27 patients while still PCR-positive and for 34 patients after becoming PCR-negative (excluded from review) [2] Patients admitted with suspected SARS-CoV-2 infection, in whom the disease was eventually excluded in the hospital and who quarantined at home, were included as a control group (n = 33) Recruitment: unclear Sample size (virus/COVID cases): 76 (43) Inclusion and exclusion criteria: suspected SARS-CoV-2 infection (fever or any respiratory symptoms, especially in those with a history of travel to Wuhan or exposure to an infected case within 2 weeks)
Patient characteristics and setting	Setting: hospital inpatients Location: Xixi Hospital of Hangzhou, Zhejiang Province Country: China Dates: January 2020-4 March 2020 Symptoms and severity: [1] COVID-19 patients: 27/43 (63%) fever; 26/43 (61%) cough; [2] non-COVID-19 patients: 24/43 (73%) fever; 15/33 (46%) cough Sex: [1] COVID-19 patients: 17/43 (40%) male. [2] Non-COVID-19 patients: 22/33 (67%) male Age: [1] COVID-19 patients: median age 47 (IQR 34–59) years; [2] non-COVID-19 patients: median age 31 (IQR 26–38) years Exposure history: [1] NR; [2] NR
Index tests	Test name: The SARS-CoV-2 IgM and IgG CLIA kits Manufacturer: Shenzhen YHLO Biotech Co., Ltd (China) Ab targets: IgM, IgG Antigens used: N protein, S protein Test method: CLIA Timing of samples: 1-55 days pso whilst still in hospital Samples used: serum Test operators: laboratory Definition of test positivity: > 10 AU/mL Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: RT-PCR testing at the Center for Disease Control of Hangzhou Samples used: oral swab or sputum Timing of reference standard: during patient care Blinded to index test: unclear Incorporated index test: no Reference standard for non-cases: 2 consecutive negative RT-PCR 24 h apart
Flow and timing	Time interval between index and reference tests: between 1 and 32 days

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Jin 2020 *(Continued)*

	Results presented by time period: days pso: 0-5 6% (n = 6); 6-10 12% (n = 12); 11-15 15% (n = 15); 16-20 22% (n = 22); 21-25 22% (n = 22); 26-30 15% (n = 15); 31-55 8% (n = 8) All participants received the same reference standard: yes Missing data: review team excluded serology data for 34 participants after becoming PCR-negative; no data reported for 16 participants while PCR-positive Uninterpretable results: none mentioned Indeterminate results: none mentioned Unit of analysis: participants overall; samples by time period
Comparative	
Notes	Funding: research Project on the Prevention and Treatment of COVID-19 in Hangzhou (establishment of a clinical diagnosis and treatment system for COVID-19 with treatment evaluation) Publication status: published paper Source: academic journal Study author COI: none mentioned

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Unclear		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Jin 2020 *(Continued)*

Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Lassauniere 2020 [A]

Study characteristics	
Patient Sampling	2-group design estimating sensitivity and specificity for 9 tests Groups: [1] COVID-19-positive group (n = 30) admitted to ICU; [2] non-COVID-19 group (n = 82) including pre-pandemic (2017) blood donors (n = 10); acute viral respiratory tract infections with other coronaviruses (n = 5) or non-coronaviruses (n = 45); dengue virus (n = 9), CMV; n = 2 and Epstein Barr virus (n = 10). 1 additional patient positive for both CMV and Epstein Barr virus Recruitment: [1] recruited consecutively (all cases in ICU on a single day); [2] unclear Sample size (virus/COVID cases): 112 (30) Inclusion and exclusion criteria: none stated

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [A] *(Continued)*

Patient characteristics and setting	Setting: [1] ICU; [2] biobank samples Location: [1] Hillerød Hospital Country: Denmark Dates: NR Symptoms and severity: NR Sex: 75% (24/32) male Age: median 67 years (IQR 52-76) Exposure history: NR
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [A]), refers to test [A] in the list below: [A] test name: Wantai SARS-CoV-2 Ab ELISA Manufacturer: Beijing Wantai Biological Pharmacy Enterprise, Beijing, China; Cat # WS-1096 Ab targets: total Ab Antigens used: SARS-CoV-2 S protein RBD Test method: ELISA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: calculated negative control value to 0.160 Blinded to reference standard: no Threshold predefined: yes [B] test name: Anti-SARS-CoV-2 IgG ELISA Manufacturer: Euroimmun Medizinische Labordiagnostika, Lübeck, Germany; Cat # EI 2668-9601 G Ab targets: IgG Antigens used: SARS-CoV-2 S protein subunit 1 (S1) Test method: ELISA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: ratio < 0.8 is considered negative, ≥ 0.8 and < 1.1 borderline, and ≥ 1.1 positive. For analysis 1.1 a more stringent cut-off was used, and all values < 1.1 were considered negative. Blinded to reference standard: no Threshold predefined: yes [C] test name: Anti-SARS-CoV-2 IgA ELISA Manufacturer: Euroimmun Medizinische Labordiagnostika, Lübeck, Germany; Cat # EI 2606-9601 A Ab targets: IgA Antigens used: SARS-CoV-2 S protein subunit 1 (S1) Test method: ELISA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: ratio < 0.8 is considered negative, ≥ 0.8 and < 1.1 borderline, and ≥ 1.1 positive. For analysis 1.1 a more stringent cut-off was used, and all values < 1.1 were considered negative. Blinded to reference standard: no Threshold predefined: yes [D] Test name: 2019-nCOV IgG/IgM Rapid Test Manufacturer: Dynamiker Biotechnology, Tianjin, China Cat # DNK-1419-1 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes [E] Test name: OnSiteTM COVID-19 IgG/IgM Rapid Test Manufacturer: CTK Biotech, Poway, CA, USA; Cat # R0180C Ab targets: IgM, IgG Antigens used: NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [A] *(Continued)*

	Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes [F] Test name: Anti-SARS-CoV-2 Rapid Test Manufacturer: AutoBio Diagnostics, Zhengzhou, China; Cat # RTA0204 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes [G] Test name: Coronavirus Diseases 2019 (COVID-19) IgM/IgG Ab Test Manufacturer: Artron Laboratories, Burnaby, Canada; Cat # A03-51-322 Ab targets: IgM, IgG. Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes [H] Test name: 2019-nCoV IgG/IgM Rapid Test Cassette Manufacturer: Acro Biotech, Rancho Cucamonga, CA, USA; Cat # INCP-402 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes [I] Test name: 2019-nCoV IgG/IgM Rapid Test Cassette Manufacturer: Hangzhou Alltest Biotech, Hangzhou, China; Cat # INCP-402 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases (including threshold): viral nucleic acid detection (no further detail) in hospital patients Samples used: respiratory Timing of reference standard: during hospital stay Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: pre-pandemic (2017)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [A] *(Continued)*

Flow and timing	Time interval between index and reference tests: unclear Results presented by time period: days since onset: 7-13 (n = 7); 14-20 (n = 15); ≥ 21 (n = 8) All participants received the same reference standard: no Missing data: some participant samples were not tested with all assays. Only 32 of the 80 control participants were tested with POC assays. Unclear how the 32 were selected Uninterpretable results: not mentioned Indeterminate results: borderline results for [2] and [3] were considered test-negative. For POC tests, weak signals for IgM and IgG were considered positive. Unit of analysis: participants
Comparative	
Notes	Funding: Danish National Biobank resource, supported by the Novo Nordisk Foundation Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [A] *(Continued)*

Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [A] *(Continued)*

Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

Lassauniere 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [B]) refers to test [B] [B] test name: Anti-SARS-CoV-2 IgG ELISA Manufacturer: Euroimmun Medizinische Labordiagnostika, Lübeck, Germany; Cat # EI 2668-9601 G Ab targets: IgG. Antigens used: SARS-CoV-2 S protein subunit 1 (S1) Test method: ELISA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: ratio < 0.8 is considered negative, ≥ 0.8 and < 1.1 borderline, and ≥ 1.1 positive. For analysis 1.1 a more stringent cut-off was used, and all values < 1.1 were considered negative. Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])

Lassauniere 2020 [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [C] *(Continued)*

Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	Nine tests evaluated, 3 ELISA and six LFIA; this entry (Lassauniere 2020 [C]) refers to test [C] [C] test name: Anti-SARS-CoV-2 IgA ELISA Manufacturer: Euroimmun Medizinische Labordiagnostika, Lübeck, Germany; Cat # EI 2606-9601 A Ab targets: IgA Antigens used: SARS-CoV-2 S protein subunit 1 (S1) Test method: ELISA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: ratio < 0.8 is considered negative, ≥ 0.8 and < 1.1 borderline, and ≥ 1.1 positive. For analysis 1.1 a more stringent cut-off was used, and all values < 1.1 were considered negative. Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [D]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [D]) refers to test [D] [D] Test name: 2019-nCOV IgG/IgM Rapid Test Manufacturer: Dynamiker Biotechnology, Tianjin, China Cat # DNK-1419-1 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [D] *(Continued)*

Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [E]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [E]) refers to test [E] [E] Test name: OnSiteTM COVID-19 IgG/IgM Rapid Test Manufacturer: CTK Biotech, Poway, CA, USA; Cat # R0180C Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [F]

Study characteristics	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [F] *(Continued)*

Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [F]) refers to test [F] [F] Test name: Anti-SARS-CoV-2 Rapid Test Manufacturer: AutoBio Diagnostics, Zhengzhou, China; Cat # RTA0204 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [G]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [G]) refers to test [G] [G] Test name: Coronavirus Diseases 2019 (COVID-19) IgM/IgG Ab Test Manufacturer: Artron Laboratories, Burnaby, Canada; Cat # A03-51-322 Ab targets: IgM, IgG. Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [G] *(Continued)*

Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [H]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [H]) refers to test [H] [H] Test name: 2019-nCoV IgG/IgM Rapid Test Cassette Manufacturer: Acro Biotech, Rancho Cucamonga, CA, USA; Cat # INCP-402 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Lassauniere 2020 [I]

Study characteristics	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lassauniere 2020 [I] *(Continued)*

Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Index tests	9 tests evaluated, 3 ELISA and 6 LFIA; this entry (Lassauniere 2020 [I]) refers to test [I] [I] Test name: 2019-nCoV IgG/IgM Rapid Test Cassette Manufacturer: Hangzhou Alltest Biotech, Hangzhou, China; Cat # INCP-402 Ab targets: IgM, IgG Antigens used: NR Test method: CGIA Timing of samples: Samples used: serum Test operators: laboratory staff Definition of test positivity: visible line Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lassauniere 2020 [A])
Comparative	
Notes	

Li 2020a

Study characteristics	
Patient Sampling	Single-group study estimating sensitivity for detection of active or recent infection Particpants with COVID-19 according to guideline of diagnosis and treatment of COVID-19 (9 Feb), 525 participants (397 PCR-positive) Data comparing results using fingerstick blood, serum and plasma for COVID-19 patients (7) and healthy volunteers (3) not extracted
Patient characteristics and setting	Samples from various hospitals and CDC testing laboratories (total 8) at 6 different provinces, China Recruitment dates NR Sample characteristics and exposure history not described
Index tests	1 Ab test, blinding not described LFIA (colloidal gold). SARS-CoV-2 rapid IgG-IgM combined Ab test kit, from Jiangsu Medomics Medical Technologies, Nanjing, China. Target: IgM and IgG, using recombinant antigen from SARS-CoV-2 S protein (MK201027) Threshold predefined, as per manufacturer Tests conducted using serum and plasma from venous blood. Samples acquired by clinical staff at each site. Timing not clearly described (dur-

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Li 2020a *(Continued)*

	ing hospital stay for inpatients); detail provided for 1 site (n = 58), sampling between day 8 and 33 pso
Target condition and reference standard(s)	COVID-19 clinically confirmed, according to guideline. (Prevention CCfDCa. The guideline of diagnosis and treatment of COVID-19. 9 February 2020). PCR test using pharyngeal (throat) swab samples and sputum (threshold NR). Timing not described Presume blinded to index test
Flow and timing	Time interval between index and reference not described. No disaggregation of results by time pso No missing data, uninterpretable or indeterminate results reported Participant-based analysis
Comparative	
Notes	Funding not described Conflicts of interest: 4 co-authors employed by Jiangsu Medomics Medical Technology Accepted for publication with full peer review

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Li 2020a *(Continued)*

Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Lin 2020a [A]

Study characteristics	
Patient Sampling	3-group study estimating sensitivity and specificity [1] COVID-19 cases (n = 79) [2] Healthy volunteers (n = 29) [3] TB patients (n = 51) Recruitment: 'Random' for [1] (method not stated), no details given for [2] and [3] Sample size (virus/COVID cases): 159 (79) Inclusion and exclusion criteria: for [1]: "combinations of epidemiological risk, clinical features and RT-PCR respiratory specimen positive"
Patient characteristics and setting	Setting: [1] specialist COVID hospital (inpatients); [2] university; [3] TB inpatient clinic Location: [1] Third People's Hospital, Shenzhen; [2] Shenzhen University; [3] Shenzhen Baoan Hospital Country: China Dates: NR Symptoms and severity: NR Sex: NR Age: [1] and [3] NR; [2] range 19-72 Exposure history: NR
Index tests	2 tests were evaluated; this entry (Lin 2020a [A]) refers to test [A] in the list below

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lin 2020a [A] *(Continued)*

	Test name: [A] not named; [B] commercial ELISA kit Manufacturer: [A] in-house; [B] Darui Biotech, China Ab targets: [A] and [B]: IgM, IgG Antigens used: [A] recombinant nucleocapsid (YP_009724397.2); [B] SARS-CoV-2 N protein Test method: [A] CLIA; [B] ELISA Timing of samples: 0 to > 14 days (maximum NR) pso Samples used: serum Test operators: NR (assume laboratory staff) Definition of test positivity: [A] IgM (RLU 162296); IgG (RLU 336697) [B] manufacturer's recommendation Blinded to reference standard: not mentioned Threshold predefined: [A] threshold derived from ROC curve; [B] yes (QUADAS ratings are for ELISA test)
Target condition and reference standard(s)	Reference standard: RT-PCR: GeneoDX kit (Taqman RT-PCR method, targeting the ORF1ab 101 and N genes) [2] and [3] were persistently negative in at least 3 tests. Samples used: respiratory Timing of reference standard: presume on presentation Blinded to index test: NR Incorporated index test: no
Flow and timing	Time interval between index and reference tests: unclear Results presented by time period:days 1-7 (15%); 8-13 (42%); 14+ (43%) All participants received the same reference standard: yes Missing data: 65/79 D+ serum samples available for ELISA; 64/80 D- serum samples available for ELISA; reason not given Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participants
Comparative	
Notes	Funding: Guangdong Provincial Science and Technology Program, National Natural Science Funds of China, Shenzhen University and the National Science and Technology Major Project Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lin 2020a [A] *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lin 2020a [A] *(Continued)*

Could the patient flow have introduced bias?	High risk

Lin 2020a [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lin 2020a [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lin 2020a [A])
Index tests	2 tests were evaluated; this entry (Lin 2020a [B]) refers to test [B] in the list below Test name: [A] not named (CLIA); [B] commercial ELISA kit Manufacturer: [A] in-house; [B] Darui Biotech, China Ab targets: [A] and [B]: IgM, IgG Antigens used: [A] recombinant nucleocapsid (YP_009724397.2); [B] SARS-CoV-2 N protein Test method: [A] CLIA; [B] ELISA Timing of samples: 0 to > 14 days (maximum NR) pso Samples used: serum Test operators: NR (assume laboratory staff) Definition of test positivity: [A] IgM (RLU 162296); IgG (RLU 336697) [B] manufacturer's recommendation Blinded to reference standard: not mentioned Threshold predefined: [A] threshold derived from ROC curve; [B] yes (QUADAS ratings are for ELISA test)
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lin 2020a [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lin 2020a [A])
Comparative	
Notes	See main entry for this study for characteristics and QUADAS-2 assessment (Lin 2020a [A])

Lippi 2020 [A]

Study characteristics	
Patient Sampling	1-group study recruiting patients estimating sensitivity and specificity [1] Suspected COVID-19; subgroup of confirmed cases included Recruitment: consecutive patients Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 131 (NR); subgroup of 48 confirmed cases included Inclusion and exclusion criteria: suspected COVID-19 patients hospitalised, in whom NP and OP swabs were collected along with blood samples during hospital stay, for purposes of COVID-19 diagnosis and/or monitoring

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lippi 2020 [A] *(Continued)*

Patient characteristics and setting	Setting: hospital inpatients Location: University Hospital of Verona Country: Italy Dates: NR Symptoms and severity: NR Sex: 60/131 (46%) male Age: mean 56 ± 21 years Exposure history: NR
Index tests	2 tests were evaluated; this entry (Lippi 2020 [A]) refers to test [A] in the list below Test name: [A] MAGLUMI 2019-nCoV IgG and IgM (2 indirect tests) [B] Anti-SARS-CoV-2 IgA and IgG ELISA Manufacturer: [A] SNIBE – Shenzhen New Industries Biomedical Engineering Co., Ltd, Shenzhen, China [B] Euroimmun AG, Lübeck, Germany Ab targets: [A] IgM or IgG ; [B] IgA or IgG Antigens used: [A] CoV-S (spike) and e CoV-N (nucleocapsid); [B] NR Test method: [A] CLIA; [B] ELISAs Timing of samples: NR Samples used: blood, serum or plasma Test operators: NR Definition of test positivity: [A] ≥ 1.10 AU/mL [B] ≥ 1.1 (absorbance of patient sample/absorbance of calibrator) Blinded to reference standard: NR Threshold predefined: yes by manufacturer
Target condition and reference standard(s)	Reference standard for cases: RT-PCR (commercial RT-PCR method, Seegene AllplexTM2019-nCoV Assay) Samples used: venous blood Timing of reference standard: during hospital stay Blinded to index test: NR Incorporated index test: no Reference standard for non-cases: same reference standard, single-group
Flow and timing	Time interval between index and reference tests: both during hospital stay Results presented by time period: no All participants received the same reference standard: yes Missing data: NR Uninterpretable results: NR Indeterminate results: 36 Inconclusive results Unit of analysis: per patient
Comparative	
Notes	Funding: none declared Publication status: published letter Source: Clinical Chemistry and Laboratory Medicine Study author COI: study authors state no conflict of interest

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lippi 2020 [A] *(Continued)*

Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lippi 2020 [A] *(Continued)*

Did all patients receive the same reference standard?	Yes	
Were all patients included in the analysis?	Yes	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Low risk

Lippi 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lippi 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lippi 2020 [A])
Index tests	2 tests were evaluated; this entry (Lippi 2020 [B]) refers to test [B] in the list below Test name: [A] MAGLUMI 2019-nCoV IgG and IgM (2 indirect tests) [B] Anti-SARS-CoV-2 IgA and IgG ELISA Manufacturer: [A] SNIBE – Shenzhen New Industries Biomedical Engineering Co., Ltd, Shenzhen, China [B] Euroimmun AG, Lübeck, Germany Ab targets: [A] IgM or IgG ; [B] IgA or IgG Antigens used: [A] CoV-S (spike) and e CoV-N (nucleocapsid); [B] NR Test method: [A] CLIA (CLIAs); [B] ELISA Timing of samples: NR Samples used: blood, serum or plasma Test operators: NR Definition of test positivity: [A] ≥1.10 AU/mL [B] ≥1.1 (absorbance of patient sample/absorbance of calibrator Blinded to reference standard: NR Threshold predefined: yes by manufacturer
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lippi 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lippi 2020 [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020a

Study characteristics	
Patient Sampling	Described as one group to estimate sensitivity and specificity (but unclear whether actually recruited as 2 groups) [1]. RT-PCR confirmed COVID-19 patients (n = 90) [2]. (a) COVID-19 suspects with RT-PCR-negative results (n = 25) and [2]. (b) inpatients with 'other disease' with RT-PCR-negative results (n = 64) Recruitment: unclear Sample size (virus/COVID cases): 179 (90 confirmed; data for 5 clinically confirmed included as D+) Inclusion and exclusion criteria:
Patient characteristics and setting	All participants considered COVID-19 suspects (criteria NR) Setting: hospital (inpatients and outpatients) Location: General Hospital of Central Theatre Command, Hubei Province Country: China Dates: 1 January to 12 March 2020 Group [1] Symptoms and severity: 46 mild/common cases; 44 severe/critical cases Sex: M/F: 60:30 (67%) Age: Age: mean 76 (SD 15) years Exposure history: NR. Group [2] [2a] Diagnoses: COVID-19 diagnoses: 5 confirmed; 20 suspected. [2b] Non-COVID-19 diagnosis: n = 64 (10 cases of Sjogren's syndrome, 8 cases of diabetes, 6 cases of systemic lupus erythematosus, 5 cases of rheumatoid arthritis, 2 cases of dermatomyositis, 2 cases of connective tissue disease, 1 case of scleroderma, and 30 cases of common injuries with no underlying diseases) Sex: M/F: 38:51 (35%) Age: mean 56 (SD 21) years Exposure history: NR
Index tests	Test name: SARS-CoV-2 IgG/IgM Ab test kit Manufacturer: A 'Chinese biotechnology company" Ab targets: IgM, IgG Antigens used: NR Test method: LFA (CGIA) Timing of samples: time pso to sample collection mean (SD) (days): PCR-postiive 30 (17), PCR-negative 18 (14) Samples used: serum Test operators: NR, but suspect in laboratory (as serum was used) Definition of test positivity: visible line Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases (including threshold): RT-PCR test positive or 'clinically confirmed' Samples used: nasal and pharyngeal swabs Timing of reference standard: NR Blinded to index test: NR Incorporated index test: NR Reference standard for non-cases [2b]: RT-PCR test negative and diagnosis of alternative condition
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: known for 115 cases: 0-7 days: n = 25 (22%); 8-15 days n = 8 (7%); ≥ 16 days n = 82 (71%) All participants received the same reference standard: no

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020a *(Continued)*

	Missing data: none mentioned Uninterpretable results: none mentioned Indeterminate results: none mentioned Unit of analysis: participants
Comparative	
Notes	Funding: none reported Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none reported

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020a *(Continued)*

Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Liu 2020b

Study characteristics	
Patient Sampling	2-group study estimating sensitivity and specificity for diagnosing active disease. [1]. Consecutively recruited cohort of patients with confirmed or suspected COVID-19 (n = 238; 153 PCR confirmed) [2]. Cohort of ordinary patients (n = 70); [3]. Cohort of randomly sampled healthy blood donors (n = 50) randomly sampled No further details
Patient characteristics and setting	[1]. Inpatients at General Hospital of Central Theater Command of People's Liberation Army (PLA), China (recruitment dates 6-14 February 2020). Symptoms included fever (87%); dry cough (54%); fatigue (33%). 235/238 (99%) had CT ground glass opacity/patchy shadowing. Exposure history not described. Median age 55 [IQR 38.3-65] years; 58% male [2]. Ordinary patients, characteristics not described. [3]. Healthy blood donors (n = 50), characteristics not described
Index tests	2 Ab tests, blinding NR Both laboratory-based a. ELISA kit (Lizhu, Zhuhai, China). Measured IgG and IgM detected using recombinant (rN) protein of SARS-CoV-2. Test threshold: NR, presumed as per manufacturer

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020b *(Continued)*

	b. In-house CLIA Serum samples acquired 17 (7%) day 0-5; 41 (17%) day 6-10; 21 (9%) day 11-12; 48 (20%) day 13-15; 111 (47%) day ≥ 16
Target condition and reference standard(s)	1. RT-PCR (Daan Gene) targeting ORF1ab and N gene; Ct-value ≤ 40 was defined as a positive test result. Pharyngeal swab specimens used Clinical diagnosis of highly-suspected cases according to General Office of National Health Committee notice (General Office of National Health Committee. Office of State Administration of Traditional Chinese Medicine. Notice on the issuance of strategic guidelines for diagnosis and treatment of novel coronavirus (2019-nCoV) infected pneumonia (Fifth edition draft) (2020-02-09) [EB/OL]) Timing: clinical diagnosis presumed on admission. RT-PCR sampling - 54 (23%) day 0-5; 71 (30%) day 6-10; 28 (12%) day 11-12; 35 (15%) day 13-15; 50 (21%) day ≥ 16 2. No reference standard described for 'ordinary' patients or healthy controls
Flow and timing	Time interval between index and reference NR, but within hospital stay. Data are disaggregated by time pso but different participants contributed samples at each time. No missing data, uninterpretable or indeterminate results described. Basis for analysis: participants
Comparative	
Notes	Funded by National Natural Science Foundation of China; National Key Research and Development Program of China; and the China Postdoctoral Science Foundation. Wuhan Institute of Virology of Chinese Academy of Sciences and Zhuhai Lizhu Diagnostics Inc. for providing assistance in ELISA detection. Conflicts of interest: Zhuhai Lizhu Diagnostics Inc. acknowledged in Funding statement. Preprint (not peer reviewed): medRxiv

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020b *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Liu 2020c

Study characteristics	
Patient Sampling	Single-group study to determine sensitivity in acute phase sera.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020c *(Continued)*

	Cohort of 133 patients diagnosed with SARS-Cov-2 according to the "pneumonia diagnosis protocol for novel coronavirus infection (trial version 5)". Inclusion and exclusion criteria not further described
Patient characteristics and setting	Inpatients at Renmin Hospital (Wuhan University), China (recruitment dates 17 February-1 March 2020). Severity of condition classified as moderate 44, 33%; severe 52, 39%; critical 37, 29%. Median age (range) per group: moderate 67.5 years (64 to 71.5 years); severe 68 years (61.25 to 74); critical 70 years (60 to 76.5). Male 70, 53% Exposure history not described
Index tests	One Ab test, blinding NR Laboratory-based evaluation of CLIA (details as per company contact) to measure IgG and IgM - SARS-CoV-2 Ab detection kit (iFLash-SARS-CoV-2 IgG/IgM CLIA) (YHLO Biotech, Shenzhen), using serum samples. Antigen used NR Sample timing not described
Target condition and reference standard(s)	1. Clinical diagnosis according to established protocol (not cited but appears to be Chinese Government-issued - National Health Commission of the People's Republic of China, pneumonia diagnosis protocol for novel coronavirus detection (trial version 5)) 2. RT-PCR (ORF1ab/N qPCR detection kit from GeneoDx Biotech, Shanghai, China). 2 tests per participant but number of positive tests required NR. Samples not described, but Table 2 refers to 'NP', which could be NP samples. Positivity threshold not described
Flow and timing	Time interval between index and reference standard not described; time pso not described No missing data, uninterpretable or indeterminate results described Basis for analysis: participants
Comparative	
Notes	Funded by National Natural Science Foundation of China (81672079 to CZ and 31800147 to ZL), the Open Research Fund Program of the State Key Laboratory of Virology of China (2019KF001 to ZL), the Outstanding Leaders Training Program of Pudong Health Bureau of Shanghai (PWR12018-05 to XL), and the Key Disciplines Group Construction Project of Pudong Health Bureau of Shanghai (PWZxq2017-15 to XL) No conflicts of interest declared Preprint (not peer reviewed): medRxiv

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020c *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020d [A]

Study characteristics	
Patient Sampling	2-group study to estimate sensitivity and specificity in acute and convalescent phase sera 1. RT-PCR confirmed COVID-19 cases (n = 214) 2. Healthy blood donors (n = 100) Retrospective design; recruitment method NR. No further detail
Patient characteristics and setting	[1] Inpatients at General Hospital of the Central Theater Command of the People's Liberation Army (PLA), China (recruitment dates 18 January-26 February). Exposure history and participant characteristics not described [2] Healthy blood donors; not further described
Index tests	2 Ab tests, blinding NR; this entry (Liu 2020d [A]) refers to test [A] in the list below Laboratory-based evaluations of ELISA assays measuring IgM and IgG using serum samples: A. rN-based ELISA (Lizhu, Zhuhai, China), using recombinant N protein B. rS-based ELISA (Hotgen, Beijing, China), using receptor-binding domain of the recombinant S polypeptide (rS) Test thresholds: A. cut-off calculated by summing 0.100 (IgM) or 0.130 (IgG) and the average A450 of negative control replicates. When A450 < cut-off value, the test was considered negative, and when A450 was ≥ cut-off value, the test was considered positive. B. cut-off values (IgM and IgG) calculated by summing 0.250 and the average A450 of negative control replicates. When A450 < cut-off value, the test was considered negative, and when A450 was ≥ cut-off value, the test was considered positive. Samples acquired 0-5 d 22, 10%; 6-10 d 38, 18%; 11-15 d 54, 25%; 16-20 d 55, 26%; ≥ 21 d 45, 21% (32/45 are d 21-30). Person applying the test not described
Target condition and reference standard(s)	[1] RT-PCR (no further detail), using pharyngeal swabs samples. Positivity threshold NR. Samples acquired at a median of 15 d pso (range 0–55 days) 2. Healthy blood donors; no description of timing of serum sample collection
Flow and timing	Sampling for index and reference for cases was conducted within same time frame. No missing data, uninterpretable or indeterminate results described Basis for analysis: participants. Includes a single sample per participant with results disaggregated by time pso, but different participants contributed data to each time period.
Comparative	
Notes	Supported by the National Natural Science Foundation, the China Postdoctoral Science Foundation (2019M664008), and the Wuhan Young and Middle-aged Medical Backbone Talents Training Project (Wuweitong [2019] 87th266) Accepted manuscript (Journal of Clinical Microbiology) No conflicts of interest declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020d [A] *(Continued)*

Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Liu 2020d [A] *(Continued)*

Did all patients receive the same reference standard?	No	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		High risk

Liu 2020d [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Liu 2020d [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Liu 2020d [A])
Index tests	2 Ab tests, blinding NR; this entry (Liu 2020d [B]) refers to test [B] in the list below Laboratory-based evaluations of ELISA assays measuring IgM and IgG using serum samples A. rN-based ELISA (Lizhu, Zhuhai, China), using recombinant N protein B. rS-based ELISA (Hotgen, Beijing, China), using receptor-binding domain of the recombinant S polypeptide (rS) Test thresholds: A. cut-off calculated by summing 0.100 (IgM) or 0.130 (IgG) and the average A450 of negative control replicates. When A450 < cut-off value, the test was considered negative, and when A450 was ≥ cut-off value, the test was considered positive. B. cut-off values (IgM and IgG) calculated by summing 0.250 and the average A450 of negative control replicates. When A450 < cut-off value, the test was considered negative, and when A450 was ≥ cut-off value, the test was considered positive. Samples acquired 0-5 d 22, 10%; 6-10 d 38, 18%; 11-15 d 54, 25%; 16-20 d 55, 26%; ≥ 21 d 45, 21% (32/45 are d 21-30). Person applying the test not described
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Liu 2020d [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Liu 2020d [A])
Comparative	
Notes	

Long 2020 (A)

Study characteristics

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Long 2020 (A) *(Continued)*

Patient Sampling	Single-group study to estimate sensitivity and specificity for detection of active or prior infection Cohort of close contacts (n = 164, 23 cases) of 2 index cases (diagnosis confirmed 4 February 2020; contacts between 20 January-6 February 2020 identified and PCR tested) Additional cohorts reported but not extracted included: a. follow-up cohort in RT-PCR-positive confirmed cases sampling every 3 days (n = 63 subset of cross-sectional study); does not provide accuracy data b. cohort of RT-PCR-negative suspects (n = 52); did not provide full accuracy data (specificity only could be extracted) c. extracted as Long 2020 (B)
Patient characteristics and setting	Close contacts identified by Chongqing CDC in Wanzhou (n = 164), China PCR testing conducted 31 January-9 February; serum samples collected 2 March 2020 13 (8%) symptomatic, 151 asymptomatic; no further details
Index tests	One Ab test, blinding NR Laboratory-based evaluated of magnetic CLIA kit (Bioscience (Chongqing) Co., Ltd), measuring IgM and IgG in serum samples, using recombinant antigen containing nucleoprotein and a peptide from S protein. Test threshold not described; presume interpretation according to manufacturer's instructions. Sample timing: 21-31 days after PCR test
Target condition and reference standard(s)	RT-PCR using nasal and pharyngeal swab specimens during hospital stay. No further detail. Theshold for positivity NR Timing of reference standard sampling: within 17-day period after contact with confirmed cases
Flow and timing	Time interval between index and reference: index 21-30 days after PCR test, potential for repeat exposure during this time. No missing data, uninterpretable or indeterminate results reported Participant-based analysis
Comparative	
Notes	Funded by Emergency Project from the Science & Technology Commission of Chongqing; The Major National S&T programme grant from Science & Technology Commission of China. No conflicts of interest reported; 1 author from BioScience Co. Ltd, Chongqing, China Preprint (not peer reviewed)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Long 2020 (A) *(Continued)*

Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		Low risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	No		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Yes		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Low risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Long 2020 (B)

Study characteristics	
Patient Sampling	Single-group study to estimate sensitivity for diagnosing acute phase infection RT-PCR-positive confirmed cases (n = 285). No further detail of inclusion or exclusion criteria. Additional cohorts reported but not extracted included: a. follow-up cohort in RT-PCR-positive confirmed cases sampling every 3 days (n = 63 subset of cross-sectional study); does not provide accuracy data b. cohort of RT-PCR-negative suspects (n = 52); did not provide full accuracy data (specificity only could be extracted) c. cohort of asymptomatic contacts of 2 confirmed cases extracted as Long 2020 (A)
Patient characteristics and setting	Inpatients at 3 hospitals, Chongqing Three Gorges Central Hospital (TGH) (n = 158), Yongchuan Hospital Affiliated to Chongqing Medical University (YCH) (n = 75), and The Public Health Center of Chongqing (PHCC), China (n = 52), recruited 5 February 2020 Median age 47 years (IQR 34-56 years); 55.4% male. 39/285 (14%) severe or critical in ICU. 103/285 (36%) patients had an history of exposure to transmission sources
Index tests	One Ab test, blinding NR Laboratory-based evaluated of magnetic CLIA kit (Bioscience (Chongqing) Co., Ltd), measuring IgM and IgG in serum samples, using recombinant antigen containing nucleoprotein and a peptide from S protein. Test threshold not described; presume interpretation according to manufacturer's instructions Sample timing: 67/363 (18%) day 2-7 from symptom onset; 149 (41%) day 8-13; and 147 (40%) day 14+
Target condition and reference standard(s)	RT-PCR using nasal and pharyngeal swab specimens during hospital stay. No further detail. Theshold for positivity NR Timing of reference standard sampling NR
Flow and timing	Time interval between index and reference NR. Data are disaggregated by time period but different participants contributed samples at each time pso Missing data: 23 participants with no information on time pso were excluded leaving 363 samples from 262 participants No uninterpretable or indeterminate results reported Basis for analysis: samples
Comparative	
Notes	Funded by Emergency Project from the Science & Technology Commission of Chongqing; The Major National S&T programme grant from Science & Technology Commission of China No conflicts of interest declared; 1 study author from BioScience Co. Ltd, Chongqing, China Preprint paper (not peer reviewed)

Methodological quality			
Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Long 2020 (B) *(Continued)*

Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Long 2020 (B) *(Continued)*

Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	No
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

Lou 2020 [A]

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] n = 80 confirmed COVID cases [2] n = 300 healthy people enrolled from the community Recruitment: Prospective or retrospective recruitment of cases: Sample size (virus/COVID cases): 380 (80) Inclusion and exclusion criteria: willing to donate blood
Patient characteristics and setting	Setting: inpatient Location: First affiliated hospital of Zhejiang University Country: China Dates: 19 January-9 February 2020 Symptoms and severity: n = 26. Critical case = any one of a) ARDS or oxygen saturation < 93% and needing mechanical ventilation invasively or non-invasively; b) shock; c) complication of organ failure requiring ICU support N= 54 non-critical case (not meeting criteria a) or b) or c) above Sex: 38.7% female Age: 55 years (IQR 45-64) Exposure history: for 45/80: incubation period (defined as interval between earliest date of SARS-Cov-2 exposure (unambiguous close contact with confirmed COVID-19 case) and earliest date of symptom onset) range 0-23 days, median 5 (IQR 2–10)
Index tests	3 tests evaluated, this entry (Lou 2020 [A]) refers to test [A] Test name: [A] ELISA; [B] CGIA; [C] CLIA Manufacturer: NR Ab targets: Ab; IgM; IgG Antigens used: IgM and Ab: RBD of the SARS-CoV-2 S protein IgG: indirect immunoassays using recombinant nucleoprotein of SARS-CoV-2 Test method: ELISA, CLIA; LFIA Timing of samples: between 0 and 29 days pso Samples used: serum Test operators: NR Definition of test positivity: NR Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: confirmed case should meet 3 criteria: 1) fever and/or respiratory symptoms; 2) abnormal lung imaging findings; and 3) positive result of the nucleic acid of SARS-CoV-2

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lou 2020 [A] *(Continued)*

	Samples used: deep sputum Timing of reference standard: on admission Blinded to index test: unclear Incorporated index test: unclear Reference standard for non-cases: NR
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: unclear Missing data: [1] 36, 71 and 58/80 contributed to 0-7, 8-14 and 15-29 days pso estimates of sensitivity for tests [A], [B] and [C] only [2] Not all control group participants were tested by all index tests (range 100-300/300) Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	Funding: China National Mega-Projects for Infectious Diseases and the Science and Technology Major Project of Xiamen Publication status: preprint Source:Pre print server (medRxiv) Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lou 2020 [A] *(Continued)*

Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Unclear		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Unclear		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Lou 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lou 2020 [B] *(Continued)*

Index tests	3 tests evaluated, this entry (Lou 2020 [B]) refers to test [B] Test name: [A] ELISA; [B] CGIA; [C] CLIA Manufacturer: NR Ab targets: Ab; IgM; IgG Antigens used: IgM and Ab: RBD of the SARS-CoV-2 S protein IgG: indirect immunoassays using recombinant nucleoprotein of SARS-CoV-2 Test method: ELISA, CLIA; LFIA Timing of samples: between 0 and 29 days pso Samples used: serum Test operators: NR Definition of test positivity: NR Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Comparative	
Notes	

Lou 2020 [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Index tests	3 tests evaluated, this entry (Lou 2020 [C]) refers to test [C] Test name: [A] ELISA; [B] CGIA; [C] CLIA Manufacturer: NR Ab targets: Ab; IgM; IgG Antigens used: IgM and Ab: RBD of the SARS-CoV-2 S protein IgG: indirect immunoassays using recombinant nucleoprotein of SARS-CoV-2 Test method: ELISA, CLIA; LFIA Timing of samples: between 0 and 29 days pso Samples used: serum Test operators: NR Definition of test positivity: NR Blinded to reference standard: unclear Threshold predefined: yes
Target condition and ref-	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Lou 2020 [C] *(Continued)*

erence standard(s)	
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Lou 2020 [A])
Comparative	
Notes	

Ma 2020a

Study characteristics	
Patient Sampling	4-group study recruiting patients estimating sensitivity and specificity [1] n = 87 confirmed COVID-19 (216 samples) [2] n = 330 healthy donors pre-October 2019 [3] n = 138 'other diseases' (no mention of PCR) [4] n = 15 suspected COVID pneumonia but negative PCR Recruitment: cases admitted between 26 January-5 March 2020 Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 570 (87) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: inpatient Location: First Affiliated Hospital of USTC Hospital and the First Affiliated Hospital of Anhui Medical University Country: China Dates: 26 January-5 March 2020 Symptoms and severity: 56/87 clinically moderate, 17 severe, 5 critical, "few mild" Sex: NR Age: NR Exposure history: NR
Index tests	Test name: CLIA RBD Manufacturer: in-house Ab targets: IgM;IgG;IgA Antigens used: SARS CoV-2 RBD protein (S-based) Test method: CLIA Timing of samples: during 'routine inpatient testing' Samples used: serum Test operators: NR Definition of test positivity: NR Blinded to reference standard: unclear Threshold predefined: no
Target condition and reference standard(s)	Reference standard for cases: New Coronavirus Pneumonia Prevention and Control Program (7th edition) published by the National Health Commission of China, RT-qPCR was used to confirm COVID-19 (all cases were RT-PCR-positive) Samples used: serum Timing of reference standard: during 'routine inpatient testing' Blinded to index test: unclear Incorporated index test: no Reference standard for non-cases: [2] Pre-pandemic [3] NR [4] NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Ma 2020a *(Continued)*

Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: no Missing data: for comparison of sensitivity and specificity of 2 antigens only 20/total of 479 control sera were used (20/138 from 'other disease' group Uninterpretable results: NR Indeterminate results: NR Unit of analysis: samples
Comparative	
Notes	Funding: T.J. is supported by the Strategic Priority Research Program of the Chinese Academy of Sciences (XDB29030104), National Natural Science Fund (Grant No.: 31870731 and U1732109), the Fundamental Research Funds for the Central Universities (WK2070000108). TJ and XLM is supported by a COVID-19 special task grant supported by Chinese Academy of Science Clinical Research Hospital (Hefei) with Grant No. YD2070002017 and YD2070002001, respectively. M.H. is supported by the new medical science fund of USTC (WK2070000130). Publication status: preprint Source: preprint server: medRxiv Study author COI: 3 study authors are employees of Kangrun Biotech LTD (Guangzhou, 308 China). 4 study authors have jointly applied for a patent related to the Ab detecting kits.

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Ma 2020a *(Continued)*

Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Yes		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	No		
Could the patient flow have introduced bias?		High risk	

Okba 2020a

Study characteristics	
Patient Sampling	2-group design estimating sensitivity and specificity in acute disease [1] SARS-CoV-2 cases confirmed by RT-PCR (n = 9, 31 samples) [2] Healthy blood donors (n = 45) date NR Recruitment method and exclusion criteria NR Third group of RT-PCR confirmed cases from France (n = 3, 10 samples excluded by review author team)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Okba 2020a *(Continued)*

Patient characteristics and setting	[1] Inpatient (plus initial testing prior to admission) at hospital in Munich, Germany. Cases are epidemiologically linked, identified through exposure to known cases, and occurred after 23 January 2020, discovered on 27 January (Woelfel 2020). Symptoms and severity, and demographics NR [2] Sanquin Blood Bank, Netherlands, date not specified
Index tests	Beta version of commercial EuroImmun IgA and IgG ELISA Ab test, from EUROIMMUN Medizinische Labordiagnostika AG. Targets IgA and IgG. Threshold not pre-defined: in-house threshold of mean background reactivity of all SARS-CoV-2–negative serum samples in the study multiplied by 3. Blinding NR
Target condition and reference standard(s)	[1] All positive on RT-PCR between days 1-5 of symptom onset, using OP or NP swab. Blind to index test [2] Blood bank samples, reported as negative but date of sampling NR
Flow and timing	Different reference standard for cases and controls, and cases were from 2 separate cohorts. Limited details available for each cohort. Results available by case, but only in graph format Indeterminate or unclear index results on graphs considered negative by review team
Comparative	
Notes	No information provided on study author conflicts. Published as early release (not final). Report the following funding "Zoonoses Anticipation and Preparedness Initiative (project Innovative Medicines Initiative grant no. 115760), the Innovative Medicines Initiative; the European Commission, and partners of the European Federation of Pharmaceutical Industries and Associations"

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Okba 2020a *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Padoan 2020

Study characteristics	
Patient Sampling	1-group study recruiting patients estimating sensitivity [1] Hospitalised patients with confirmed COVID-19 Recruitment: cases with residual serum samples collected between 18 March-26 March 2020 Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 37 (37) Inclusion and exclusion criteria:

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Padoan 2020 *(Continued)*

Patient characteristics and setting	Setting: inpatient Location: University Hospital of Padova Country: Italy Dates: 18 March-26 March 2020 Symptoms and severity: NR Sex: NR Age: NR Exposure history: NR
Index tests	Test name: MAGLUMI 2000 Plus nCoV IgM and IgG Manufacturer: New Industries Biomedical Engineering Co., Ltd [Snibe], Shenzhen, China Ab targets: IgM; IgG Antigens used: NR Test method: CLIA Timing of samples: days since symptom onset: ≤ 5 days 4/37 (11%) 6-7 days 6/37 (16%) 0-7 days: 10/37 (27%) 8-9 days 12/37 (32%) 10-11 days 14/37 (38%) 12-13 days 9/37 (24%) 8-13 days: 35/37 (95%) > 13 days 25/37 (68%) Samples used: serum Test operators: NR Definition of test positivity: [A] IgM 1.0 AU/mL [B] IgG 1.1 AU/mL Blinded to reference standard: no Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: PCR Samples used: NP Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: N/A
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: yes Missing data: text describes 87 samples from 37 participants but only 70 samples reported per time period and no per participant data are reported Uninterpretable results: NR Indeterminate results: NR Unit of analysis: sample
Comparative	
Notes	Funding: none declared Publication status: published Source: academic journal Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Padoan 2020 *(Continued)*

DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Padoan 2020 *(Continued)*

Did all participants receive a reference standard?	Yes	
Were results presented per patient?	No	
Could the patient flow have introduced bias?		High risk

Pan 2020a

Study characteristics	
Patient Sampling	Single group of cases to estimate sensitivity in acute disease SARS-CoV-2-positive cases (n = 105, 134 samples) of which 67 cases (86 samples) confirmed by RT-PCR, and 37 patients (39 samples) clinically diagnosed (RT-PCR-negative, radiography-positive) Recruitment method NR Exclusion criteria NR
Patient characteristics and setting	Inpatients in Zhongnan hospital (Wuhan University, China). Testing 6 February-23 February 2020, symptom onset 7 January-18 February 2020 (for subgroup of 108) 48 male, 57 female, median age 58 years (range 20-96). Symptoms and severity and exposure status NR
Index tests	Commercial Ab test LFA (conducted in laboratory setting). Colloidal gold-based immunochromatographic strip assay (Zhuhai Livzon Diagnositic Inc) to detect IgM, IgG. Antigen used NR (as per manufacturer) Presence of T line indicating positive Serum or plasma samples used (includes comparison with whole blood for subgroup; not extracted). No information on timing or who read the test results.
Target condition and reference standard(s)	1. RT-PCR following WHO guidelines for qRT-PCR, using throat swabs (Chinese CDC recommended kit used, BioGerm, Shanghai, China) 2. clinically diagnosed as SARS-CoV-2 infection according to the 5th edition of guideline on diagnosis and treatment of the novel coronavirus pneumonia. Specifically, the clinical diagnosis means the suspected cases were negative to the real-time RT-PCR test but presented viral pneumonia by radiography Samples taken during inpatient stay but no details about timing or personnel for test interpretation
Flow and timing	All participants received a reference standard, but there was differential verification with some patients confirmed by RT-PCR and others RT-PCR-negative but confirmed by radiography. Subset who were RT-PCR-positive are reported separately. Timing of index tests and reference standard unclear. Data reported only for those with symptom onset information; 26 samples excluded. No reporting of test failures or indeterminate results. Per-sample analysis; multiple samples (2 or 3) per participant disaggregated over time
Comparative	
Notes	Funding from the National Key Research and Development Program of China (2018YFE0204500) Declared no conflict of interest Published in the Journal of Infection

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Pan 2020a *(Continued)*

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Pan 2020a *(Continued)*

DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Unclear
Did all patients receive the same reference standard?	Yes
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	Unclear risk

Paradiso 2020a

Study characteristics	
Patient Sampling	Single-group study to estimate sensitivity and specificity for diagnosing SARS-Cov-2 [1] Cohort of patients attending A&E with COVID-19-like symptoms Recruitment: consecutive Sample size (virus/COVID cases): 191 (70) Inclusion and exclusion criteria: no further details
Patient characteristics and setting	Setting: A&E Location: Ospedale Policlinico Consorziale of Bari Country: Italy Dates: 23-29 March 2020 Symptoms and severity: 14/160 (9%) asymptomatic; symptoms not available for 31/191 Sex: 116, 60.6% male Age: median 58.5 years Exposure history: NR
Index tests	Test name: VivaDiag Manufacturer: Jiangsu Medomics Medical Technologies Ab targets: IgM, IgG Antigens used: surface antigen from SARSCoV-2 POC or laboratory: POC Test method: LFA (CGIA) Timing of samples: on presentation; time from symptom onset varied from asymptomatic 14, 9%; d 0-5 97, 61%; d 6-8 17, 11%; d 9-10 21, 13%; d 11-15 5, 3%, > 15 d 6, 5%; NR 31, 19%) Samples used: venous blood Test operators: 2 operators in the laboratory (operators obtained images of the device and disagreements evaluated by a third party) Definition of test positivity: presence of red/purple line in the specific region indicated on the device Blinded to reference standard: yes Threshold predefined: as per manufacturer

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Paradiso 2020a *(Continued)*

Target condition and reference standard(s)	Reference standard for cases including threshold: RT-PCR (Allplex2019-nCoV Assay; Seegene, Seoul, Republic of Korea); target genes E gene, RdRP gene and N gene; threshold NR Single PCR-negative for D- presumed (NR) Samples used: NP/OP swabs Timing of reference standard: obtained simultaneously with blood samples (on presentation) Blinded to index test: yes Incorporated index test: no
Flow and timing	Time interval between index and reference tests: simultaneous testing All participants received the same reference standard: yes Missing data: 1 participant missing from 2x2 table with no explanation although all participants had the reference standard and index test. No data on time pso for 31/191 Uninterpretable results: none stated Indeterminate results: none stated Unit of analysis: participant. A considerable range in time pso was reported however, and results were not disaggregated by time pso.
Comparative	
Notes	Funding: none stated Publication status: preprint (not peer reviewed) Source: medRxiv Study author COI: none stated

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Paradiso 2020a *(Continued)*

If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Low risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Yes		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Qian 2020

Study characteristics	
Patient Sampling	4-group study recruiting patients estimating sensitivity and specificity [1] Confirmed COVID-19 cases (RT-PCR-positive) (n = 503) and [2] suspected COVID-19 cases based on epidemiological history, clinical symptoms and chest X-ray but 3 x PCR-negative (n = 52) Apparently contemporaneous controls, including:

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Qian 2020 *(Continued)*

	[3] hospitalised with non-COVID-19 conditions (PCR testing not described) (n = 972) [4] healthy controls (n = 586) Recruitment: unclear Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 2113 (555) Inclusion and exclusion criteria: NR
Patient characteristics and setting	Setting: hospital inpatients (cases) Location: 10 hospitals Country: China Dates: unclear Symptoms and severity: NR Sex: NR Age: NR Exposure history: NR
Index tests	Test name: NR Manufacturer: in-house Ab targets: IgG, IgM Antigens used: recombinant antigen from viral N protein and S protein Test method: CLIA Timing of samples: NR Samples used: serum Test operators: unclear Definition of test positivity: ≥ 10 AU/mL Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: RT-PCR for confirmed cases; suspected cases according to National Health Commission guideline (version 5) Samples used: unclear Timing of reference standard: during hospitalisation Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: unclear
Flow and timing	Time interval between index and reference tests: unclear Results presented by time period: no All participants received the same reference standard: unclear Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Qian 2020 *(Continued)*

Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Yes		
Did all participants receive a reference standard?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Qian 2020 *(Continued)*

Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

To 2020a [A]

Study characteristics	
Patient Sampling	Single-group study recruiting patients estimating sensitivity and specificity [1] Confirmed COVID-19 patients from 2 hospitals (n = 23) Recruitment: consecutive cases between 22 January-12 February, but excluding people with insufficient stored material Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 108 serum samples from 23 participants (23 cases). Only extractable > 14-day subset of 16 cases Inclusion and exclusion criteria: confirmed cases
Patient characteristics and setting	Setting: hospital inpatients Location: Princess Margaret Hospital and Queen Mary Hospital, Hong Kong Country: Hong Kong, China Dates: 22 January-12 February Symptoms and severity: 10/23 (43%) severe Sex: 13/23 (57%) male Age: median 62 years (range 37-75) Exposure history: NR
Index tests	2 tests evaluated, this entry (To 2020a [A]) refers to test [A] Test name: EIAs for [A] SARS-CoV-2 nucleoprotein and [B] S protein RBD Manufacturer: in-house Ab targets: IgG IgM Antigens used: [A] nucleoprotein and [B] S protein RBD Test method: EIA (considered with ELISA tests for analysis purposes) Timing of samples: 3-30 days pso Samples used: serum remnant from blood samples Test operators: NR Definition of test positivity: mean of 93 archived serum samples plus 3 x SD Blinded to reference standard: NR Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: laboratory confirmed - exact test unclear Samples used: NP or sputum specimens Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: n/a
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no, not extractable All participants received the same reference standard: yes Missing data: 7/23 (30%) were not tested between days 14 and 30 Uninterpretable results: NR Indeterminate results: NR Unit of analysis: unclear

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

To 2020a [A] *(Continued)*

Comparative	
Notes	Funding: this study was partly supported by the Consultancy Service for Enhancing Laboratory Surveillance of Emerging Infectious Diseases and Research Capability on Antimicrobial Resistance for the Department of Health of Hong Kong; the Theme-Based Research Scheme (T11/707/15) of the Research Grants Council, Hong Kong Special Administrative Region; Sanming Project of Medicine in Shenzhen, China (SZSM201911014); the High Level-Hospital Program, Health Commission of Guangdong Province, China; and donations from the Shaw Foundation Hong Kong, Richard Yu and Carol Yu, May Tam Mak Mei Yin, Michael Seak-Kan Tong, Respiratory Viral Research Foundation, Hui Ming, Hui Hoy and Chow Sin Lan Charity Fund Limited, Chan Yin Chuen Memorial Charitable Foundation, Marina Man-Wai Lee, and the Hong Kong Hainan Commercial Association South China Microbiology Research Fund Publication status: published paper Source: Lancet Infectious Diseases Study author COI: declare they have none

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	No		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

To 2020a [A] *(Continued)*

DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Unclear		
Could the patient flow have introduced bias?		High risk	

To 2020a [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (To 2020a [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (To 2020a [A])
Index tests	2 tests evaluated, this entry (To 2020a [B]) refers to test [B] Test name: EIAs for [A] SARS-CoV-2 nucleoprotein and [B] S protein RBD Manufacturer: in-house Ab targets: IgG IgM Antigens used: [A] nucleoprotein and [B] S protein RBD Test method: EIA (considered with ELISA tests for analysis purposes)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

To 2020a [B] *(Continued)*

	Timing of samples: 3-30 days pso Samples used: serum remnant from blood samples Test operators: NR Definition of test positivity: mean of 93 archived serum samples plus 3 x SD Blinded to reference standard: NR Threshold predefined: yes
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (To 2020a [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (To 2020a [A])
Comparative	
Notes	

Wan 2020 [A]

Study characteristics	
Patient Sampling	2-group design estimating sensitivity and specificity in acute disease [1] SARS-Cov-2-positive cases confirmed by RT-PCR (n = 7, 26 samples) [2] prepandemic sera (n = 5) and controls SARS-Cov-2 negative on 2 occasions (n = 5) Recruitment method NR Exclusion criteria NR
Patient characteristics and setting	[1] Inpatients at Singapore General Hospital, Singapore. Recruitment dates NR. Symptoms and severity, demographics and exposure history NR [2] Archived controls (n = 5) from Singapore General Hospital from 2015; recent patients with pneumonia investigated for COVID-19 but RT-PCR-negative twice and not meeting the criteria for suspected SARS-Cov-2 (n = 5)
Index tests	2 Ab tests used on serology samples, this entry (Wan 2020 [A]) refers to test [A] [A] in-house SARS-CoV total Ab ELISA laboratory assay (not a SARS-CoV-2-specific test). Measured total Ab; antigens NR. Positive defined as ≥ 400 [B] anti-SARS CoV IIFT laboratory assay from Euroimmun (Germany) (not a SARS-CoV-2-specific test). Measured IgM and IgG; antigens NR. Threshold NR Samples anonymised and blinded
Target condition and reference standard(s)	[1] Confirmed COVID-19 determined by RT-PCR; samples and methods NR. Tests undertaken during inpatient stay; blind to the index test [2] Confirmed not COVID-19 by chronology in n = 5, and by 2 repeated RT-PCR-negative results and not fulfilling criteria for suspected COVID-19 in n = 5; samples and methods NR. Tests undertaken during inpatient stay; blind to the index test
Flow and timing	All participants received a reference standard, but different reference standards were used in [1] and [2]. Multiple samples were included per participant; however these were disaggregated by time pso. Timing of reference standard and index tests NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wan 2020 [A] *(Continued)*

	Uninterpretable results not mentioned; 1/10 samples in group [2] indeterminate due to non-specific fluorescence. 5/26 samples in group [1] excluded due to narrow interval between tests or close proximity to the date of onset of illness. In group [1] between 1 and 9 samples per participant (mean = 3.7). Results for all samples per participant are presented allowing participant- and sample-based analyses.
Comparative	
Notes	No funding declared No conflicts of interest noted Report from a medRxiv preprint (not peer reviewed)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wan 2020 [A] *(Continued)*

Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Wan 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Wan 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Wan 2020 [A])
Index tests	2 Ab tests used on serology samples, this entry (Wan 2020 [B]) refers to test [B] [A) in-house SARS-CoV total Ab ELISA laboratory assay (not a SARS-CoV-2-specific test). Measured total Ab; antigens NR. Positive defined as ≥ 400 [B] anti-SARS CoV IIFT laboratory assay from Euroimmun (Germany) (not a SARS-CoV-2 specific test). Measured IgM and IgG; antigens NR. Threshold NR Samples anonymised and blinded
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Wan 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Wan 2020 [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wan 2020 [B] *(Continued)*

Comparative	
Notes	

Wang 2020a [A]

Study characteristics	
Patient Sampling	Purpose: diagnosis of active infection Design: 2-group study to estimate sensitivity and specificity for diagnosis of acute infection [1] COVID-19 patients, meeting diagnostic criteria a to Chinese Government guidelines (fifth edition) (n = 14) [2] Sera from patients with different pathogen infections and related chronic diseases with no clinical symptoms or imaging evidence of COVID-19 (n = 72), (with deliberate selection of rheumatoid factor IgM-positive sera) Recruitment: NR Sample size (virus/COVID cases): 86 (14) Inclusion and exclusion criteria: not described
Patient characteristics and setting	Setting: inpatient Location: affiliated Hospital of North Sichu, Chinaan Medical College and Nanchong Central Hospital Country: China Dates: 25 January -15 February 2020 Symptoms and severity: NR Demographics: NR Exposure history: NR Non-COVID patients group: other infection/chronic disease controls Source and time: 25 January-15 February 2020 Characteristics: IgM-positive sera from patients with different pathogen infections and related chronic diseases with no clinical symptoms or imaging evidence of COVID-19 (n = 72); flu A (n = 5), flu B (n = 5), *Mycoplasma pneumoniae* (n = 5), *Legionella pneumophila* (n = 5), positive rheumatoid factor (n = 36), HIV infection (n = 6), hypertension (n = 5) and diabetes mellitus (n = 5)
Index tests	2 tests evaluated, this entry (Wang 2020a [A]) refers to test [A] A. SARS-CoV-2 IgM detection kit CGIA (Beijing Hotgen Biotechnology Co., Beijing, China) (POC test, evaluation appears to be laboratory-based) B. ELISA (Beijing Hotgen Biotechnology Co., Beijing, China) (laboratory test) Ab targets: IgM Antigens used: NR Timing of samples: within 3-7 days after the beginning of the clinical symptoms for COVID-19 cases Samples used: serum Test operators: NR Definition of test positivity: A. as per manufacturer, colloidal gold colour reaction occurs at both T-line and C-line positions B. not described Blinded to reference standard: NR Threshold predefined: yes, as per manufacturer

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wang 2020a [A] *(Continued)*

Target condition and reference standard(s)	Reference standard for cases including threshold: diagnostic criteria from "Notice on the Issuance of Strategic Guidelines for Diagnosis and Treatment of Novel Coronavirus (SARS-CoV-2) Infected Pneumonia (Fifth Edition Version) Samples used: NR/ N/A Timing of reference standard: during hospital stay Blinded to index test: NR Incorporated index test: no Reference standard for controls: no clinical symptoms or imaging evidence of COVID-19 Samples used: NR Timing of reference standard: NR Blinded to index test: NR Incorporated index test: no
Flow and timing	Time interval between index and reference tests: NR, but all serology samples acquired within first week pso All participants received the same reference standard: yes Missing data: none stated Uninterpretable results: none stated Indeterminate results: none stated Unit of analysis: participant
Comparative	
Notes	Funding: none declared Publication status: accepted manuscript Source: Journal of Clinical Microbiology Study author COI: none declared

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wang 2020a [A] *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Wang 2020a [B]

Study characteristics

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Wang 2020a [B] *(Continued)*

Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Wang 2020a [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Wang 2020a [A])
Index tests	2 tests evaluated, this entry(Wang 2020a [B]) refers to test [B] A. SARS-CoV-2 IgM detection kit CGIA (Beijing Hotgen Biotechnology Co., Beijing, China) (POC test, evaluation appears to be laboratory-based) B. ELISA (Beijing Hotgen Biotechnology Co., Beijing, China) (laboratory test) Ab targets: IgM Antigens used: NR Timing of samples: within 3-7 days after the beginning of the clinical symptoms for COVID-19 cases Samples used: serum Test operators: NR Definition of test positivity: A. as per manufacturer, colloidal gold colour reaction occurs at both T-line and C-line positions B. not described Blinded to reference standard: NR Threshold predefined: yes, as per manufacturer
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Wang 2020a [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Wang 2020a [A])
Comparative	
Notes	

Xiang 2020a [A]

Study characteristics	
Patient Sampling	2-group design estimating sensitivity and specificity in acute disease [1] SARS-Cov-2 diagnosed patients (n = 63 for ELISA, n = 91 for GICA, some overlap of cases) [2] Healthy individuals (n = 35) Group [1] were recruited as a consecutive series and were inpatients with confirmed COVID-19 diagnosed according to WHO interim guidance
Patient characteristics and setting	[1] Inpatients at Wuhan Jinyintan Hospital, China, admitted 1-28 January 2020. Samples taken 2-4 February 2020. For ELISA 4/63 (6%) and GICA 4/91 (4%) classified as severe; 35/63 (56%) and 49/91 (54%) male. Median (IQR) age 65 (55-74) (n = 63) and 61 (48.5-67) years. Exposure NR [2] Healthy controls (n = 35). 17/35 (49%) male. Median (IQR) age 44 (39-49.5) years. No other detail given
Index tests	2 tests evaluated, this entry (Xiang 2020a [A]) refers to test [A]

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020a [A] *(Continued)*

	[A] novel coronavirus IgG/IgM Ab ELISA kits (laboratory kit manufactured by Zhu Hai Livzon Diagnostics). Measured IgM and IgG; antigen reported as "Enzyme-labelled antibody-linked antigen" for IgM and "recombinant antigen of new coronavirus" for IgG. Threshold NR [B] novel coronavirus IgG/IgM Ab GICA kits (POC test strips manufactured by Zhu Hai Livzon Diagnostics). Measured IgM and IgG; antigens NR. Threshold based on observing a coloured band turning red. A subset of participants who provided throat swab samples were also re-tested with a qRT-PCR test. Discussion states "that the new type of coronavirus antibody of the kit (doesn't specify which kit though) is against the severe acute respiratory syndrome (SARS)-like coronavirus, not only against SARS-CoV-2"
Target condition and reference standard(s)	[1] Confirmed COVID-19 determined according to WHO interim guidance; tests, samples and methods NR. Diagnosis made during inpatient stay; prior to the index test [2] No description given
Flow and timing	Unclear which participants received a reference standard, and the form of the reference standard Timing of reference standard and index tests NR Uninterpretable, indeterminate and missing results not mentioned One sample tested by each test per participant, unstated overlap of participants
Comparative	
Notes	Supported by the Zhongnan Hospital of Wuhan University Science, Technology and Innovation Seed Fund. No conflicts of interest noted. Report from a medRxiv preprint (not peer reviewed)

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Yes		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020a [A] *(Continued)*

If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Xiang 2020a [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Xiang 2020a [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Xiang 2020a [A])

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020a [B] *(Continued)*

Index tests	2 tests evaluated, this entry (Xiang 2020a [B] refers to test [B] [A] novel coronavirus IgG/IgM Ab ELISA kits (laboratory kit manufactured by Zhu Hai Livzon Diagnostics) Measured IgM and IgG; antigen reported as "Enzyme-labelled antibody-linked antigen" for IgM and "recombinant antigen of new coronavirus" for IgG. Threshold NR [B] novel coronavirus IgG/IgM Ab GICA kits (POC test strips manufactured by Zhu Hai Livzon Diagnostics) Measured IgM and IgG; antigens NR. Threshold based on observing a coloured band turning red. A subset of participants who provided throat swab samples were also re-tested with a qRT-PCR test. Discussion states "that the new type of coronavirus antibody of the kit (doesn't specify which kit though) is against the severe acute respiratory syndrome (SARS)-like coronavirus, not only against SARS-CoV-2"
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Xiang 2020a [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Xiang 2020a [A])
Comparative	
Notes	

Xiang 2020b

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity PCR conducted for patients presenting with a history of travel to or residence in Wuhan or local endemic areas; contact history with confirmed or suspected COVID-19 patients or part of a clustering outbreak, combined with clinical manifestation of 1) fever and/or respiratory symptoms, or 2) positive findings similar to COVID-19 pneumonia on chest CT scan, or 3) laboratory tests showing reduced lymphocytes and white blood cell counts in the early stage. Resulted in inclusion of [1] 85 RT-PCR-confirmed cases [2] 24 suspected cases with ≥ 2 negative RT-PCR and none positive (and protocol is to retest RT-PCR negatives every 1-2 days) [3] 60 control group of healthy blood donors (hospital staff) or from patients with other lung diseases in the same hospital (all PCR-negative) Recruitment: NR Prospective or retrospective recruitment of cases: unclear Sample size (virus/COVID cases): 169 (109; data for 66 lab-confirmed and 24 suspected cases extracted as D+ group) Inclusion and exclusion criteria: unclear
Patient characteristics and setting	Setting: hospital inpatients Location: Wuhan Country: China Dates: 19 January-2 March 2020 Symptoms and severity: [1] severe 18/85 (21%) [2] 2/24 (8%) severe Sex: [1] female 54/85 (64%) [2] female 12/24 (50%) [3] 35/60 (58%) female Age: [1] median 51 (IQR 32-65) [2] median 44 (IQR 36-61) [3] median 34 (IQR 29-51) Exposure history: NR
Index tests	Test name: ELISA Livzon Manufacturer: ELISA kits, Livzon Inc, Zhuhai, P.R.China, lot number of IgM: 20200308, IgG: 20200308

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020b *(Continued)*

	Ab targets: IgG IgM Antigens used: N protein? Test method: ELISA Timing of samples: NR Samples used: serum Test operators: NR Definition of test positivity: unclear "The optical density of each well was determined by a microplate reader set to 450 nm within 30 min. The ratio of optical density to the cut off value (optical density of the blank well + 0.1) was reported as the Ab concentration. For detection of IgG, the dilution factor was changed (1:20) and the cut off value was modified (optical density of the blank well + 0.13)." Blinded to reference standard: no Threshold predefined: unclear
Target condition and reference standard(s)	Reference standard for cases: [1] RT-PCR [2] Symptoms and PCR-negative (no guideline cited but criteria clearly elaborated) Samples used: NP and/or OP swabs Timing of reference standard: NR Blinded to index test: yes Incorporated index test: no Reference standard for non-cases: (no exposure or symptoms) and RT-PCR-negative
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no All participants received the same reference standard: Missing data: data per sample are provided for the 85 confirmed cases, however per participant data are available only for 66/85 confirmed cases plus 24/24 suspected cases (total number of cases reported = 90) Uninterpretable results: NR Indeterminate results: NR Unit of analysis: reports both samples and participants
Comparative	
Notes	Funding: this work is funded by National Natural Science Foundation of China (No. 81973990, 91643101), and Science Foundation of Huazhong University of Science and Technology (No. 2020kfyXGYJ100) Publication status: published in journal Source:Infectious Disease Society of America Study author COI: declare that they have none

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020b *(Continued)*

Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it prespecified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiang 2020b *(Continued)*

Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Xiao 2020a

Study characteristics	
Patient Sampling	Single-group study to estimate sensitivity for diagnosing active or prior infection Confirmed cases of COVID-19 (n = 34) according to the diagnosis and treatment guideline for SARS-CoV-2 from Chinese National Health Committee (Version 5) and the interim guidance from Centers for Disease Control and Prevention Recruitment method not clearly reported, likely convenience sample
Patient characteristics and setting	Inpatients, presumably at study authors' institution (Tongji Hospital) Wuhan, China. Admission date: 1-29 February 2020; final follow-up date 3 March 2020 NR Exposure history Sex: 12 female, 22 male Median age (review team estimated) 49 years (range 26-87), 22 (65%) male. Exposure history not described
Index tests	1 Ab test, blinding NR Laboratory-based CLIA (Shenzhen Yahuilong Biotechnology Co. Ltd.) measuring IgM and IgG. Antigen used not described. Threshold ≤ 10 AU/mL (describes following manufacturer protocol, but unclear if this includes threshold setting) Blood samples acquired ≥ 2 weeks after symptoms onset for 32/34 participants; and on day 2 and day 3 for remaining 2 participants
Target condition and reference standard(s)	COVID-19 according to diagnosis and treatment guideline for SARS-CoV-2 from Chinese National Health Committee (Version 5) and the interim guidance from Centers for Disease Control and Prevention; no further detail Timing and blinding to index test not described
Flow and timing	Time interval between index and reference not described. Study provides a breakdown in results by time pso but is different participants in each time period rather than multiple samplings for same participants No missing data, uninterpretable or indeterminate results described
Comparative	
Notes	No funding sources declared No conflicts of interest declared Pre-proof paper accepted for publication (Journal of Infection)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiao 2020a *(Continued)*

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xiao 2020a *(Continued)*

Was there an appropriate interval between index test and reference standard?	Unclear	
Did all patients receive the same reference standard?	Unclear	
Were all patients included in the analysis?	Unclear	
Did all participants receive a reference standard?	Yes	
Were results presented per patient?	Yes	
Could the patient flow have introduced bias?		Unclear risk

Xie 2020a

Study characteristics	
Patient Sampling	Single-group study recruiting patients estimating sensitivity to detect active disease [1] 16 confirmed COVID-19 using RT-PCR [2] 40 suspected cases using Chinese criteria but PCR-negative Recruitment: upon admission between 15-25 February 2020, unclear if consecutive Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 56 (56) of which 16 confirmed by RT-PCR Inclusion and exclusion criteria: unclear
Patient characteristics and setting	Setting: hospital inpatient Location: Unit Z6 at the Cancer Center of Wuhan Union Hospital Country: China Dates: enrolled 15-25 February 2020 Symptoms and severity: 34 severe, 22 not severe (more details on data extraction) Sex: 32/56 (57% female) Age: median age was 56.5 years (IQR 49.25-64.75) Exposure history: NR
Index tests	Test name: CLIA Manufacturer: YHLO Biological Technology Co., Ltd., Shenzhen, China Ab targets: IgG IgM Antigens used: envelope (E) protein and N protein Test method: CLIA Timing of samples: upon admission to hospital (with questionnaire to determine how many days prior to this symptom onset) Samples used: serum Test operators: NR Definition of test positivity: ≥ 10 AU/mL Blinded to reference standard: yes (upon admission) Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: [1] RT-PCR QIAamp RNA virus kit (Qiagen, Heiden, Germany), 1ab (ORF1ab) and N protein [2] diagnosed according to the 5th edition of the Guideline on diagnosis and treatment of COVID-19 established by China's National Health Commission, in-

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xie 2020a *(Continued)*

	cluding patient's epidemic history, clinical characteristics, chest CT scan and laboratory findings - RT-PCR-negative Samples used: NP and throat swabs Timing of reference standard: NR Blinded to index test: NR Incorporated index test: no Reference standard for non-cases: N/A
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: no All participants received the same reference standard: yes Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	Funding: this work was funded by the Special Project for Emergency Scientific and Technological Research on New Coronavirus Infection

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Yes		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Low risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xie 2020a *(Continued)*

DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Xu 2020a

Study characteristics	
Patient Sampling	Single-group study recruiting patients estimating sensitivity [1] confirmed COVID-19 cases Recruitment: unclear Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 10 (10) patients Inclusion and exclusion criteria: unclear
Patient characteristics and setting	Setting: hospital inpatients Location: Affiliated hospitals of Shanghai University of Medicine & Health Sciences Country: China Dates: NR Symptoms and severity: 2/10 died, 10/10 required oxygen Sex: 6/10 (60%) male Age: NR Exposure history: NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xu 2020a *(Continued)*

Index tests	Test name: COVID-19 IgG and IgM LFA Manufacturer: in-house Ab targets: IgG and IgM Antigens used: recombinant antigen (R18850) Test method: NR, lateral flow type Timing of samples: day 15-30 of observation Samples used: NR Test operators: NR Definition of test positivity: NR Blinded to reference standard: NR Threshold predefined: NR
Target condition and reference standard(s)	Reference standard for cases: RT-PCR Samples used: NR Timing of reference standard: NR Blinded to index test: NR Incorporated index test: no Reference standard for non-cases: N/A
Flow and timing	Time interval between index and reference tests: unclear Results presented by time period: no All participants received the same reference standard: yes Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	Funding: NR Publication status: preprint Source: medRxiv Study author COI: NR

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Xu 2020a *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Yongchen 2020

Study characteristics	
Patient Sampling	1-group study recruiting patients estimating sensitivity [1] 11 non-severe COVID-19 patients [2] 5 severe COVID-19 patients [3] 5 asymptomatic carriers Recruitment: Prospective or retrospective recruitment of cases: retrospective Sample size (virus/COVID cases): 21 (21) Inclusion and exclusion criteria: no more details available

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Yongchen 2020 *(Continued)*

Patient characteristics and setting	Setting: hospital Location: 2 medical centres - Second Hospital of Nanjing and the Affiliated Hospital of Xuzhou Medical University in Jiangsu Province Country: China Dates: 25 January-18 March 2020 Symptoms and severity: 5 severe, 11 non-severe and 5 asymptomatic cases. Illness severity defined according to the Chinese management guideline for COVID-19 (version 6.0). Severe cases defined as having any of the following: (a) respiratory distress; (b) hypoxia (SpO2 ≤ 93%); (c) abnormal blood gas analysis (PaO2/FiO2 ≤ 300 mm Hg); or (d) severe disease complications including respiratory failure, which requires mechanical ventilation, septic shock, or non-respiratory organ failure. Asymptomatic carriers were defined as individuals who were positive for COVID-19 nucleic acid but without any symptoms during screening of close contacts. Sex: 13/21 (62%) male Age: median (range) = 37 (10-73) Exposure history: NR
Index tests	Test name: no commercial name stated Manufacturer: Innovita Co., Ltd, China Ab targets: IgG and IgM Antigens used: SARS-CoV-2 S protein and N protein Test method: GICA Timing of samples: NR Samples used: serum Test operators: NR Definition of test positivity: NR Blinded to reference standard: NR and no assumptions made based on timing of the test Threshold predefined: NR
Target condition and reference standard(s)	Reference standard for cases: RT-PCR - confirmed after 2 sequential positive respiratory tract sample results Samples used: throat swabs Timing of reference standard: throat swab samples collected every 1-2 days Blinded to index test: yes (serum samples for serological evaluation were stored for later evaluation) Incorporated index test: no Reference standard for non-cases: N/A
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes All participants received the same reference standard: yes Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	Funding: supported by the National Natural Science Foundation of China, Jiangsu Provincial Medical Talent, Six talent peaks project of Jiangsu Province, Advanced health talent of six-one project of Jiangsu Province, Nanjing Medical Science and Technique Development Foundation Publication status: published paper Source: Emerging Microbes & Infections Study author COI: none was declared
Methodological quality	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Yongchen 2020 *(Continued)*

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Yongchen 2020 *(Continued)*

Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?			Unclear risk

Zeng 2020a

Study characteristics	
Patient Sampling	2-group study recruiting patients estimating sensitivity and specificity [1] COVID-19 cases [2] Healthy controls Recruitment: NR Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 63 (27) Inclusion and exclusion criteria: no details available
Patient characteristics and setting	Setting: hospital inpatient Location: Zhongnan Hospital, Wuhan Country: China Dates: NR Symptoms and severity: 17 severe cases. No further details Sex: 14/27 (52%) male Age: cases only - median (range) 62 (29-87) years; IQR 46-67 years Exposure history: NR
Index tests	Test name: none Manufacturer: Zhuhai Livzon Diagnostics INC Ab targets: IgG and IgM Antigens used: NR Test method: ELISA Timing of samples: 3-39 days for cases Samples used: serum Test operators: NR Definition of test positivity: OD = 0.105 Blinded to reference standard: NR Threshold predefined: unclear
Target condition and reference standard(s)	Reference standard for cases: NR

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zeng 2020a *(Continued)*

	Samples used: NR Timing of reference standard: NR Blinded to index test: NR Incorporated index test: NR Reference standard for non-cases: healthy controls; no indication of timing, PCR testing
Flow and timing	Time interval between index and reference tests: NR Results presented by time period: yes but only average Ab levels All participants received the same reference standard: NR Missing data: NR Uninterpretable results: NR Indeterminate results: NR Unit of analysis: participant
Comparative	
Notes	Funding: supported by National Key Research and Development Program of China and Emergency Science and Technology Project of Hubei Province Publication status: Journal pre-proof Source: Journal of Infection Study author COI: none

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zeng 2020a *(Continued)*

DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Unclear		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Unclear		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Zhang 2020a

Study characteristics	
Patient Sampling	Single-group design estimating sensitivity in acute and convalescent phase sera SARS-Cov-2 laboratory (RT-PCR detection or Ab assay) confirmed patients (n = 222) Participants were identified retrospectively, likely as a consecutive series
Patient characteristics and setting	Inpatients at Renmin Hospital of Wuhan University, China, admitted 13 January-1 March 2020. Samples dates not known. 87/222 (39%) classified as severe; 35/63 (56%) male. Median (IQR) age 62 (52-69) years. Exposure NR
Index tests	2 Ab tests used on serology samples iFlash-SARS-CoV-2 IgG and iFlash-SARS-CoV-2 IgM (laboratory tests manufactured by Shenzhen YHLO Biotech Co., Ltd.,). Measured IgM and IgG; antigens NR. Thresholds NR. Serum taken between day 1 and 35, 148/222 (67%) from day 21 onwards.
Target condition and reference standard(s)	COVID-19 determined with laboratory RT-PCR or anti-SARS-CoV-2 assay from nasal or pharyngeal swabs. No further detail given (cod-

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020a *(Continued)*

	ed as Chinese government guideline, 7th Ed) guideline. Diagnosis made during inpatient stay; prior to the index test
Flow and timing	Unclear which participants received which test (RT-PCR or Ab test as the reference standard). Samples acquired over considerable period pso; only disaggregation is for day 21 and over Timing of reference standard and index tests NR Uninterpretable, indeterminate and missing results not mentioned One sample tested by each test per participant
Comparative	
Notes	No funding declared. No conflicts of interest noted Report from a medRxiv preprint (not peer reviewed)

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	No		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020a *(Continued)*

The reference standard does not incorporate the index test	No		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Low concern
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Zhang 2020b

Study characteristics	
Patient Sampling	Multi-group design estimating sensitivity and specificity in acute phase sera First group included as single cohort to estimate sensitivity and specificity [1] Suspected COVID-19 cases (n = 228) admitted to fever clinic with RT-PCR testing for COVID-19 Other groups recruited but not analysed as part of this review: [2] Controls - outpatients with other diseases (n = 222) [3] Controls - medical staff working for the fever clinic (n = 63) [4] Controls - pre-pandemic healthy physical examinees (n = 223) No information about recruitment
Patient characteristics and setting	[1] Inpatients at Fever Clinic, Shengjing Hospital of China Medical University, China, admitted between 21 January-16 February 2020, samples dates not known. Median (range) age 35 (1-86). 124/225 (55%) male. Exposure NR [2] Outpatients at Shengjing Hospital of China Medical University, China, admitted between 21 January-16 February 2020, samples dates not known. Median (range) age 50 (27-85). 62/222 (28%) male [3] Medical staff at Fever Clinic, Shengjing Hospital of China Medical University, China, samples dates not known. Median (range) age 40 (25-61). 7/63 (11%) male [4] Healthy controls. Physical examinees in 2018. No setting stated. Median (range) age 59 (29-95). 77/223 (35%) male
Index tests	1 Ab test, no mention of blinding Unnamed IgG and IgM CLIA assay (laboratory tests manufactured by Shenzhen YHLO Biotech Co., Ltd). Measured IgM and IgG in sera; 2019-nCoV S protein S and N protein N antigen. Thresholds > 10.0 AU/mL (Ab concentration per mL. Sample timing only described for 3 cases (tests repeated every 1-3 days until between day 11 and day 17 (from Figure 1)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020b *(Continued)*

Target condition and reference standard(s)	[1] Virus detected with RT-PCR from NP/OP swabs. Ct value according to manufacturers instructions (NR); one of ORF1ab and N gene were required to be positive in same sample. Tests repeated once in negatives. Timing of swabs unclear Excluded cohorts: [2] No reference standard stated [3] No reference standard stated [4] Reference standard based on being pre-pandemic samples
Flow and timing	Timing of reference standard NR. Time pso reported only for the 3 confirmed cases Uninterpretable, indeterminate and missing results not mentioned 1 sample tested per participant
Comparative	
Notes	Funded by National Science and Technology Major Project of China, Liaoning Province Natural Science Foundation Project, Liaoning Province Central Government's special project to guide local scientific and technological development, Guangdong Province Major key projects of indusTentative technology, Major Special Project of Construction Program of China Medical University in 2018 and 345 talent project of Shengjing Hospital of China Medical University No conflicts of interest noted Report from a preprint (not peer reviewed)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Yes		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020b *(Continued)*

Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Yes		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Low risk	

Zhang 2020c

Study characteristics	
Patient Sampling	Single-group design estimating sensitivity in acute phase sera. RT-PCR positive confirmed patients (n = 139) who received around 10 days of medical treatment after admission (n = 16) were identified. No information about recruitment

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020c *(Continued)*

	The study includes a separate group of patients reporting multiple RT-PCR results
Patient characteristics and setting	Inpatients at Wuhan pulmonary hospital, China, admission dates NR, samples dates not known. No demographic or clinical information. Exposure NR
Index tests	One Ab test, blinding not described Anti-SARSr-CoV IgG and IgM ELISA kits (in-house laboratory method). Measured IgM and IgG in serum from samples on day 0 and day 5; antigen: SARSr-CoV Rp3 nucleoprotein. Threshold NR
Target condition and reference standard(s)	COVID-19 confirmed with laboratory RT-PCR. No further detail given. Diagnosis made during inpatient stay; prior to the index test
Flow and timing	Timing of reference standard NR Excluded if < 10 days medical treatment (n = 123) Uninterpretable, indeterminate results not mentioned One sample tested per participant at each time point; samples obtained on same days pso and all participants had ≥ 10 days medical Rx post admission
Comparative	
Notes	Supported by the Mega-Project for Infectious Disease from Minister of Science and Technology of the People's Republic of China, China Natural Science Foundation for excellent scholars, Strategic Priority Research Program of the CAS, Youth innovation promotion association of CAS No conflicts of interest noted Report from a published peer reviewed paper

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	No		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020c *(Continued)*

Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Zhang 2020d

Study characteristics	
Patient Sampling	Single-group study recruiting patients estimating sensitivity and specificity [1] Patients with suspected COVID-19 (n = 824, 154 cases) Recruitment: unclear
Patient characteristics and setting	Setting: hospital Location: 5 hospitals - Huoshenshan Hospital (Wuhan), General Hospital of Central 19 Threater Command of the PLA (Wuhan), the Sixth People's Hospital of Shenyang, Peking Union Medical College Hospital, and Shijiazhuang Fifth Hospital.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020d *(Continued)*

	Country: China Dates: no details Symptoms and severity: no details Sex: no details Age: no details Exposure history: no details
Index tests	Test name: colloidal GICA Manufacturer: in-house Ab targets: total Abs (IgG and IgM) Antigens used: rS1 and rS-RBD-mFc S proteins Test method: CGIA Timing of samples: NR Samples used: serum Test operators: NR Definition of test positivity: visible line Blinded to reference standard: unclear Threshold predefined: yes
Target condition and reference standard(s)	Reference standard for cases: real-time PCR kit, included patients PCR-negative but clinically diagnosed by CT as D+; D- are RT-PCR negative but unclear if all had CT to confirm absence Samples used: nasal/pharyngeal swab Timing of reference standard: unclear Blinded to index test: unclear Incorporated index test: no Reference standard for non-cases: single PCR-negative
Flow and timing	Time interval between index and reference tests: no information Results presented by time period: no All participants received the same reference standard: yes Missing data: no information Uninterpretable results: no information Indeterminate results: no information Unit of analysis: participant
Comparative	
Notes	Funding: The National Key Research and Development Program of China, and The National Science and Technology Major Project Publication status: preprint Source:preprint server (medRxiv) Study author COI: report no COI but 1 author from a company (Beijing Hotgen Biotechnology Inc., Beijing)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	Yes		
Did the study avoid inappropriate exclusions?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhang 2020d *(Continued)*

Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		Unclear risk	
Are there concerns that the included patients and setting do not match the review question?			Low concern
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	No		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		High risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	Yes		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		Unclear risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhao 2020a

Study characteristics	
Patient Sampling	2-group design estimating sensitivity and specificity in acute phase sera [1] Confirmed COVID-19 cases (n = 173) with positive RT-PCR testing for COVID-19 [2] Controls - pre-pandemic healthy individuals (n = 213) No information about recruitment
Patient characteristics and setting	[1] Inpatients at Shenzhen Third People's Hospital, Shenzhen, China, admitted between 11 January-9 February 2020, samples between day 1 and day 39. Median (IQR) age 48 (35-61). 84/173 (49%) male. 126/173 (73%) clear exposure identified. 32/173 (18%) considered critical (presence of ARDS or oxygen saturation < 93%, requiring mechanical ventilation) [2] No information given
Index tests	One Ab test, no mention of blinding ELISA double antigen sandwich immunoassay (laboratory tests manufactured by Shenzhen YHLO Biotech Co.,Ltd). Measured total Ab, IgM and IgG in plasma; Ab and IgM - RBD of the S protein of SARS-CoV-2; IgG - recombinant nucleoprotein antigen. Thresholds NR. Sample timing described for all participants Results from repeat RT-PCR test mentioned, but no details given
Target condition and reference standard(s)	[1] Virus detected with RT-PCR from respiratory swabs. Timing of swabs unclear but precedes serology tests [2] Reference standard based on being pre-pandemic samples
Flow and timing	Timing of reference standard NR, all within hospital stay Inadequate plasma samples for 2 IgM tests and 1 IgG test Uninterpretable and indeterminate results not mentioned 535 samples tested from 173 participants; data disaggregated over time. Overall sensitivity and specificity defined as positive at any time point. Accuracy in different time periods based on fewer repeat samples (numbers not known)
Comparative	
Notes	Supported by Bill & Melinda Gates Foundation No conflicts of interest noted Report from a preprint (not peer reviewed)

Methodological quality

Item	**Authors' judgement**	**Risk of bias**	**Applicability concerns**
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhao 2020a *(Continued)*

Did the study avoid inappropriate inclusions?	Yes		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	No		
If a threshold was used, was it pre-specified?	Unclear		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			Low concern
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Low risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	No		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhao 2020b

Study characteristics	
Patient Sampling	3-group study recruiting patients estimating sensitivity and specificity [1] Pre-pandemic controls (n = 257) [2] Controls selected during pandemic (n = 155) [3] Cases from hospitalised or recovered patients (n = 69) Recruitment: various sources and locations Prospective or retrospective recruitment of cases: prospective Sample size (virus/COVID cases): 481 (69) Inclusion and exclusion criteria: no details
Patient characteristics and setting	Setting: hospital inpatient (cases), community/hospital/clinical lab (controls) Location: for cases various hospitals (including 2 in Beijing and one in Wuhan); group 2 controls from Beijing (N = 15) and Zheiiang province (N = 140) Country: China Dates: NR Symptoms and severity: cases-at different clinic stages. No more detail Sex: no overall details Age: no details Exposure history: no details
Index tests	Test name: SARS-CoV-2 virus serology ELISA kit Manufacturer: in-house Ab targets: total Ab (IgG + IgM) Antigens used: SARS-CoV-2-S1 protein Test method: ELISA Timing of samples: during hospitalisation Samples used: plasma Test operators: NR Definition of test positivity: standard ELISA method Blinded to reference standard: unclear Threshold predefined: as per controls supplied with ELISA
Target condition and reference standard(s)	Reference standard for cases: unclear Samples used: unclear Timing of reference standard: unclear Blinded to index test: yes Incorporated index test: unclear Reference standard for non-cases: group 1-pre-pandemic, group 2-unclear
Flow and timing	Time interval between index and reference tests: unclear Results presented by time period: no but possible for a subset of the cases All participants received the same reference standard: no Missing data: no details Uninterpretable results: no details Indeterminate results: no details Unit of analysis: unclear
Comparative	
Notes	Funding: research Grants from Beijing Science and Technology Commission, Bill & Melinda Gates Foundation, National Natural Science Foundation of China (NSFC) and the National Science and Technology Major Project Publication status: preprint Source: preprint server medRxiv Study author COI: no details but 3 authors are from 3 different companies (Any-Go Technology Co., Ltd, Beijing; AbMax Biotechnology Co., LTD, Beijing; Zhenge Biotechnology Co., LTD, Shanghai)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhao 2020b *(Continued)*

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	Yes		
Could the conduct or interpretation of the index test have introduced bias?		Unclear risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Unclear		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Yes		
The reference standard does not incorporate the index test	Unclear		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			Unclear

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhao 2020b *(Continued)*

DOMAIN 4: Flow and Timing	
Was there an appropriate interval between index test and reference standard?	Unclear
Did all patients receive the same reference standard?	No
Were all patients included in the analysis?	Unclear
Did all participants receive a reference standard?	Yes
Were results presented per patient?	Yes
Could the patient flow have introduced bias?	High risk

Zhong 2020 [A]

Study characteristics	
Patient Sampling	2-group study to estimate sensitivity and specificity for diagnosis of active infection [1] PCR-positive COVID-19 patients (n = 47) [2] Healthy controls (n = 300) No further details of inclusion or exclusion criteria
Patient characteristics and setting	[1] Source of cases not described. Study conducted in China. Recruitment period not described (symptom onset for cases dates from 15 January-13 February 2020; sampling dates from 28 January-21 February 2020) Severity (cases only): mild = 22 (47%); moderate = 14 (30%); severe = 6 (13%); critical 5 (11%) Sex: 34% male Age: median 48 (range 18-82) years. Exposure history not described [2] Healthy controls not described in regard to timing of sampling or characteristics
Index tests	3 tests evaluated, this entry (Zhong 2020 [A]) refers to test [A] Both laboratory-based evaluations to detect IgM and IgG A. ELISA using N gene of the SARS-CoV-2 cloned into a pET28a vector (rN-based assay) B ELISA using S gene cloned into a pMFcIg vector-based (rS-based assay) C. CLIA (not clearly described; potentially uses both of above described antigens) Thesholds defined retrospectively in regard to optimal cut-off on ROC curve
Target condition and reference standard(s)	[1] PCR (no further details); positivity threshold not described. Symptom onset 15 January-13 February, with serology sampling up to 21 February 2020. RT-PCR probably SARS-Cov-2 specific, but not certain [2] No description of healthy controls provided
Flow and timing	Time interval between index and reference not described. Results not disaggregated by time period pso No missing data, uninterpretable or indeterminate results described

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhong 2020 [A] *(Continued)*

	Patient-based analysis
Comparative	
Notes	Work was supported by the grants from Sichuan Science and Technology Program (2020YFS0014 and 2020YFS0558), the Chinese Academy of Medical Sciences (2019-I2M-5-032) and Technology & Science & Technology Bureau of Chengdu (2020-YF05-00060-SN and 2020-YF05-00075-SN) Authors declare no COI present; 3 co-authors employed by Maccura Biotech Published letter to Editor (Sci China Life Sci)

Methodological quality

Item	Authors' judgement	Risk of bias	Applicability concerns
DOMAIN 1: Patient Selection			
Was a consecutive or random sample of patients enrolled?	Unclear		
Was a case-control design avoided?	No		
Did the study avoid inappropriate exclusions?	Unclear		
Did the study avoid inappropriate inclusions?	Unclear		
Could the selection of patients have introduced bias?		High risk	
Are there concerns that the included patients and setting do not match the review question?			High
DOMAIN 2: Index Test (All tests)			
DOMAIN 2: Index Test (Antibody tests)			
Were the index test results interpreted without knowledge of the results of the reference standard?	Unclear		
If a threshold was used, was it pre-specified?	No		
Could the conduct or interpretation of the index test have introduced bias?		High risk	
Are there concerns that the index test, its conduct, or interpretation differ from the review question?			High
DOMAIN 3: Reference Standard			
Is the reference standards likely to correctly classify the target condition?	Yes		
Were the reference standard results interpreted without knowledge of the results of the index tests?	Unclear		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhong 2020 [A] *(Continued)*

The reference standard does not incorporate the index test	Yes		
Could the reference standard, its conduct, or its interpretation have introduced bias?		Unclear risk	
Are there concerns that the target condition as defined by the reference standard does not match the question?			High
DOMAIN 4: Flow and Timing			
Was there an appropriate interval between index test and reference standard?	Unclear		
Did all patients receive the same reference standard?	No		
Were all patients included in the analysis?	Unclear		
Did all participants receive a reference standard?	Yes		
Were results presented per patient?	Yes		
Could the patient flow have introduced bias?		High risk	

Zhong 2020 [B]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Index tests	3 tests evaluated, this entry (Zhong 2020 [B]) refers to test [B] Both laboratory-based evaluations to detect IgM and IgG A. ELISA using N gene of the SARS-CoV-2 cloned into a pET28a vector (rN-based assay) B ELISA using S gene cloned into a pMFcIg vector-based (rS-based assay) C. CLIA (not clearly described; potentially uses both of above described antigens) Thesholds defined retrospectively in regard to optimal cut-off on ROC curve
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Comparative	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Zhong 2020 [C]

Study characteristics	
Patient Sampling	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Patient characteristics and setting	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Index tests	3 tests evaluated, this entry (Zhong 2020 [C]) refers to test [C] Both laboratory-based evaluations to detect IgM and IgG A. ELISA using N gene of the SARS-CoV-2 cloned into a pET28a vector (rN-based assay) B ELISA using S gene cloned into a pMFcIg vector-based (rS-based assay) C. CLIA (not clearly described; potentially uses both of above described antigens) Thesholds defined retrospectively in regard to optimal cut-off on ROC curve
Target condition and reference standard(s)	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Flow and timing	See main entry for this study for characteristics and QUADAS-2 assessment (Zhong 2020 [A])
Comparative	
Notes	

A&E: Accident and Emergency Department; **Ab:** antibody; **ARDS:** acute respiratory distress syndrome; **AU:** arbitrary unit; **CDC:** Center for Disease Control; **CMV:** cytomegalovirus; **CT:** computed tomography; **CGIA:** colloidal gold immunoassay; **CLIA:** chemiluminescence immunoassay; **COI:** conflict of interest; **D-:** disease negative; **D+:** disease positive; **EIA:** enzyme immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **Flu:** fluorescence intensity; **GICA:** gold immunochromatography assay; **HCW:** healthcare worker; **ICU:** intensive care unit; **IIFT:** indirect Immunofluorescence test; **LFA:** lateral flow assay; **LFIA:** lateral flow immunoassay; **LIPS:** luciferase immunoprecipitation system; **LRTI:** lower respiratory tract infection; **N protein:** nucleocapsid protein; **N/A:** not applicable; **NAAT:** nucleic acid amplification test; **NIH:** National Institues of Health; **NIHR:** National Institute for Health Research; **NP:** nasopharyngeal; **NR:** not reported; **OP:** oropharyngeal; **PCR:** polymerase chain reaction; **POC:** point-of-care; **pso:** post-symptom onset; **RBD:** receptor binding domain; **RNA:** ribonucleic acid; **ROC:** receiver operating characteristic; **RT-PCR:** reverse transcriptase polymerase chain reaction; **RT-qPCR:** reverse transcriptase quantitative polymerase chain reaction; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **S-flow:** flow-cytometry based test; **S protein:** spike protein; **SD:** standard deviation; **TB:** tuberculosis; **WHO:** World Health Organization

Characteristics of excluded studies *[ordered by study ID]*

Study	Reason for exclusion
Ai 2020	Ineligible reference standard
Aitken 2020	Ineligible study design
Amanat 2020	Accuracy data cannot be extracted
Annamalai 2020	Ineligible study design
Argenziano 2020	Ineligible index test
Arons 2020	Ineligible index test
Arumugam 2020	Ineligible study design

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Baggett 2020	Ineligible study design
Bai 2020	Inadequate sample size
Bajema 2020	Ineligible study design
Barra 2020	Ineligible study design
Batista 2020	Ineligible index test
Beltran Corbellini 2020	Ineligible index test
Beltran Pavez 2020	Inadequate sample size
Ben Ami 2020	Ineligible index test
Bhadra 2020	Ineligible study design
Bordi 2020	Ineligible study design
Burhan 2020	Ineligible study design
Cai 2020	Ineligible study design
Callahan 2020	Accuracy data cannot be extracted
Chan 2020	Ineligible study design
Chandler Brown 2020	Ineligible study design
Chen 2020b	Ineligible target condition
Chen 2020c	Ineligible study design
Cheng 2020a	Ineligible reference standard
Chu 2020	Ineligible study design
Colson 2020	Inadequate sample size
Comar 2020	Ineligible reference standard
Corman 2020	Ineligible study design
Cui 2020	Ineligible study design
Curti 2020	Ineligible study design
Dahlke 2020	Inadequate sample size
Ding 2020	Ineligible study design
Fang 2020z	Ineligible index test
Farfan 2020	Ineligible study design

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Feng 2020	Ineligible index test
Fontanet 2020	Ineligible study design
Fu 2020a	Ineligible population
Fu 2020b	Accuracy data cannot be extracted
Fumeaux 2020	Ineligible study design
Gao 2020	Ineligible index test
Giamarellos Bourboulis 2020	Ineligible study design
Gietema 2020	Ineligible index test
Gonzalez Gonzalez 2020a	Ineligible study design
Gonzalez Gonzalez 2020b	Ineligible study design
Guan 2020	Ineligible study design
Guo 2020b	Ineligible study design
Guo 2020c	Ineligible population
Han 2020	Ineligible index test
Hao 2020	Ineligible study design
Hass 2020	Ineligible target condition
Hirotsu 2020	Ineligible study design
Hogan 2020	Ineligible index test
Holland 2020	Ineligible study design
Hu 2020b	Ineligible study design
Hu 2020c	Author contact needed
Hu 2020d	Ineligible index test
Huang 2020a	Ineligible study design
Jenkins 2020	Ineligible study design
Jiang 2020a	Ineligible study design
Jiang 2020b	Accuracy data cannot be extracted
Jung 2020	Ineligible study design
Khan 2020	Ineligible study design

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Kim 2019	Ineligible study design
Kong 2020	Ineligible study design
Konrad 2020	Ineligible study design
Kurstjens 2020	Ineligible index test
Lamb 2020	Ineligible study design
Lan 2020	Ineligible population
Lechien 2020	Ineligible index test
Lei 2020	Ineligible study design
Li 2020c	Inadequate sample size
Li 2020d	Ineligible study design
Li 2020e	Ineligible index test
Li 2020f	Ineligible population
Li 2020g	Ineligible index test
Liang 2020a	Ineligible index test
Liang 2020b	Ineligible study design
Ling 2020	Ineligible target condition
Liu 2020e	Ineligible index test
Liu 2020f	Ineligible index test
Liu 2020g	Ineligible index test
Liu 2020h	Ineligible study design
Lo 2020	Ineligible index test
Lopez-Rincon 2020	Ineligible study design
Lu 2020	Ineligible study design
Ma 2020b	Ineligible study design
Mahari 2020	Ineligible study design
Mardani 2020	Ineligible index test
Marzinotto 2020	Accuracy data cannot be extracted
McKay 2020	Ineligible study design

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
McRae 2020	Ineligible index test
Mei 2020	Ineligible index test
Meng 2020	Ineligible index test
Mercurio 2020	Ineligible study design
Metsky 2020	Ineligible study design
Nelson 2020	Ineligible study design
Nemati 2020	Ineligible study design
Nie 2020	Ineligible study design
Nunez Bajo 2020	Ineligible study design
Okba 2020b	Ineligible study design
Paden 2020	Ineligible study design
Pan 2020b	Ineligible index test
Pan 2020c	Ineligible study design
Pan 2020d	Ineligible index test
Pan 2020e	Ineligible study design
Paradiso 2020b	Accuracy data cannot be extracted
Park 2020	Ineligible study design
Peng 2020	Ineligible index test
Pfefferle 2020	Ineligible study design
Rauch 2020	Ineligible study design
Scallan 2020	Accuracy data cannot be extracted
Seo 2020	Accuracy data cannot be extracted
Shental 2020	Ineligible study design
Shi 2020	Ineligible index test
Shirato 2020	Ineligible study design
Song 2020	Ineligible index test
Su 2020	Ineligible index test
Sun 2020a	Ineligible index test

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Sun 2020b	Ineligible index test
Sun 2020c	Ineligible study design
Tagarro 2020	Ineligible index test
Tan 2020a	Ineligible study design
Tan 2020b	Ineligible index test
Tan 2020c	Ineligible study design
Toptan 2020	Ineligible study design
Tsang 2003	Ineligible target condition
Vermeiren 2020	Accuracy data cannot be extracted
Viehweger 2020	Ineligible study design
Vogels 2020	Ineligible study design
Waghmare 2020	Ineligible population
Wang 2020b	Ineligible index test
Wang 2020c	Accuracy data cannot be extracted
Wang 2020d	Accuracy data cannot be extracted
Wang 2020e	Accuracy data cannot be extracted
Wang 2020f	Ineligible study design
Wang 2020g	Retracted study
Wang 2020h	Accuracy data cannot be extracted
Wang 2020i	Ineligible index test
Wee 2020	Ineligible study design
Weiss 2020	Accuracy data cannot be extracted
Woelfel 2020	Ineligible reference standard
Won 2020	Ineligible study design
Woo 2020	Ineligible study design
Wu 2020a	Ineligible index test
Wu 2020b	Ineligible study design
Wu 2020c	Accuracy data cannot be extracted

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Reason for exclusion
Xia 2020a	Ineligible index test
Xia 2020b	Ineligible study design
Xie 2020b	Ineligible population
Xie 2020c	Accuracy data cannot be extracted
Xing 2020a	Inadequate sample size
Xing 2020b	Ineligible reference standard
Xu 2020b	Ineligible study design
Xu 2020c	Inadequate sample size
Xu 2020d	Ineligible index test
Yan 2020	Ineligible study design
Yang 2020a	Ineligible reference standard
Yang 2020b	Ineligible study design
Yelin 2020	Ineligible study design
Yuan 2020	Accuracy data cannot be extracted
Yun 2020	Ineligible study design
Zeng 2020b	Accuracy data cannot be extracted
Zhang 2020e	Ineligible study design
Zhang 2020f	Ineligible study design
Zhang 2020g	Accuracy data cannot be extracted
Zhang 2020h	Accuracy data cannot be extracted
Zhao 2020c	Ineligible study design
Zhao 2020d	Ineligible study design
Zhifeng 2020	Ineligible reference standard
Zhou 2020	Accuracy data cannot be extracted
Zhuang 2020	Retracted study

Characteristics of studies awaiting classification *[ordered by study ID]*

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Li 2020b

Patient Sampling	Foreign language study awaiting translation
Patient characteristics and setting	
Index tests	
Target condition and reference standard(s)	
Flow and timing	
Comparative	
Notes	

Thompson 2020

Patient Sampling	Study of neutralising antibodies; to be assessed for inclusion in review update
Patient characteristics and setting	
Index tests	
Target condition and reference standard(s)	
Flow and timing	
Comparative	
Notes	

Xiong 2020

Patient Sampling	Foreign language study awaiting translation
Patient characteristics and setting	
Index tests	
Target condition and reference standard(s)	
Flow and timing	
Comparative	
Notes	

Characteristics of ongoing studies *[ordered by study ID]*

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000029625

Study name	Construction of early warning and prediction system for patients with severe / critical novel coronavirus pneumonia (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000029695

Study name	Early detection of novel coronavirus pneumonia (COVID-19) based on a novel high-throughput mass spectrometry analysis with exhaled breath
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000029810

Study name	Clinical study of a novel high sensitivity nucleic acid assay for novel coronavirus pneumonia (COVID-19) based on CRISPR-cas protein
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000029870

Study name	Evaluation of rapid diagnostic kit (IgM/IgG) for novel coronavirus pneumonia (COVID-19)
Target condition and reference standard(s)	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000029870 *(Continued)*

Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000029883

Study name	A comparative study on the sensitivity of nasopharyngeal and oropharyngeal swabbing for the detection of SARS-CoV-2 by re-al-time PCR
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000029982

Study name	Study for using multiomics in the diagnosis and treatment of novel coronavirus pneumonia (COVID-19
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030005

Study name	Nucleic acid analysis of novel coronavirus pneumonia (COVID-19) in morning sputum samples and pharyngeal swabs-a prospectively diag-nostic test
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030005 *(Continued)*

Contact information	
Notes	

ChiCTR2000030085

Study name	Cancelled by the investigator Study for the false positive rate of IgM / IgG antibody test kit for novel coronavirus pneumonia (COVID-19) in different inpatients
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030185

Study name	The value of critical care ultrasound in rapid screening, diagnosis, evaluation of effectiveness and intensive prevention of novel coronavirus pneumonia (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030253

Study name	Exploration and research for a new method for detection of novel coronavirus (COVID-19) nucleic acid
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030334

Study name	MicroRNA as a marker for early diagnosis of novel coronavirus infection (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030542

Study name	A clinical study about the diagnosis and prognosis evaluation of novel coronavirus pneumonia (COVID-19) based on viral genome, host genomic sequencing, relative cytokines and other laboratory indexes
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030543

Study name	Detection of coronavirus in simultaneously collecting tears and throat swab samples collected from the patients with novel coronavirus pneumonia (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030558

Study name	Cancelled by the investigator Epidemiological research of novel coronavirus pneumonia (COVID-19) suspected cases based on virus nucleic acid test combined with low-dose chest CT screening in primary hospital
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030706

Study name	Cancelled by the investigator Application of cas13a-mediated RNA detection in the assay of novel coronavirus nucleic acid (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030721

Study name	A comparative study for the sensitivity of induced sputum and throat swabs for the detection of SARS-CoV-2 by real-time PCR in patients with novel coronavirus pneumonia (COVID-19)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030754

Study name	Medical records based study for the accuracy of SARS-CoV-2 IgM antibody screening for diagnosis of novel coronavirus pneumonia (COVID-19)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030754 *(Continued)*

Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030833

Study name	Clinical validation and application of high-throughput novel coronavirus (2019-nCoV) screening detection kit
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030834

Study name	Epidemiological characteristics and antibody levels of novel coronavirus pneumonia (COVID-19) of pediatric medical staff working in quarantine area
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030838

Study name	Development of warning system with clinical differential diagnosis and prediction for severe type of novel coronavirus pneumonia (COVID-19) patients based on artificial intelligence and CT images
Target condition and reference standard(s)	
Index and comparator tests	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030838 *(Continued)*

Starting date	
Contact information	
Notes	

ChiCTR2000030856

Study name	An artificial intelligence assistant system for suspected novel coronavirus pneumonia (COVID-19) based on chest CT
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030859

Study name	A medical based analysis for influencing factors of death of novel coronavirus pneumonia (COVID-19) patients in Wuhan Third Hospital
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

ChiCTR2000030860

Study name	A medical records based study for investigation of dynamic profile of RT-PCR test for SARS-CoV-2 nucleic acid of novel coronavirus pneumonia (COVID-19) patients
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

ChiCTR2000030860 *(Continued)*

Notes	

ChiCTR2000030862

Study name	Correlation analysis of blood eosinophil cell levels and clinical type category of novel coronavirus pneumonia (COVID-19): a medical records based retrospective study
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04245631

Study name	Development of a simple, fast and portable recombinase aided amplification assay for 2019-nCoV
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04259892

Study name	Viral excretion in contact subjects at high/moderate risk of coronavirus 2019-nCoV infection
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

NCT04279795

Study name	Detection of 2019 novel coronavirus in multiple organ system and its relationship with clinical manifestations
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04304690

Study name	SARS-CoV2 seroconversion among front line medical and paramedical staff in emergency, intensive care units and infectious disease departments during the 2020 epidemic
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04311398

Study name	Development and verification of a new coronavirus multiplex nucleic acid detection system
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04316728

Study name	Clinical performance of the VivaDiag ™ COVID-19 IgM IgG rapid test in early detecting the infection of COVID-19
Target condition and reference standard(s)	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

NCT04316728 *(Continued)*

Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04321369

Study name	Impact of swab site and sample collector on testing sensitivity for SARS-CoV-2 virus in symptomatic individuals
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04322279

Study name	Factors associated with a positive SARS-CoV-2 serology in contact subjects at high/moderate risk of coronavirus SARS-CoV-2 infection (CoV-CONTACT-SERO)
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

NCT04322513

Study name	Biomarkers for identification of SARS-COV-2 infection
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

NCT04322513 *(Continued)*

Contact information	
Notes	

Sullivan 2020

Study name	Detection of SARS-CoV-2 RNA and antibodies in diverse samples: protocol to validate the sufficiency of provider-observed home-collected blood, saliva and oropharyngeal samples
Target condition and reference standard(s)	
Index and comparator tests	
Starting date	
Contact information	
Notes	

DATA

Presented below are all the data for all of the tests entered into the review.

Table Tests. Data tables by test

Test	No. of studies	No. of participants
1 IgG (all time points)	62	11748
2 IgG (1 to 7 days)	33	585
3 IgG (8 to 14 days)	34	1220
4 IgG (15 to 21 days)	32	1108
5 IgG (22 to 35 days)	20	495
6 IgG (over 35 days)	12	259
7 IgM (all time points)	58	11436
8 IgM (8 to 14 days)	31	1166
9 IgM (1 to 7 days)	34	658
10 IgM (15 to 21 days)	30	1057
11 IgM (22 to 35 days)	18	492

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test	No. of studies	No. of participants
12 IgM (over 35 days)	12	222
13 IgG/IgM (all time points)	44	9496
14 IgG/IgM (1 to 7 days)	17	259
15 IgG/IgM (8 to 14 days)	21	608
16 IgG/IgM (15 to 21 days)	21	692
17 IgG/IgM (22 to 35 days)	16	152
18 IgG/IgM (over 35 days)	9	153
19 IgA (all time points)	5	1278
20 IgA (1 to 7 days)	4	100
21 IgA (8 to 14 days)	4	65
22 IgA (15 to 21 days)	3	78
23 IgA (22 to 35 days)	3	90
24 IgA (over 35 days)	1	23
25 Total antibodies (Ab) (all time points)	17	5339
27 Total antibodies (Ab) (1 to 7 days)	5	144
29 Total antibodies (Ab) (8 to 14 days)	6	247
30 Total antibodies (Ab) (15 to 21 days)	6	176
31 Total antibodies (Ab) (21 to 35 days)	4	19
32 Total antibodies (Ab) (over 35 days)	2	28
33 IgA/IgG (all time points)	2	775
34 IgA/IgG (1 to 7 days)	1	12
35 IgA/IgG (8 to 14 days)	1	10
36 IgA/IgG (15 to 21 days)	1	8
37 IgA/IgG (22 to 35 days)	1	1
38 IgA/IgM (all time points)	1	699
39 IgG in PCR+ve (all time points)	4	558
40 IgG in PCR +ve (1 to 7 days)	2	28
41 IgG in PCR+ve (8 to 14 days)	2	33

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test	No. of studies	No. of participants
42 IgG in PCR+ve (15 to 21 days)	2	40
43 IgG in PCR-ve (all time points)	6	252
44 IgG in PCR-ve (1 to 7 days)	2	13
45 IgG in PCR-ve (8 to 14 days)	3	30
46 IgG in PCR-ve (15 to 21 days)	3	72
47 IgM in PCR+ve (all time points)	6	740
48 IgM in PCR+ve (1 to 7 days)	2	28
49 IgM in PCR+ve (8 to 14 days)	2	33
50 IgM in PCR+ve (15 to 21 days)	2	16
51 IgM in PCR-ve (all time points)	8	352
52 IgM in PCR-ve (1 to 7 days)	2	13
53 IgM in PCR-ve (8 to 14 days)	3	30
54 IgM in PCR-ve (15 to 21 days)	3	72
55 IgG/IgM in PCR+ve (all time points)	2	177
56 IgG/IgM in PCR+ve (1 to 7 days)	2	36
57 IgG/IgM in PCR+ve (8 to 14 days)	2	53
58 IgG/IgM in PCR+ve (15 to 21 days)	2	150
59 IgG/IgM in PCR-ve (all time points)	4	215
60 IgG/IgM in PCR-ve (1 to 7 days)	2	17
61 IgG/IgM in PCR-ve (8 to 14 days)	3	40
62 IgG/IgM in PCR-ve (15 to 21 days)	3	113
63 IgG (moderate)	1	44
64 IgG (severe)	1	52
65 IgG (critical)	1	37
66 IgM (moderate)	1	44
67 IgM (severe)	1	52
68 IgM (critical)	1	37
69 RT-PCR (all time points - throat)	2	276

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test	No. of studies	No. of participants
70 RT-PCR (1 to 7 days throat)	2	67
71 RT-PCR (8 to 14 days - throat)	2	142
72 RT-PCR (15 to 21 days - throat)	2	73
73 RT-PCR (all time points - sputum)	1	53
74 RT-PCR (1 to 7 days - sputum)	1	13
75 RT-PCR (8 to 14 days - sputum)	1	8
76 RT-PCR (15 to 21 days - sputum)	1	23

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 1. IgG (all time points)


IgG (all time points)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	34	0	6	50	0.85 [0.70, 0.94]	1.00 [0.93, 1.00]		
Adams 2020 [D]	21	2	12	58	0.64 [0.45, 0.80]	0.97 [0.88, 1.00]		
Adams 2020 [E]	25	1	13	59	0.66 [0.49, 0.80]	0.98 [0.91, 1.00]		
Adams 2020 [F]	18	1	13	59	0.58 [0.39, 0.75]	0.98 [0.91, 1.00]		
Adams 2020 [G]	17	0	14	60	0.55 [0.36, 0.73]	1.00 [0.94, 1.00]		
Adams 2020 [H]	20	2	13	58	0.61 [0.42, 0.77]	0.97 [0.88, 1.00]		
Adams 2020 [I]	15	0	17	60	0.47 [0.29, 0.65]	1.00 [0.94, 1.00]		
Adams 2020 [J]	17	0	23	142	0.42 [0.27, 0.59]	1.00 [0.97, 1.00]		
Cai 2020a	197	0	79	167	0.71 [0.66, 0.77]	1.00 [0.98, 1.00]		
Cassaniti 2020 (A)	24	0	6	30	0.80 [0.61, 0.92]	1.00 [0.88, 1.00]		
Cassaniti 2020 (B)	5	0	33	12	0.13 [0.04, 0.28]	1.00 [0.74, 1.00]		
Chen 2020a	7	1	0	11	1.00 [0.59, 1.00]	0.92 [0.62, 1.00]		
Du 2020	60	0	0	0	1.00 [0.94, 1.00]	Not estimable		
Freeman 2020	94	0	5	0	0.95 [0.89, 0.98]	Not estimable		
Gao 2020a	35	0	3	0	0.92 [0.79, 0.98]	Not estimable		
Gao 2020b [A]	19	0	18	0	0.51 [0.34, 0.68]	Not estimable		
Gao 2020b [B]	19	0	18	0	0.51 [0.34, 0.68]	Not estimable		
Gao 2020b [C]	24	0	13	0	0.65 [0.47, 0.80]	Not estimable		
Garcia 2020 (A)	23	0	32	45	0.42 [0.29, 0.56]	1.00 [0.92, 1.00]		
Garcia 2020 (B)	56	0	7	0	0.89 [0.78, 0.95]	Not estimable		
Grzelak 2020 [C]	127	23	34	468	0.79 [0.72, 0.85]	0.95 [0.93, 0.97]		
Guo 2020a	162	0	46	135	0.78 [0.72, 0.83]	1.00 [0.97, 1.00]		
Infantino 2020	44	0	17	64	0.72 [0.59, 0.83]	1.00 [0.94, 1.00]		
Jia 2020	31	0	26	0	0.54 [0.41, 0.68]	Not estimable		
Jin 2020	24	3	3	30	0.89 [0.71, 0.98]	0.91 [0.76, 0.98]		
Lassauniere 2020 [B]	20	3	10	79	0.67 [0.47, 0.83]	0.96 [0.90, 0.99]		
Li 2020a	280	0	117	0	0.71 [0.66, 0.75]	Not estimable		
Lin 2020a [A]	65	2	14	78	0.82 [0.72, 0.90]	0.97 [0.91, 1.00]		
Lin 2020a [B]	15	0	50	64	0.23 [0.14, 0.35]	1.00 [0.94, 1.00]		
Lippi 2020 [A]	19	0	29	0	0.40 [0.26, 0.55]	Not estimable		
Lippi 2020 [B]	7	0	41	0	0.15 [0.06, 0.28]	Not estimable		
Liu 2020a	77	5	18	79	0.81 [0.72, 0.88]	0.94 [0.87, 0.98]		
Liu 2020b	168	2	70	118	0.71 [0.64, 0.76]	0.98 [0.94, 1.00]		
Liu 2020c	129	0	4	0	0.97 [0.92, 0.99]	Not estimable		
Liu 2020d [A]	150	0	64	100	0.70 [0.63, 0.76]	1.00 [0.96, 1.00]		
Liu 2020d [B]	159	0	55	100	0.74 [0.68, 0.80]	1.00 [0.96, 1.00]		
Long 2020 (B)	287	0	76	0	0.79 [0.75, 0.83]	Not estimable		
Lou 2020 [A]	71	0	9	100	0.89 [0.80, 0.95]	1.00 [0.96, 1.00]		
Lou 2020 [B]	69	1	11	208	0.86 [0.77, 0.93]	1.00 [0.97, 1.00]		
Ma 2020a	209	1	7	482	0.97 [0.93, 0.99]	1.00 [0.99, 1.00]		
Okba 2020a	11	0	20	45	0.35 [0.19, 0.55]	1.00 [0.92, 1.00]		
Padoan 2020	57	0	13	0	0.81 [0.70, 0.90]	Not estimable		
Pan 2020a	60	0	48	0	0.56 [0.46, 0.65]	Not estimable		
Qian 2020	531	30	24	1528	0.96 [0.94, 0.97]	0.98 [0.97, 0.99]		
To 2020a [A]	15	0	1	0	0.94 [0.70, 1.00]	Not estimable		
To 2020a [B]	16	0	0	0	1.00 [0.79, 1.00]	Not estimable		
Wan 2020 [A]	6	0	1	10	0.86 [0.42, 1.00]	1.00 [0.69, 1.00]		
Wang 2020a [A]	14	22	0	50	1.00 [0.77, 1.00]	0.69 [0.57, 0.80]		
Xiang 2020a [A]	52	0	11	35	0.83 [0.71, 0.91]	1.00 [0.90, 1.00]		
Xiang 2020a [B]	74	0	17	35	0.81 [0.72, 0.89]	1.00 [0.90, 1.00]		
Xiang 2020b	72	3	18	57	0.80 [0.70, 0.88]	0.95 [0.86, 0.99]		
Xiao 2020a	32	0	2	0	0.94 [0.80, 0.99]	Not estimable		
Xie 2020a	56	0	0	0	1.00 [0.94, 1.00]	Not estimable		
Xu 2020a	3	0	7	0	0.30 [0.07, 0.65]	Not estimable		
Zeng 2020a	0	0	27	36	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]		
Zhang 2020a	219	0	3	0	0.99 [0.96, 1.00]	Not estimable		
Zhang 2020b	3	1	0	224	1.00 [0.29, 1.00]	1.00 [0.98, 1.00]		
Zhang 2020c	13	0	3	0	0.81 [0.54, 0.96]	Not estimable		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 1. (Continued)


Zhang 2020b	3	1	0	224	1.00 [0.29, 1.00]	1.00 [0.98, 1.00]
Zhang 2020c	13	0	3	0	0.81 [0.54, 0.96]	Not estimable
Zhao 2020a	112	2	61	195	0.65 [0.57, 0.72]	0.99 [0.96, 1.00]
Zhong 2020 [A]	46	1	1	299	0.98 [0.89, 1.00]	1.00 [0.98, 1.00]
Zhong 2020 [B]	45	43	2	257	0.96 [0.85, 0.99]	0.86 [0.81, 0.89]
Zhong 2020 [C]	45	10	2	290	0.96 [0.85, 0.99]	0.97 [0.94, 0.98]

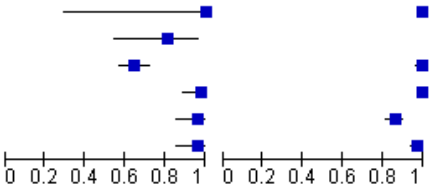

Test 2. IgG (1 to 7 days)

IgG (1 to 7 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [D]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [H]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [J]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Gao 2020a	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Gao 2020b [A]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Gao 2020b [B]	2	0	8	0	0.20 [0.03, 0.56]	Not estimable
Gao 2020b [C]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Garcia 2020 (A)	1	0	7	0	0.13 [0.00, 0.53]	Not estimable
Hu 2020a	11	0	14	0	0.44 [0.24, 0.65]	Not estimable
Jin 2020	2	0	4	0	0.33 [0.04, 0.78]	Not estimable
Lin 2020a [A]	8	0	4	0	0.67 [0.35, 0.90]	Not estimable
Lippi 2020 [A]	7	0	23	0	0.23 [0.10, 0.42]	Not estimable
Lippi 2020 [B]	0	0	30	0	0.00 [0.00, 0.12]	Not estimable
Liu 2020a	2	0	14	0	0.13 [0.02, 0.38]	Not estimable
Liu 2020b	4	0	13	0	0.24 [0.07, 0.50]	Not estimable
Liu 2020d [A]	7	0	15	0	0.32 [0.14, 0.55]	Not estimable
Liu 2020d [B]	9	0	13	0	0.41 [0.21, 0.64]	Not estimable
Long 2020 (B)	32	0	35	0	0.48 [0.35, 0.60]	Not estimable
Lou 2020 [A]	13	0	26	0	0.33 [0.19, 0.50]	Not estimable
Ma 2020a	15	0	2	0	0.88 [0.64, 0.99]	Not estimable
Okba 2020a	0	0	12	0	0.00 [0.00, 0.26]	Not estimable
Padoan 2020	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Pan 2020a	5	0	31	0	0.14 [0.05, 0.29]	Not estimable
Wan 2020 [A]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Xiang 2020b	6	0	8	0	0.43 [0.18, 0.71]	Not estimable
Xiao 2020a	0	0	2	0	0.00 [0.00, 0.84]	Not estimable
Zeng 2020a	0	0	27	0	0.00 [0.00, 0.13]	Not estimable
Zhao 2020a	18	0	76	0	0.19 [0.12, 0.29]	Not estimable

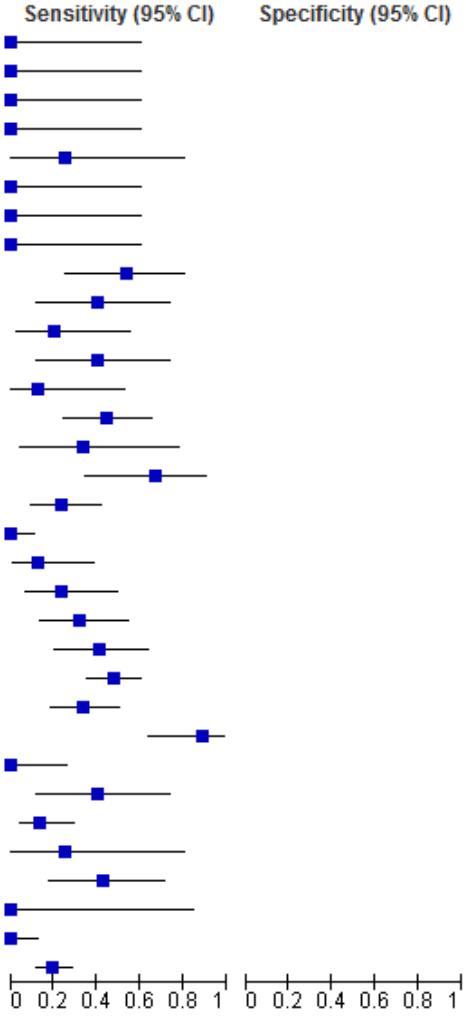


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 3. IgG (8 to 14 days)

IgG (8 to 14 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	11	0	2	0	0.85 [0.55, 0.98]	Not estimable
Adams 2020 [D]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [E]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [F]	9	0	4	0	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [G]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [H]	9	0	4	0	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [I]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [J]	6	0	7	0	0.46 [0.19, 0.75]	Not estimable
Gao 2020a	7	0	1	0	0.88 [0.47, 1.00]	Not estimable
Gao 2020b [A]	6	0	7	0	0.46 [0.19, 0.75]	Not estimable
Gao 2020b [B]	6	0	7	0	0.46 [0.19, 0.75]	Not estimable
Gao 2020b [C]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Garcia 2020 (A)	6	0	18	0	0.25 [0.10, 0.47]	Not estimable
Garcia 2020 (B)	15	0	3	0	0.83 [0.59, 0.96]	Not estimable
Hu 2020a	97	0	48	0	0.67 [0.59, 0.74]	Not estimable
Jin 2020	26	0	1	0	0.96 [0.81, 1.00]	Not estimable
Lassauniere 2020 [B]	6	0	1	0	0.86 [0.42, 1.00]	Not estimable
Lin 2020a [A]	24	0	9	0	0.73 [0.54, 0.87]	Not estimable
Lippi 2020 [A]	12	0	6	0	0.67 [0.41, 0.87]	Not estimable
Lippi 2020 [B]	7	0	11	0	0.39 [0.17, 0.64]	Not estimable
Liu 2020a	5	0	1	0	0.83 [0.36, 1.00]	Not estimable
Liu 2020b	62	0	48	0	0.56 [0.47, 0.66]	Not estimable
Liu 2020d [A]	54	0	38	0	0.59 [0.48, 0.69]	Not estimable
Liu 2020d [B]	60	0	32	0	0.65 [0.55, 0.75]	Not estimable
Long 2020 (B)	32	0	35	0	0.48 [0.35, 0.60]	Not estimable
Lou 2020 [A]	57	0	18	0	0.76 [0.65, 0.85]	Not estimable
Ma 2020a	29	0	1	0	0.97 [0.83, 1.00]	Not estimable
Okba 2020a	3	0	7	0	0.30 [0.07, 0.65]	Not estimable
Padoan 2020	28	0	7	0	0.80 [0.63, 0.92]	Not estimable
Pan 2020a	20	0	14	0	0.59 [0.41, 0.75]	Not estimable
Wan 2020 [A]	3	0	2	0	0.60 [0.15, 0.95]	Not estimable
Xiang 2020b	47	0	39	0	0.55 [0.44, 0.65]	Not estimable
Xiao 2020a	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Zhao 2020a	73	0	62	0	0.54 [0.45, 0.63]	Not estimable

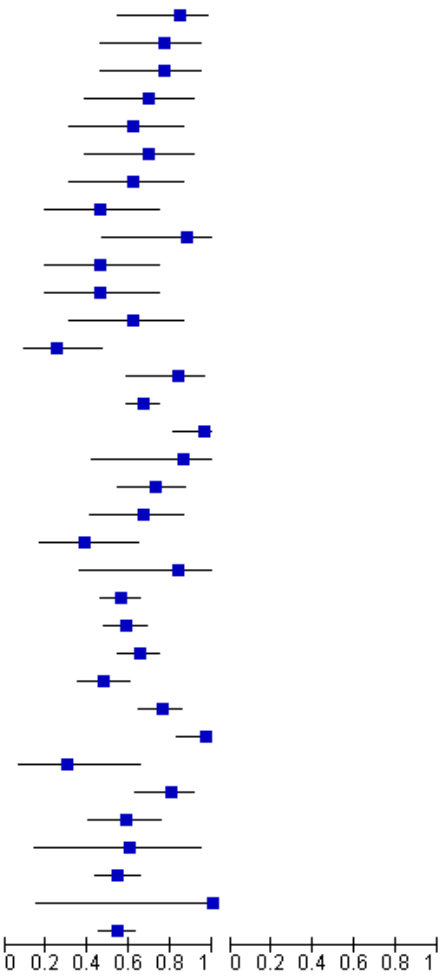


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 4. IgG (15 to 21 days)

IgG (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [D]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [E]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [F]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [G]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [H]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [I]	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [J]	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Gao 2020a	21	0	2	0	0.91 [0.72, 0.99]	Not estimable
Gao 2020b [A]	9	0	5	0	0.64 [0.35, 0.87]	Not estimable
Gao 2020b [B]	11	0	3	0	0.79 [0.49, 0.95]	Not estimable
Gao 2020b [C]	12	0	2	0	0.86 [0.57, 0.98]	Not estimable
Garcia 2020 (A)	16	0	7	0	0.70 [0.47, 0.87]	Not estimable
Garcia 2020 (B)	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Hu 2020a	81	0	29	0	0.74 [0.64, 0.82]	Not estimable
Jin 2020	21	0	1	0	0.95 [0.77, 1.00]	Not estimable
Lassauniere 2020 [B]	14	0	1	0	0.93 [0.68, 1.00]	Not estimable
Lin 2020a [A]	33	0	1	0	0.97 [0.85, 1.00]	Not estimable
Liu 2020a	68	0	0	0	1.00 [0.95, 1.00]	Not estimable
Liu 2020b	102	0	9	0	0.92 [0.85, 0.96]	Not estimable
Liu 2020d [A]	48	0	7	0	0.87 [0.76, 0.95]	Not estimable
Liu 2020d [B]	51	0	4	0	0.93 [0.82, 0.98]	Not estimable
Long 2020 (B)	127	0	7	0	0.95 [0.90, 0.98]	Not estimable
Lou 2020 [A]	56	0	4	0	0.93 [0.84, 0.98]	Not estimable
Ma 2020a	55	0	0	0	1.00 [0.94, 1.00]	Not estimable
Okba 2020a	7	0	1	0	0.88 [0.47, 1.00]	Not estimable
Padoan 2020	25	0	0	0	1.00 [0.86, 1.00]	Not estimable
Pan 2020a	35	0	3	0	0.92 [0.79, 0.98]	Not estimable
Wan 2020 [A]	3	0	0	0	1.00 [0.29, 1.00]	Not estimable
Xiang 2020b	47	0	10	0	0.82 [0.70, 0.91]	Not estimable
Xiao 2020a	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Zhao 2020a	71	0	18	0	0.80 [0.70, 0.88]	Not estimable

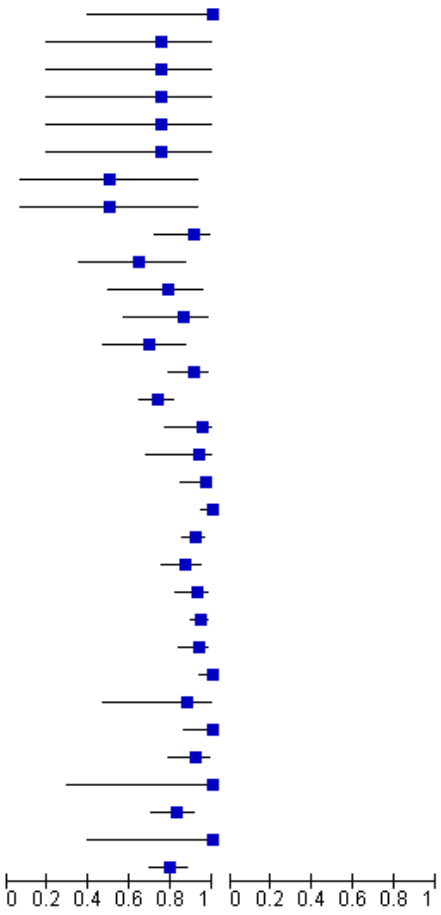


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 5. IgG (22 to 35 days)

IgG (22 to 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Adams 2020 [D]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [E]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [F]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Du 2020	7	0	0	0	1.00 [0.59, 1.00]	Not estimable
Hu 2020a	85	0	66	0	0.56 [0.48, 0.64]	Not estimable
Jin 2020	45	0	0	0	1.00 [0.92, 1.00]	Not estimable
Lassauniere 2020 [B]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Liu 2020d [A]	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Liu 2020d [B]	39	0	6	0	0.87 [0.73, 0.95]	Not estimable
Long 2020 (B)	13	0	0	0	1.00 [0.75, 1.00]	Not estimable
Ma 2020a	91	0	0	0	1.00 [0.96, 1.00]	Not estimable
Okba 2020a	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Wan 2020 [A]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Xiang 2020b	50	0	9	0	0.85 [0.73, 0.93]	Not estimable
Xiao 2020a	19	0	0	0	1.00 [0.82, 1.00]	Not estimable

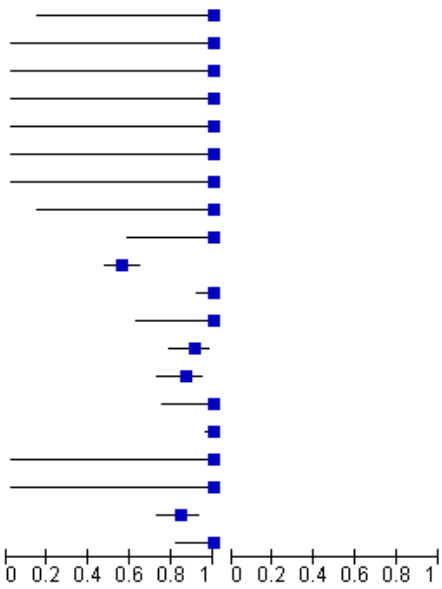

Test 6. IgG (over 35 days)

IgG (over 35 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	17	0	0	0	1.00 [0.80, 1.00]	Not estimable
Adams 2020 [D]	7	0	4	0	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [E]	11	0	5	0	0.69 [0.41, 0.89]	Not estimable
Adams 2020 [F]	5	0	4	0	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [G]	4	0	5	0	0.44 [0.14, 0.79]	Not estimable
Adams 2020 [H]	7	0	4	0	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [I]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Adams 2020 [J]	7	0	10	0	0.41 [0.18, 0.67]	Not estimable
Du 2020	53	0	0	0	1.00 [0.93, 1.00]	Not estimable
Hu 2020a	75	0	1	0	0.99 [0.93, 1.00]	Not estimable
Ma 2020a	23	0	0	0	1.00 [0.85, 1.00]	Not estimable
Xiao 2020a	7	0	0	0	1.00 [0.59, 1.00]	Not estimable

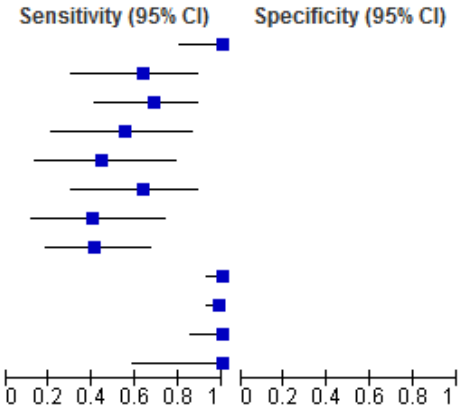


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 7. IgM (all time points)

IgM (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	28	0	12	50	0.70 [0.53, 0.83]	1.00 [0.93, 1.00]
Adams 2020 [D]	3	0	30	60	0.09 [0.02, 0.24]	1.00 [0.94, 1.00]
Adams 2020 [E]	2	0	36	60	0.05 [0.01, 0.18]	1.00 [0.94, 1.00]
Adams 2020 [F]	15	1	16	59	0.48 [0.30, 0.67]	0.98 [0.91, 1.00]
Adams 2020 [G]	14	1	17	59	0.45 [0.27, 0.64]	0.98 [0.91, 1.00]
Adams 2020 [H]	17	1	16	59	0.52 [0.34, 0.69]	0.98 [0.91, 1.00]
Adams 2020 [I]	14	0	18	60	0.44 [0.26, 0.62]	1.00 [0.94, 1.00]
Adams 2020 [J]	15	4	25	138	0.38 [0.23, 0.54]	0.97 [0.93, 0.99]
Cai 2020a	158	0	118	167	0.57 [0.51, 0.63]	1.00 [0.98, 1.00]
Cassaniti 2020 (A)	25	0	5	30	0.83 [0.65, 0.94]	1.00 [0.88, 1.00]
Cassaniti 2020 (B)	6	1	32	11	0.16 [0.06, 0.31]	0.92 [0.62, 1.00]
Du 2020	47	0	13	0	0.78 [0.66, 0.88]	Not estimable
Freeman 2020	75	0	24	0	0.76 [0.66, 0.84]	Not estimable
Gao 2020a	19	0	19	0	0.50 [0.33, 0.67]	Not estimable
Gao 2020b [A]	14	0	23	0	0.38 [0.22, 0.55]	Not estimable
Gao 2020b [B]	19	0	18	0	0.51 [0.34, 0.68]	Not estimable
Gao 2020b [C]	11	0	26	0	0.30 [0.16, 0.47]	Not estimable
Garcia 2020 (A)	12	0	43	45	0.22 [0.12, 0.35]	1.00 [0.92, 1.00]
Garcia 2020 (B)	25	0	38	0	0.40 [0.28, 0.53]	Not estimable
Guo 2020a	188	0	20	135	0.90 [0.86, 0.94]	1.00 [0.97, 1.00]
Infantino 2020	46	4	15	59	0.75 [0.63, 0.86]	0.94 [0.85, 0.98]
Jia 2020	39	0	18	0	0.68 [0.55, 0.80]	Not estimable
Jin 2020	13	0	14	33	0.48 [0.29, 0.68]	1.00 [0.89, 1.00]
Li 2020a	328	0	69	0	0.83 [0.79, 0.86]	Not estimable
Lin 2020a [A]	65	15	14	65	0.82 [0.72, 0.90]	0.81 [0.71, 0.89]
Lin 2020a [B]	30	14	35	50	0.46 [0.34, 0.59]	0.78 [0.66, 0.87]
Lippi 2020 [A]	6	0	42	0	0.13 [0.05, 0.25]	Not estimable
Liu 2020a	35	5	60	79	0.37 [0.27, 0.47]	0.94 [0.87, 0.98]
Liu 2020b	167	3	71	117	0.70 [0.64, 0.76]	0.97 [0.93, 0.99]
Liu 2020c	105	0	28	0	0.79 [0.71, 0.86]	Not estimable
Liu 2020d [A]	146	0	68	100	0.68 [0.62, 0.74]	1.00 [0.96, 1.00]
Liu 2020d [B]	165	0	49	100	0.77 [0.71, 0.83]	1.00 [0.96, 1.00]
Long 2020 (B)	243	0	120	0	0.67 [0.62, 0.72]	Not estimable
Lou 2020 [A]	74	0	6	300	0.93 [0.84, 0.97]	1.00 [0.99, 1.00]
Lou 2020 [B]	71	4	9	205	0.89 [0.80, 0.95]	0.98 [0.95, 0.99]
Lou 2020 [C]	69	2	11	298	0.86 [0.77, 0.93]	0.99 [0.98, 1.00]
Ma 2020a	209	37	7	446	0.97 [0.93, 0.99]	0.92 [0.90, 0.95]
Padoan 2020	44	0	26	0	0.63 [0.50, 0.74]	Not estimable
Pan 2020a	56	0	52	0	0.52 [0.42, 0.62]	Not estimable
Qian 2020	470	29	85	1529	0.85 [0.81, 0.88]	0.98 [0.97, 0.99]
To 2020a [A]	14	0	2	0	0.88 [0.62, 0.98]	Not estimable
To 2020a [B]	15	0	1	0	0.94 [0.70, 1.00]	Not estimable
Wan 2020 [A]	2	1	5	9	0.29 [0.04, 0.71]	0.90 [0.55, 1.00]
Wang 2020a [B]	14	22	0	50	1.00 [0.77, 1.00]	0.69 [0.57, 0.80]
Xiang 2020a [A]	35	0	28	35	0.56 [0.42, 0.68]	1.00 [0.90, 1.00]
Xiang 2020a [B]	52	0	39	35	0.57 [0.46, 0.67]	1.00 [0.90, 1.00]
Xiang 2020b	72	0	18	60	0.80 [0.70, 0.88]	1.00 [0.94, 1.00]
Xiao 2020a	28	0	6	0	0.82 [0.65, 0.93]	Not estimable
Xie 2020a	49	0	7	0	0.88 [0.76, 0.95]	Not estimable
Xu 2020a	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Zeng 2020a	0	0	27	36	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]
Zhang 2020a	182	0	40	0	0.82 [0.76, 0.87]	Not estimable
Zhang 2020b	3	6	0	219	1.00 [0.29, 1.00]	0.97 [0.94, 0.99]
Zhang 2020c	16	0	0	0	1.00 [0.79, 1.00]	Not estimable
Zhao 2020a	143	3	30	210	0.83 [0.76, 0.88]	0.99 [0.96, 1.00]
Zhong 2020 [A]	46	1	1	299	0.98 [0.89, 1.00]	1.00 [0.98, 1.00]
Zhong 2020 [B]	42	9	5	291	0.89 [0.77, 0.96]	0.97 [0.94, 0.99]

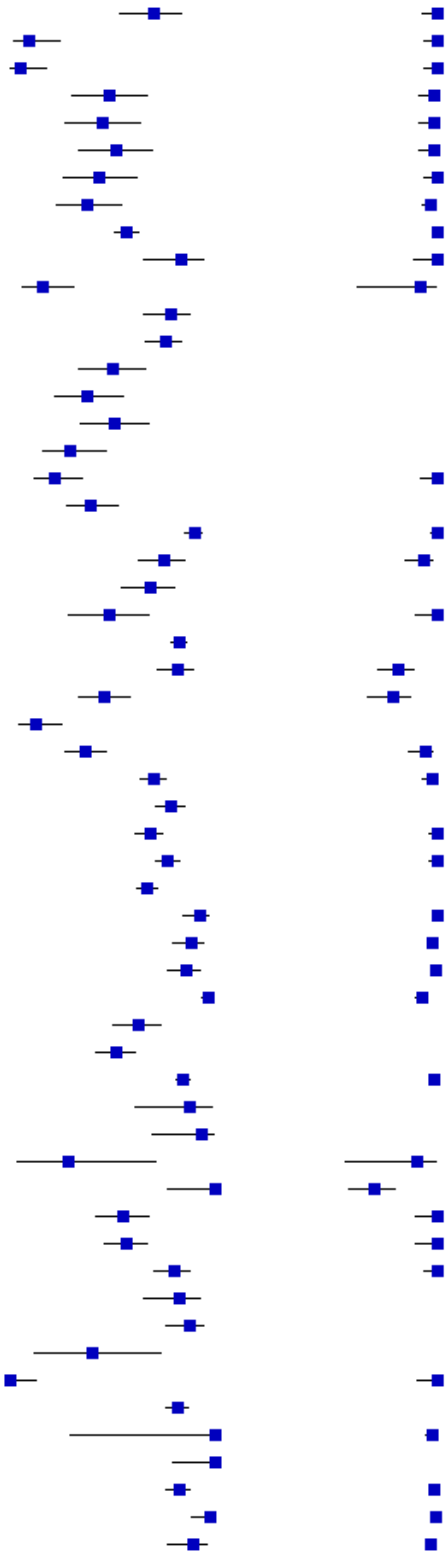

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 7. (Continued)


Zhong 2020 [A]	46	1	1	299	0.98 [0.89, 1.00]	1.00 [0.98, 1.00]
Zhong 2020 [B]	42	9	5	291	0.89 [0.77, 0.96]	0.97 [0.94, 0.99]
Zhong 2020 [C]	46	14	1	286	0.98 [0.89, 1.00]	0.95 [0.92, 0.97]



Test 8. IgM (8 to 14 days)

IgM (8 to 14 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	11	0	2	0	0.85 [0.55, 0.98]	Not estimable
Adams 2020 [D]	2	0	11	0	0.15 [0.02, 0.45]	Not estimable
Adams 2020 [E]	1	0	12	0	0.08 [0.00, 0.36]	Not estimable
Adams 2020 [F]	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Adams 2020 [G]	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Adams 2020 [H]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [I]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [J]	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Gao 2020a	4	0	4	0	0.50 [0.16, 0.84]	Not estimable
Gao 2020b [A]	4	0	9	0	0.31 [0.09, 0.61]	Not estimable
Gao 2020b [B]	5	0	8	0	0.38 [0.14, 0.68]	Not estimable
Gao 2020b [C]	1	0	12	0	0.08 [0.00, 0.36]	Not estimable
Garcia 2020 (A)	3	0	21	0	0.13 [0.03, 0.32]	Not estimable
Garcia 2020 (B)	7	0	11	0	0.39 [0.17, 0.64]	Not estimable
Hu 2020a	78	0	48	0	0.62 [0.53, 0.70]	Not estimable
Jin 2020	12	0	15	0	0.44 [0.25, 0.65]	Not estimable
Lin 2020a [A]	24	0	9	0	0.73 [0.54, 0.87]	Not estimable
Lippi 2020 [A]	5	0	13	0	0.28 [0.10, 0.53]	Not estimable
Liu 2020a	6	0	0	0	1.00 [0.54, 1.00]	Not estimable
Liu 2020b	72	0	38	0	0.65 [0.56, 0.74]	Not estimable
Liu 2020d [A]	59	0	33	0	0.64 [0.53, 0.74]	Not estimable
Liu 2020d [B]	64	0	28	0	0.70 [0.59, 0.79]	Not estimable
Long 2020 (B)	21	0	46	0	0.31 [0.21, 0.44]	Not estimable
Lou 2020 [A]	65	0	10	0	0.87 [0.77, 0.93]	Not estimable
Ma 2020a	30	0	0	0	1.00 [0.88, 1.00]	Not estimable
Padoan 2020	19	0	16	0	0.54 [0.37, 0.71]	Not estimable
Pan 2020a	24	0	10	0	0.71 [0.53, 0.85]	Not estimable
Wan 2020 [A]	1	0	4	0	0.20 [0.01, 0.72]	Not estimable
Xiang 2020b	57	0	29	0	0.66 [0.55, 0.76]	Not estimable
Xiao 2020a	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Zhao 2020a	99	0	36	0	0.73 [0.65, 0.81]	Not estimable

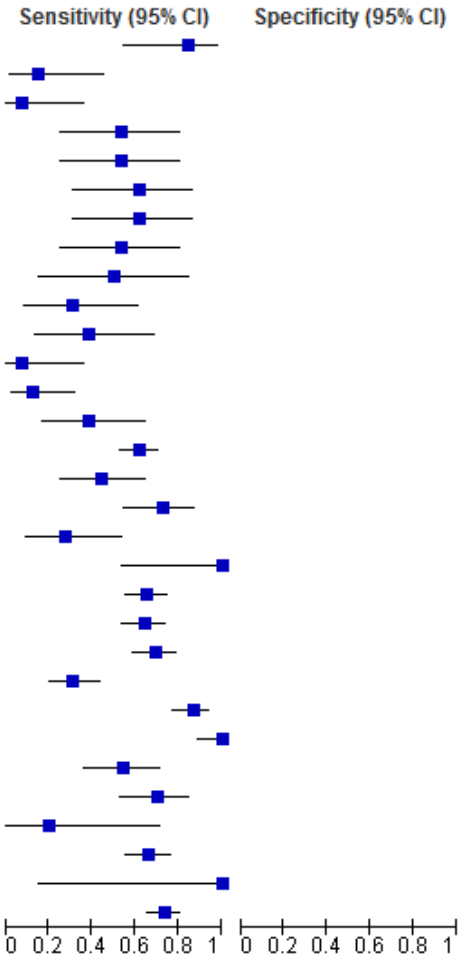


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 9. IgM (1 to 7 days)

IgM (1 to 7 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [D]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [H]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [J]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Gao 2020a	3	0	10	0	0.23 [0.05, 0.54]	Not estimable
Gao 2020b [A]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Gao 2020b [B]	5	0	5	0	0.50 [0.19, 0.81]	Not estimable
Gao 2020b [C]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Garcia 2020 (A)	0	0	8	0	0.00 [0.00, 0.37]	Not estimable
Guo 2020a	35	0	6	0	0.85 [0.71, 0.94]	Not estimable
Hu 2020a	7	0	14	0	0.33 [0.15, 0.57]	Not estimable
Jin 2020	1	0	5	0	0.17 [0.00, 0.64]	Not estimable
Lin 2020a [A]	10	0	2	0	0.83 [0.52, 0.98]	Not estimable
Lippi 2020 [A]	1	0	29	0	0.03 [0.00, 0.17]	Not estimable
Liu 2020a	3	0	13	0	0.19 [0.04, 0.46]	Not estimable
Liu 2020b	3	0	14	0	0.18 [0.04, 0.43]	Not estimable
Liu 2020d [A]	7	0	15	0	0.32 [0.14, 0.55]	Not estimable
Liu 2020d [B]	8	0	14	0	0.36 [0.17, 0.59]	Not estimable
Long 2020 (B)	21	0	46	0	0.31 [0.21, 0.44]	Not estimable
Lou 2020 [A]	13	0	26	0	0.33 [0.19, 0.50]	Not estimable
Ma 2020a	11	0	6	0	0.65 [0.38, 0.86]	Not estimable
Padoan 2020	3	0	7	0	0.30 [0.07, 0.65]	Not estimable
Pan 2020a	5	0	31	0	0.14 [0.05, 0.29]	Not estimable
Wan 2020 [A]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Wang 2020a [A]	14	0	0	50	1.00 [0.77, 1.00]	1.00 [0.93, 1.00]
Wang 2020a [B]	14	0	0	0	1.00 [0.77, 1.00]	Not estimable
Xiang 2020b	7	0	7	0	0.50 [0.23, 0.77]	Not estimable
Xiao 2020a	0	0	2	0	0.00 [0.00, 0.84]	Not estimable
Zeng 2020a	0	0	27	0	0.00 [0.00, 0.13]	Not estimable
Zhao 2020a	27	0	67	0	0.29 [0.20, 0.39]	Not estimable

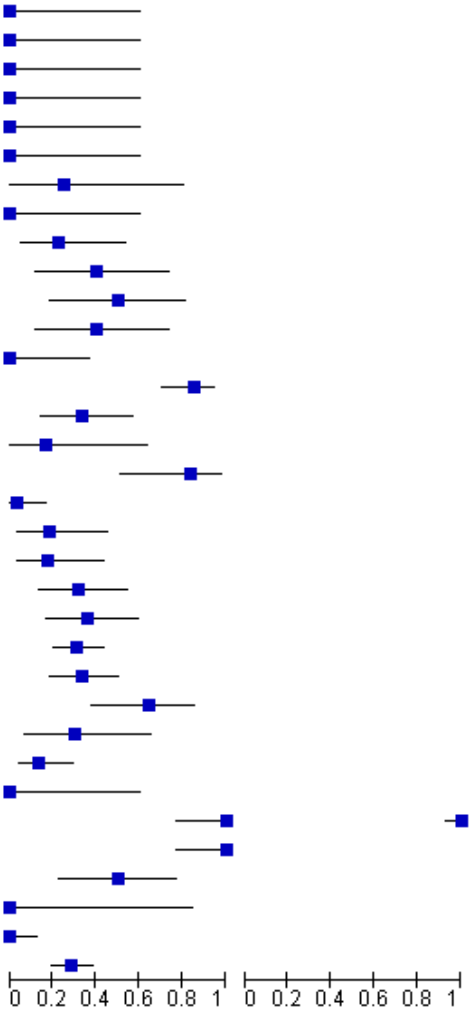


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 10. IgM (15 to 21 days)

IgM (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [D]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [G]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [H]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [I]	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [J]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Gao 2020a	12	0	11	0	0.52 [0.31, 0.73]	Not estimable
Gao 2020b [A]	6	0	8	0	0.43 [0.18, 0.71]	Not estimable
Gao 2020b [B]	9	0	5	0	0.64 [0.35, 0.87]	Not estimable
Gao 2020b [C]	6	0	8	0	0.43 [0.18, 0.71]	Not estimable
Garcia 2020 (A)	9	0	14	0	0.39 [0.20, 0.61]	Not estimable
Garcia 2020 (B)	18	0	27	0	0.40 [0.26, 0.56]	Not estimable
Hu 2020a	54	0	29	0	0.65 [0.54, 0.75]	Not estimable
Jin 2020	16	0	6	0	0.73 [0.50, 0.89]	Not estimable
Lin 2020a [A]	31	0	3	0	0.91 [0.76, 0.98]	Not estimable
Liu 2020a	25	0	43	0	0.37 [0.25, 0.49]	Not estimable
Liu 2020b	92	0	19	0	0.83 [0.75, 0.89]	Not estimable
Liu 2020d [A]	45	0	10	0	0.82 [0.69, 0.91]	Not estimable
Liu 2020d [B]	53	0	2	0	0.96 [0.87, 1.00]	Not estimable
Long 2020 (B)	113	0	21	0	0.84 [0.77, 0.90]	Not estimable
Lou 2020 [A]	58	0	2	0	0.97 [0.88, 1.00]	Not estimable
Ma 2020a	55	0	0	0	1.00 [0.94, 1.00]	Not estimable
Padoan 2020	22	0	3	0	0.88 [0.69, 0.97]	Not estimable
Pan 2020a	27	0	11	0	0.71 [0.54, 0.85]	Not estimable
Wan 2020 [A]	2	0	1	0	0.67 [0.09, 0.99]	Not estimable
Xiang 2020b	45	0	12	0	0.79 [0.66, 0.89]	Not estimable
Xiao 2020a	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Zhao 2020a	83	0	5	0	0.94 [0.87, 0.98]	Not estimable

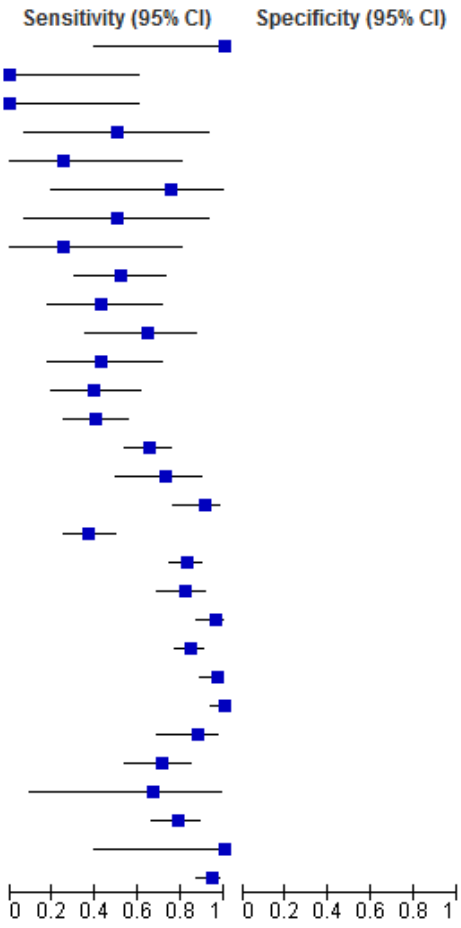


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 11. IgM (22 to 35 days)

IgM (22 to 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	2	0	6	0	0.25 [0.03, 0.65]	Not estimable
Adams 2020 [D]	0	0	1	0	0.00 [0.00, 0.97]	Not estimable
Adams 2020 [E]	0	0	1	0	0.00 [0.00, 0.97]	Not estimable
Adams 2020 [F]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	1	0	1	0	0.50 [0.01, 0.99]	Not estimable
Du 2020	7	0	0	0	1.00 [0.59, 1.00]	Not estimable
Hu 2020a	85	0	66	0	0.56 [0.48, 0.64]	Not estimable
Jin 2020	29	0	16	0	0.64 [0.49, 0.78]	Not estimable
Liu 2020d [A]	35	0	10	0	0.78 [0.63, 0.89]	Not estimable
Liu 2020d [B]	40	0	5	0	0.89 [0.76, 0.96]	Not estimable
Long 2020 (B)	12	0	1	0	0.92 [0.64, 1.00]	Not estimable
Ma 2020a	91	0	0	0	1.00 [0.96, 1.00]	Not estimable
Wan 2020 [A]	0	0	1	0	0.00 [0.00, 0.97]	Not estimable
Xiang 2020b	43	0	16	0	0.73 [0.60, 0.84]	Not estimable
Xiao 2020a	17	0	2	0	0.89 [0.67, 0.99]	Not estimable

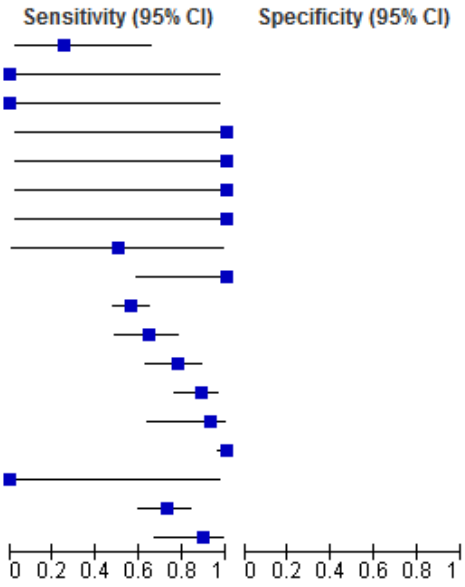

Test 12. IgM (over 35 days)

IgM (over 35 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	11	0	6	0	0.65 [0.38, 0.86]	Not estimable
Adams 2020 [D]	1	0	10	0	0.09 [0.00, 0.41]	Not estimable
Adams 2020 [E]	1	0	15	0	0.06 [0.00, 0.30]	Not estimable
Adams 2020 [F]	5	0	4	0	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [G]	5	0	4	0	0.56 [0.21, 0.86]	Not estimable
Adams 2020 [H]	5	0	6	0	0.45 [0.17, 0.77]	Not estimable
Adams 2020 [I]	0	0	0	0	Not estimable	Not estimable
Adams 2020 [J]	6	0	11	0	0.35 [0.14, 0.62]	Not estimable
Du 2020	40	0	13	0	0.75 [0.62, 0.86]	Not estimable
Hu 2020a	24	0	25	0	0.49 [0.34, 0.64]	Not estimable
Ma 2020a	20	0	3	0	0.87 [0.66, 0.97]	Not estimable
Xiao 2020a	5	0	2	0	0.71 [0.29, 0.96]	Not estimable

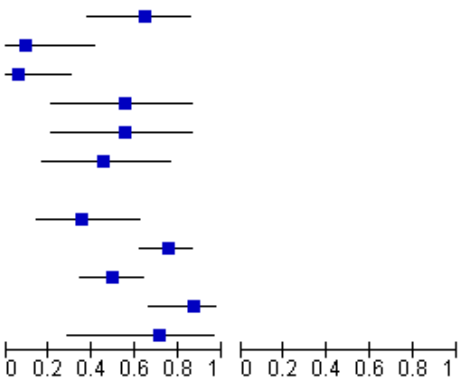


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 13. IgG/IgM (all time points)

IgG/IgM (all time points)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	34	0	6	50	0.85 [0.70, 0.94]	1.00 [0.93, 1.00]
Adams 2020 [D]	21	2	12	58	0.64 [0.45, 0.80]	0.97 [0.88, 1.00]
Adams 2020 [E]	25	1	13	59	0.66 [0.49, 0.80]	0.98 [0.91, 1.00]
Adams 2020 [F]	19	2	12	58	0.61 [0.42, 0.78]	0.97 [0.88, 1.00]
Adams 2020 [G]	20	1	11	59	0.65 [0.45, 0.81]	0.98 [0.91, 1.00]
Adams 2020 [H]	23	3	10	57	0.70 [0.51, 0.84]	0.95 [0.86, 0.99]
Adams 2020 [I]	18	0	14	60	0.56 [0.38, 0.74]	1.00 [0.94, 1.00]
Adams 2020 [J]	22	4	18	138	0.55 [0.38, 0.71]	0.97 [0.93, 0.99]
Bendavid 2020	130	16	27	3308	0.83 [0.76, 0.88]	1.00 [0.99, 1.00]
Cai 2020a	225	0	51	167	0.82 [0.76, 0.86]	1.00 [0.98, 1.00]
Cassaniti 2020 (A)	25	0	5	30	0.83 [0.65, 0.94]	1.00 [0.88, 1.00]
Cassaniti 2020 (B)	7	1	31	11	0.18 [0.08, 0.34]	0.92 [0.62, 1.00]
Dohla 2020	8	3	14	24	0.36 [0.17, 0.59]	0.89 [0.71, 0.98]
Du 2020	60	0	0	0	1.00 [0.94, 1.00]	Not estimable
Garcia 2020 (A)	26	0	29	45	0.47 [0.34, 0.61]	1.00 [0.92, 1.00]
Garcia 2020 (B)	56	0	7	0	0.89 [0.78, 0.95]	Not estimable
Grzelak 2020 [D]	106	0	14	134	0.88 [0.81, 0.93]	1.00 [0.97, 1.00]
Infantino 2020	49	4	12	59	0.80 [0.68, 0.89]	0.94 [0.85, 0.98]
Jia 2020	45	0	12	0	0.79 [0.66, 0.89]	Not estimable
Jin 2020	24	3	3	30	0.89 [0.71, 0.98]	0.91 [0.76, 0.98]
Lassauniere 2020 [D]	27	0	3	32	0.90 [0.73, 0.98]	1.00 [0.89, 1.00]
Lassauniere 2020 [E]	27	0	3	32	0.90 [0.73, 0.98]	1.00 [0.89, 1.00]
Lassauniere 2020 [F]	28	0	2	32	0.93 [0.78, 0.99]	1.00 [0.89, 1.00]
Lassauniere 2020 [G]	25	0	5	17	0.83 [0.65, 0.94]	1.00 [0.80, 1.00]
Lassauniere 2020 [H]	4	3	1	12	0.80 [0.28, 0.99]	0.80 [0.52, 0.96]
Lassauniere 2020 [I]	1	2	0	13	1.00 [0.03, 1.00]	0.87 [0.60, 0.98]
Li 2020a	352	0	45	0	0.89 [0.85, 0.92]	Not estimable
Lin 2020a [A]	72	16	7	64	0.91 [0.83, 0.96]	0.80 [0.70, 0.88]
Liu 2020a	79	6	16	78	0.83 [0.74, 0.90]	0.93 [0.85, 0.97]
Liu 2020b	194	4	44	116	0.82 [0.76, 0.86]	0.97 [0.92, 0.99]
Liu 2020d [A]	172	0	42	100	0.80 [0.74, 0.85]	1.00 [0.96, 1.00]
Liu 2020d [B]	176	0	38	100	0.82 [0.76, 0.87]	1.00 [0.96, 1.00]
Long 2020 (A)	16	7	0	141	1.00 [0.79, 1.00]	0.95 [0.90, 0.98]
Long 2020 (B)	302	0	61	0	0.83 [0.79, 0.87]	Not estimable
Ma 2020a	213	0	3	483	0.99 [0.96, 1.00]	1.00 [0.99, 1.00]
Pan 2020a	73	0	35	0	0.68 [0.58, 0.76]	Not estimable
Paradiso 2020a	21	13	49	107	0.30 [0.20, 0.42]	0.89 [0.82, 0.94]
Wan 2020 [A]	6	0	1	10	0.86 [0.42, 1.00]	1.00 [0.69, 1.00]
Xiang 2020a [A]	55	0	8	35	0.87 [0.77, 0.94]	1.00 [0.90, 1.00]
Xiang 2020a [B]	75	0	16	35	0.82 [0.73, 0.90]	1.00 [0.90, 1.00]
Xu 2020a	9	0	1	0	0.90 [0.55, 1.00]	Not estimable
Yongchen 2020	17	0	4	0	0.81 [0.58, 0.95]	Not estimable
Zeng 2020a	0	0	27	36	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]
Zhang 2020c	13	0	3	0	0.81 [0.54, 0.96]	Not estimable

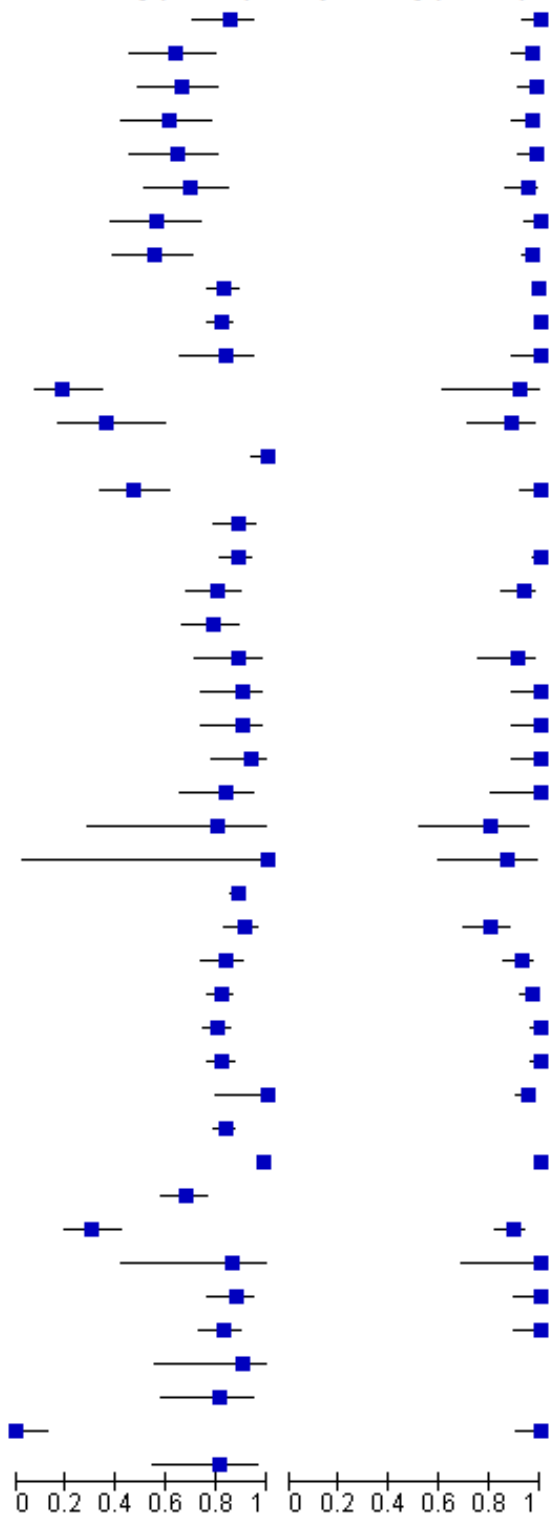


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 14. IgG/IgM (1 to 7 days)

IgG/IgM (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [D]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [E]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [F]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [G]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [H]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [I]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Adams 2020 [J]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Garcia 2020 (A)	1	0	7	0	0.13 [0.00, 0.53]	Not estimable
Lin 2020a [A]	10	0	2	0	0.83 [0.52, 0.98]	Not estimable
Liu 2020a	3	0	13	0	0.19 [0.04, 0.46]	Not estimable
Liu 2020b	5	0	12	0	0.29 [0.10, 0.56]	Not estimable
Liu 2020d [A]	9	0	13	0	0.41 [0.21, 0.64]	Not estimable
Liu 2020d [B]	10	0	12	0	0.45 [0.24, 0.68]	Not estimable
Long 2020 (B)	34	0	33	0	0.51 [0.38, 0.63]	Not estimable
Pan 2020a	7	0	29	0	0.19 [0.08, 0.36]	Not estimable
Zeng 2020a	0	0	27	0	0.00 [0.00, 0.13]	Not estimable

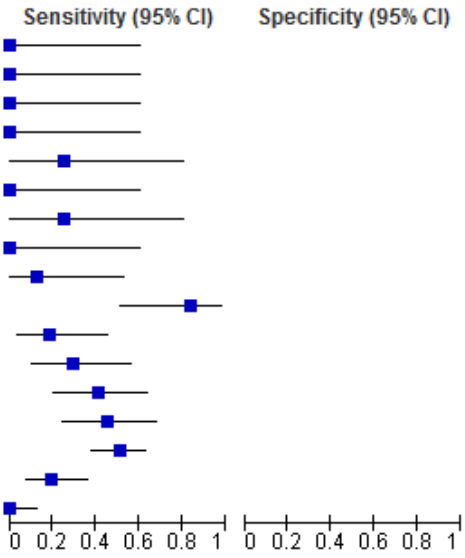

Test 15. IgG/IgM (8 to 14 days)

IgG/IgM (8 to 14 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	11	0	2	0	0.85 [0.55, 0.98]	Not estimable
Adams 2020 [D]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [E]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [F]	9	0	4	0	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [G]	8	0	5	0	0.62 [0.32, 0.86]	Not estimable
Adams 2020 [H]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [I]	10	0	3	0	0.77 [0.46, 0.95]	Not estimable
Adams 2020 [J]	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Garcia 2020 (A)	8	0	16	0	0.33 [0.16, 0.55]	Not estimable
Garcia 2020 (B)	15	0	3	0	0.83 [0.59, 0.96]	Not estimable
Lassauniere 2020 [D]	5	0	2	0	0.71 [0.29, 0.96]	Not estimable
Lassauniere 2020 [E]	5	0	2	0	0.71 [0.29, 0.96]	Not estimable
Lassauniere 2020 [F]	6	0	1	0	0.86 [0.42, 1.00]	Not estimable
Lassauniere 2020 [G]	5	0	2	0	0.71 [0.29, 0.96]	Not estimable
Lin 2020a [A]	29	0	4	0	0.88 [0.72, 0.97]	Not estimable
Liu 2020a	6	0	0	0	1.00 [0.54, 1.00]	Not estimable
Liu 2020b	82	0	28	0	0.75 [0.65, 0.82]	Not estimable
Liu 2020d [A]	68	0	24	0	0.74 [0.64, 0.83]	Not estimable
Liu 2020d [B]	72	0	20	0	0.78 [0.68, 0.86]	Not estimable
Long 2020 (B)	34	0	33	0	0.51 [0.38, 0.63]	Not estimable
Pan 2020a	31	0	3	0	0.91 [0.76, 0.98]	Not estimable

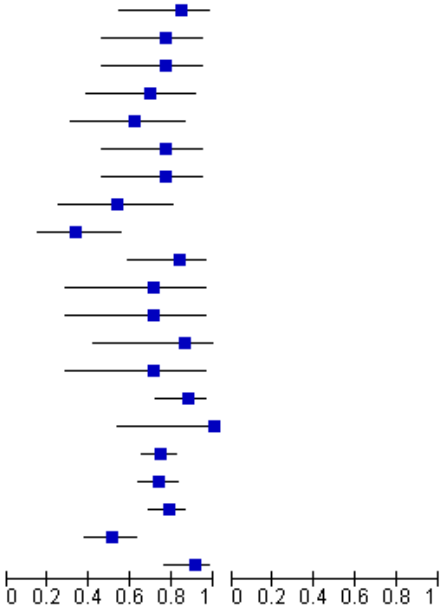


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 16. IgG/IgM (15 to 21 days)

IgG/IgM (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [D]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [E]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [F]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [G]	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [H]	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Adams 2020 [I]	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Adams 2020 [J]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Garcia 2020 (A)	17	0	6	0	0.74 [0.52, 0.90]	Not estimable
Garcia 2020 (B)	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Lassauniere 2020 [D]	14	0	1	0	0.93 [0.68, 1.00]	Not estimable
Lassauniere 2020 [E]	14	0	1	0	0.93 [0.68, 1.00]	Not estimable
Lassauniere 2020 [F]	14	0	1	0	0.93 [0.68, 1.00]	Not estimable
Lassauniere 2020 [G]	12	0	3	0	0.80 [0.52, 0.96]	Not estimable
Lin 2020a [A]	33	0	1	0	0.97 [0.85, 1.00]	Not estimable
Liu 2020a	68	0	0	0	1.00 [0.95, 1.00]	Not estimable
Liu 2020b	107	0	4	0	0.96 [0.91, 0.99]	Not estimable
Liu 2020d [A]	52	0	3	0	0.95 [0.85, 0.99]	Not estimable
Liu 2020d [B]	72	0	20	0	0.78 [0.68, 0.86]	Not estimable
Long 2020 (B)	131	0	3	0	0.98 [0.94, 1.00]	Not estimable
Pan 2020a	35	0	3	0	0.92 [0.79, 0.98]	Not estimable

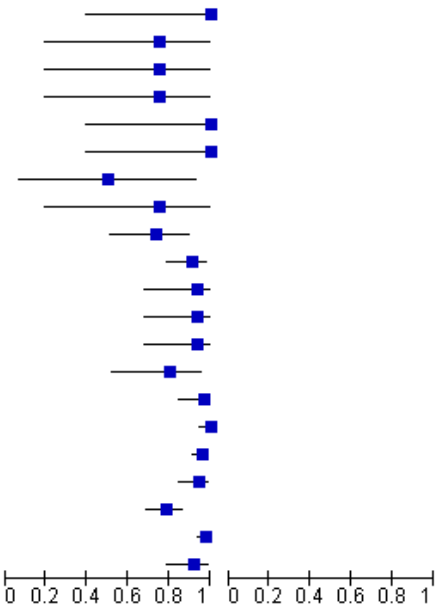

Test 17. IgG/IgM (22 to 35 days)

IgG/IgM (22 to 35 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Adams 2020 [D]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [E]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [F]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [G]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [H]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [I]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [J]	2	0	0	0	1.00 [0.16, 1.00]	Not estimable
Du 2020	7	0	0	0	1.00 [0.59, 1.00]	Not estimable
Lassauniere 2020 [D]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [E]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [F]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Lassauniere 2020 [G]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Liu 2020d [A]	43	0	2	0	0.96 [0.85, 0.99]	Not estimable
Liu 2020d [B]	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Long 2020 (B)	13	0	0	0	1.00 [0.75, 1.00]	Not estimable

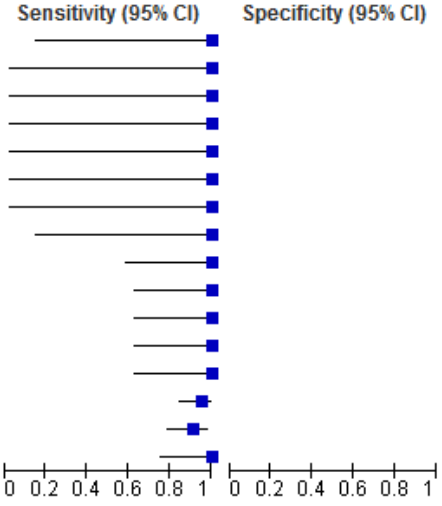


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 18. IgG/IgM (over 35 days)

IgG/IgM (over 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	17	0	0	0	1.00 [0.80, 1.00]	Not estimable
Adams 2020 [D]	7	0	4	0	0.64 [0.31, 0.89]	Not estimable
Adams 2020 [E]	11	0	5	0	0.69 [0.41, 0.89]	Not estimable
Adams 2020 [F]	6	0	3	0	0.67 [0.30, 0.93]	Not estimable
Adams 2020 [G]	6	0	3	0	0.67 [0.30, 0.93]	Not estimable
Adams 2020 [H]	8	0	3	0	0.73 [0.39, 0.94]	Not estimable
Adams 2020 [I]	4	0	6	0	0.40 [0.12, 0.74]	Not estimable
Adams 2020 [J]	10	0	7	0	0.59 [0.33, 0.82]	Not estimable
Du 2020	53	0	0	0	1.00 [0.93, 1.00]	Not estimable

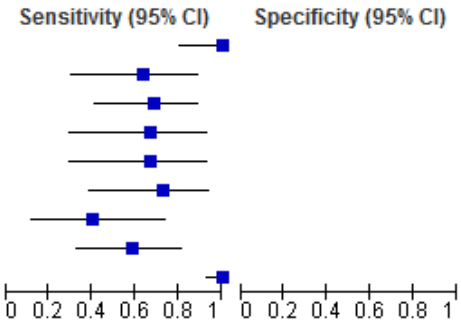

Test 19. IgA (all time points)

IgA (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Guo 2020a	194	0	14	135	0.93 [0.89, 0.96]	1.00 [0.97, 1.00]
Lassauniere 2020 [C]	28	6	2	76	0.93 [0.78, 0.99]	0.93 [0.85, 0.97]
Lippi 2020 [B]	10	0	38	0	0.21 [0.10, 0.35]	Not estimable
Ma 2020a	213	9	3	474	0.99 [0.96, 1.00]	0.98 [0.96, 0.99]
Okba 2020a	11	1	20	44	0.35 [0.19, 0.55]	0.98 [0.88, 1.00]

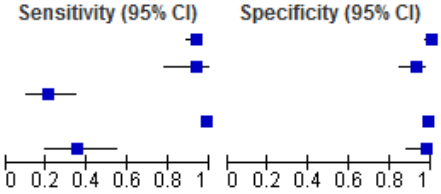

Test 20. IgA (1 to 7 days)

IgA (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Guo 2020a	38	0	3	0	0.93 [0.80, 0.98]	Not estimable
Lippi 2020 [B]	1	0	29	0	0.03 [0.00, 0.17]	Not estimable
Ma 2020a	15	0	2	0	0.88 [0.64, 0.99]	Not estimable
Okba 2020a	0	0	12	0	0.00 [0.00, 0.26]	Not estimable

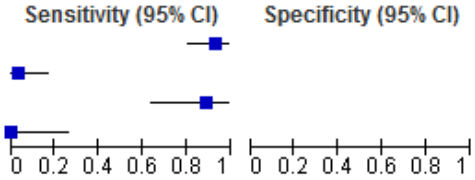

Test 21. IgA (8 to 14 days)

IgA (8 to 14 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [C]	3	0	4	0	0.43 [0.10, 0.82]	Not estimable
Lippi 2020 [B]	9	0	9	0	0.50 [0.26, 0.74]	Not estimable
Ma 2020a	30	0	0	0	1.00 [0.88, 1.00]	Not estimable
Okba 2020a	4	0	6	0	0.40 [0.12, 0.74]	Not estimable

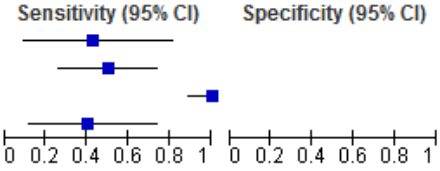


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 22. IgA (15 to 21 days)

IgA (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [C]	10	0	5	0	0.67 [0.38, 0.88]	Not estimable
Ma 2020a	55	0	0	0	1.00 [0.94, 1.00]	Not estimable
Okba 2020a	6	0	2	0	0.75 [0.35, 0.97]	Not estimable

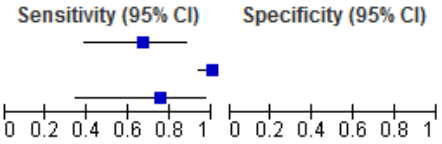

Test 23. IgA (22 to 35 days)

IgA (22 to 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Lassauniere 2020 [C]	7	0	1	0	0.88 [0.47, 1.00]	Not estimable
Ma 2020a	80	0	1	0	0.99 [0.93, 1.00]	Not estimable
Okba 2020a	1	0	0	0	1.00 [0.03, 1.00]	Not estimable

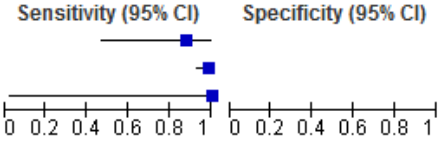

Test 24. IgA (over 35 days)

IgA (over 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Ma 2020a	23	0	0	0	1.00 [0.85, 1.00]	Not estimable



Test 25. Total antibodies (Ab) (all time points)

Total antibodies (Ab) (all time points)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	18	0	15	60	0.55 [0.36, 0.72]	1.00 [0.94, 1.00]
Adams 2020 [C]	23	1	15	90	0.61 [0.43, 0.76]	0.99 [0.94, 1.00]
Burbelo 2020 [A]	76	0	32	32	0.70 [0.61, 0.79]	1.00 [0.89, 1.00]
Burbelo 2020 [B]	60	0	40	32	0.60 [0.50, 0.70]	1.00 [0.89, 1.00]
Freeman 2020	95	4	4	515	0.96 [0.90, 0.99]	0.99 [0.98, 1.00]
Grzelak 2020 [A]	65	0	96	280	0.40 [0.33, 0.48]	1.00 [0.99, 1.00]
Grzelak 2020 [B]	130	3	31	277	0.81 [0.74, 0.87]	0.99 [0.97, 1.00]
Grzelak 2020 [E]	132	5	27	95	0.83 [0.76, 0.89]	0.95 [0.89, 0.98]
Lassauniere 2020 [A]	28	0	2	82	0.93 [0.78, 0.99]	1.00 [0.96, 1.00]
Lou 2020 [A]	78	0	2	300	0.97 [0.91, 1.00]	1.00 [0.99, 1.00]
Lou 2020 [B]	78	10	2	199	0.97 [0.91, 1.00]	0.95 [0.91, 0.98]
Lou 2020 [C]	77	2	3	298	0.96 [0.89, 0.99]	0.99 [0.98, 1.00]
Ma 2020a	215	0	1	4	1.00 [0.97, 1.00]	1.00 [0.40, 1.00]
Wan 2020 [B]	7	0	6	0	0.54 [0.25, 0.81]	Not estimable
Zhang 2020d	127	4	27	667	0.82 [0.76, 0.88]	0.99 [0.98, 1.00]
Zhao 2020a	161	2	12	211	0.93 [0.88, 0.96]	0.99 [0.97, 1.00]
Zhao 2020b	67	10	2	402	0.97 [0.90, 1.00]	0.98 [0.96, 0.99]

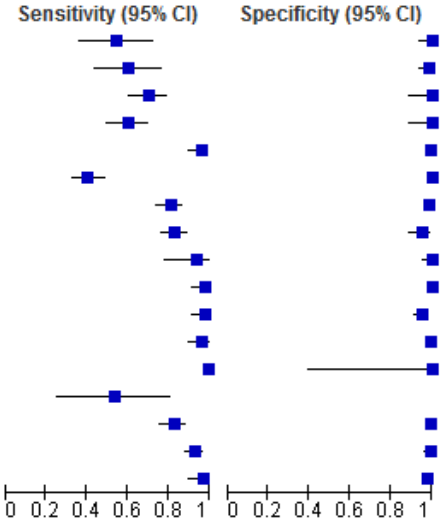


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 27. Total antibodies (Ab) (1 to 7 days)

Total antibodies (Ab) (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	0	0	4	0	0.00 [0.00, 0.60]	Not estimable
Adams 2020 [C]	0	0	3	0	0.00 [0.00, 0.71]	Not estimable
Lou 2020 [A]	25	0	14	0	0.64 [0.47, 0.79]	Not estimable
Wan 2020 [B]	1	0	3	0	0.25 [0.01, 0.81]	Not estimable
Zhao 2020a	36	0	58	0	0.38 [0.28, 0.49]	Not estimable

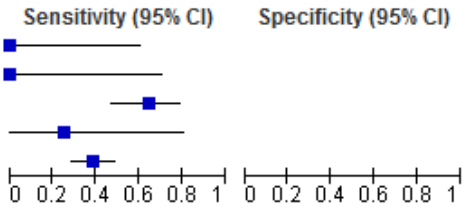

Test 29. Total antibodies (Ab) (8 to 14 days)

Total antibodies (Ab) (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	9	0	4	0	0.69 [0.39, 0.91]	Not estimable
Adams 2020 [C]	8	0	4	0	0.67 [0.35, 0.90]	Not estimable
Lassauniere 2020 [A]	5	0	2	0	0.71 [0.29, 0.96]	Not estimable
Lou 2020 [A]	74	0	1	0	0.99 [0.93, 1.00]	Not estimable
Wan 2020 [B]	3	0	2	0	0.60 [0.15, 0.95]	Not estimable
Zhao 2020a	121	0	14	0	0.90 [0.83, 0.94]	Not estimable

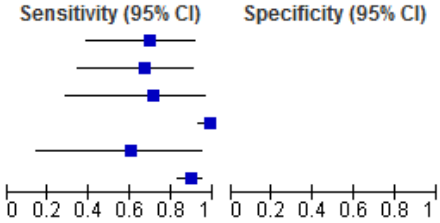

Test 30. Total antibodies (Ab) (15 to 21 days)

Total antibodies (Ab) (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Adams 2020 [C]	3	0	1	0	0.75 [0.19, 0.99]	Not estimable
Lassauniere 2020 [A]	15	0	0	0	1.00 [0.78, 1.00]	Not estimable
Lou 2020 [A]	60	0	0	0	1.00 [0.94, 1.00]	Not estimable
Wan 2020 [B]	3	0	0	0	1.00 [0.29, 1.00]	Not estimable
Zhao 2020a	90	0	0	0	1.00 [0.96, 1.00]	Not estimable

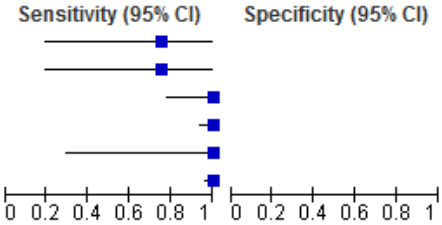

Test 31. Total antibodies (Ab) (21 to 35 days)

Total antibodies (Ab) (21 to 35 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	1	0	0	0	1.00 [0.03, 1.00]	Not estimable
Adams 2020 [C]	2	0	7	0	0.22 [0.03, 0.60]	Not estimable
Lassauniere 2020 [A]	8	0	0	0	1.00 [0.63, 1.00]	Not estimable
Wan 2020 [B]	0	0	1	0	0.00 [0.00, 0.97]	Not estimable

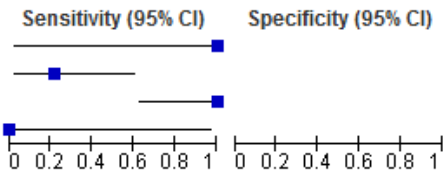


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 32. Total antibodies (Ab) (over 35 days)

Total antibodies (Ab) (over 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [B]	5	0	6	0	0.45 [0.17, 0.77]	Not estimable		
Adams 2020 [C]	10	0	7	0	0.59 [0.33, 0.82]	Not estimable		

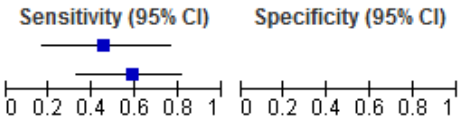

Test 33. IgA/IgG (all time points)

IgA/IgG (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Ma 2020a	214	0	2	483	0.99 [0.97, 1.00]	1.00 [0.99, 1.00]		
Okba 2020a	13	1	18	44	0.42 [0.25, 0.61]	0.98 [0.88, 1.00]		



Test 34. IgA/IgG (1 to 7 days)

IgA/IgG (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Okba 2020a	0	0	12	0	0.00 [0.00, 0.26]	Not estimable		



Test 35. IgA/IgG (8 to 14 days)

IgA/IgG (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Okba 2020a	5	0	5	0	0.50 [0.19, 0.81]	Not estimable		



Test 36. IgA/IgG (15 to 21 days)

IgA/IgG (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Okba 2020a	7	0	1	0	0.88 [0.47, 1.00]	Not estimable		




Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 37. IgA/IgG (22 to 35 days)

IgA/IgG (22 to 35 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Okba 2020a	1	0	0	0	1.00 [0.03, 1.00]	Not estimable



Test 38. IgA/IgM (all time points)

IgA/IgM (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Ma 2020a	215	1	1	482	1.00 [0.97, 1.00]	1.00 [0.99, 1.00]



Test 39. IgG in PCR+ve (all time points)

IgG in PCR+ve (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	14	0	1	0	0.93 [0.68, 1.00]	Not estimable
Jia 2020	16	0	8	0	0.67 [0.45, 0.84]	Not estimable
Qian 2020	486	0	17	0	0.97 [0.95, 0.98]	Not estimable
Xie 2020a	16	0	0	0	1.00 [0.79, 1.00]	Not estimable

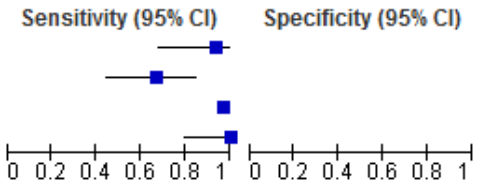

Test 40. IgG in PCR +ve (1 to 7 days)

IgG in PCR +ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	0	0	1	0	0.00 [0.00, 0.97]	Not estimable
Pan 2020a	1	0	26	0	0.04 [0.00, 0.19]	Not estimable

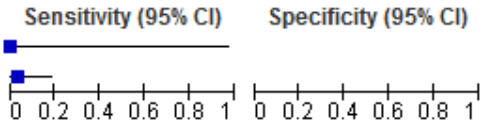

Test 41. IgG in PCR+ve (8 to 14 days)

IgG in PCR+ve (8 to 14 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	5	0	0	0	1.00 [0.48, 1.00]	Not estimable
Pan 2020a	16	0	12	0	0.57 [0.37, 0.76]	Not estimable

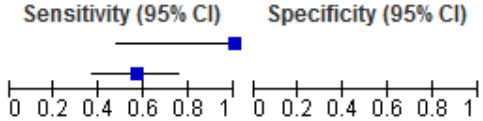


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 42. IgG in PCR+ve (15 to 21 days)

IgG in PCR+ve (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	9	0	0	0	1.00 [0.66, 1.00]	Not estimable
Pan 2020a	30	0	1	0	0.97 [0.83, 1.00]	Not estimable

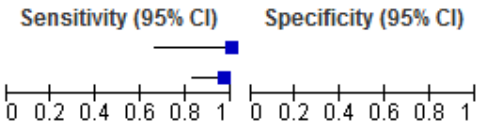

Test 43. IgG in PCR-ve (all time points)

IgG in PCR-ve (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	28	0	2	0	0.93 [0.78, 0.99]	Not estimable
Garcia 2020 (B)	56	0	7	0	0.89 [0.78, 0.95]	Not estimable
Jia 2020	15	0	18	0	0.45 [0.28, 0.64]	Not estimable
Jin 2020	32	0	2	0	0.94 [0.80, 0.99]	Not estimable
Qian 2020	45	0	7	0	0.87 [0.74, 0.94]	Not estimable
Xie 2020a	40	0	0	0	1.00 [0.91, 1.00]	Not estimable

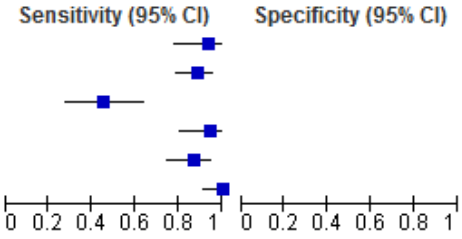

Test 44. IgG in PCR-ve (1 to 7 days)

IgG in PCR-ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	4	0	0	0	1.00 [0.40, 1.00]	Not estimable
Pan 2020a	4	0	5	0	0.44 [0.14, 0.79]	Not estimable

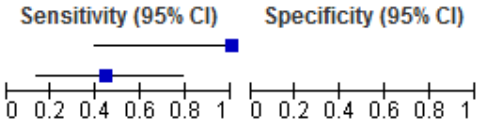

Test 45. IgG in PCR-ve (8 to 14 days)

IgG in PCR-ve (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	6	0	0	0	1.00 [0.54, 1.00]	Not estimable
Garcia 2020 (B)	15	0	3	0	0.83 [0.59, 0.96]	Not estimable
Pan 2020a	4	0	2	0	0.67 [0.22, 0.96]	Not estimable

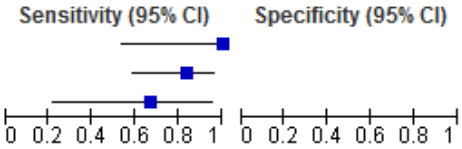

Test 46. IgG in PCR-ve (15 to 21 days)

IgG in PCR-ve (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	18	0	2	0	0.90 [0.68, 0.99]	Not estimable
Garcia 2020 (B)	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Pan 2020a	5	0	2	0	0.71 [0.29, 0.96]	Not estimable

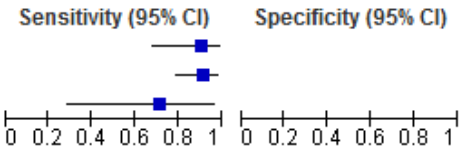


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 47. IgM in PCR+ve (all time points)

IgM in PCR+ve (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	7	0	8	0	0.47 [0.21, 0.73]	Not estimable
Guo 2020a	62	0	20	0	0.76 [0.65, 0.84]	Not estimable
Jia 2020	19	0	5	0	0.79 [0.58, 0.93]	Not estimable
Liu 2020c	74	0	17	0	0.81 [0.72, 0.89]	Not estimable
Qian 2020	432	0	71	0	0.86 [0.83, 0.89]	Not estimable
Xie 2020a	15	0	10	0	0.60 [0.39, 0.79]	Not estimable

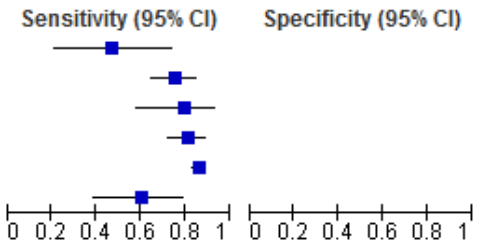

Test 48. IgM in PCR+ve (1 to 7 days)

IgM in PCR+ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	0	0	1	0	0.00 [0.00, 0.97]	Not estimable
Pan 2020a	3	0	24	0	0.11 [0.02, 0.29]	Not estimable



Test 49. IgM in PCR+ve (8 to 14 days)

IgM in PCR+ve (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	3	0	2	0	0.60 [0.15, 0.95]	Not estimable
Pan 2020a	22	0	6	0	0.79 [0.59, 0.92]	Not estimable

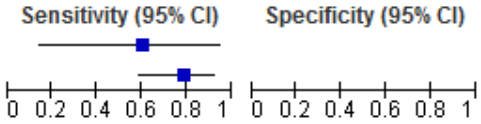

Test 50. IgM in PCR+ve (15 to 21 days)

IgM in PCR+ve (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	4	0	5	0	0.44 [0.14, 0.79]	Not estimable
Pan 2020a	4	0	3	0	0.57 [0.18, 0.90]	Not estimable

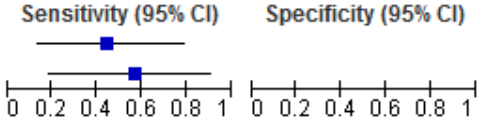


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 51. IgM in PCR-ve (all time points)

IgM in PCR-ve (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	13	0	17	0	0.43 [0.25, 0.63]	Not estimable
Garcia 2020 (B)	25	0	38	0	0.40 [0.28, 0.53]	Not estimable
Guo 2020a	54	0	4	0	0.93 [0.83, 0.98]	Not estimable
Jia 2020	20	0	13	0	0.61 [0.42, 0.77]	Not estimable
Jin 2020	19	0	15	0	0.56 [0.38, 0.73]	Not estimable
Liu 2020c	31	0	11	0	0.74 [0.58, 0.86]	Not estimable
Qian 2020	38	0	14	0	0.73 [0.59, 0.84]	Not estimable
Xie 2020a	34	0	6	0	0.85 [0.70, 0.94]	Not estimable

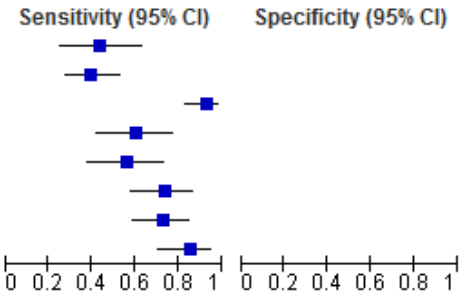

Test 52. IgM in PCR-ve (1 to 7 days)

IgM in PCR-ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	2	0	2	0	0.50 [0.07, 0.93]	Not estimable
Pan 2020a	2	0	7	0	0.22 [0.03, 0.60]	Not estimable

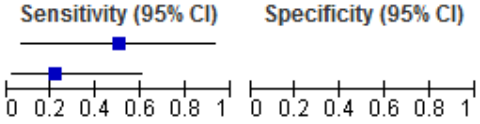

Test 53. IgM in PCR-ve (8 to 14 days)

IgM in PCR-ve (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	2	0	4	0	0.33 [0.04, 0.78]	Not estimable
Garcia 2020 (B)	7	0	11	0	0.39 [0.17, 0.64]	Not estimable
Pan 2020a	2	0	4	0	0.33 [0.04, 0.78]	Not estimable

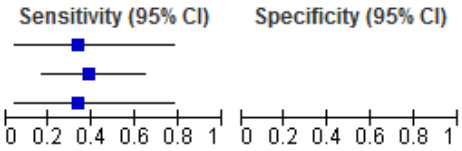

Test 54. IgM in PCR-ve (15 to 21 days)

IgM in PCR-ve (15 to 21 days)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	9	0	11	0	0.45 [0.23, 0.68]	Not estimable
Garcia 2020 (B)	18	0	27	0	0.40 [0.26, 0.56]	Not estimable
Pan 2020a	4	0	3	0	0.57 [0.18, 0.90]	Not estimable

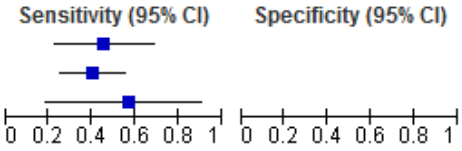


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 55. IgG/IgM in PCR+ve (all time points)

IgG/IgM in PCR+ve (all time points)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Jia 2020	21	0	3	0	0.88 [0.68, 0.97]	Not estimable
Liu 2020b	127	0	26	0	0.83 [0.76, 0.89]	Not estimable

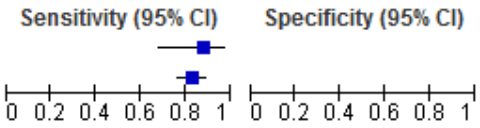

Test 56. IgG/IgM in PCR+ve (1 to 7 days)

IgG/IgM in PCR+ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	5	0	4	0	0.56 [0.21, 0.86]	Not estimable
Pan 2020a	3	0	24	0	0.11 [0.02, 0.29]	Not estimable

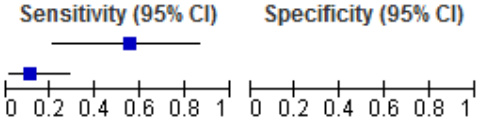

Test 57. IgG/IgM in PCR+ve (8 to 14 days)

IgG/IgM in PCR+ve (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	11	0	14	0	0.44 [0.24, 0.65]	Not estimable
Pan 2020a	26	0	2	0	0.93 [0.76, 0.99]	Not estimable

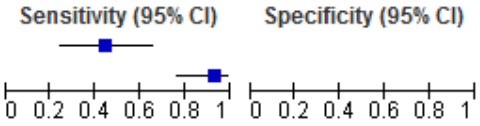

Test 58. IgG/IgM in PCR+ve (15 to 21 days)

IgG/IgM in PCR+ve (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	111	0	8	0	0.93 [0.87, 0.97]	Not estimable
Pan 2020a	30	0	1	0	0.97 [0.83, 1.00]	Not estimable

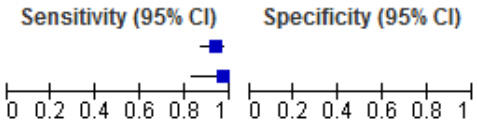

Test 59. IgG/IgM in PCR-ve (all time points)

IgG/IgM in PCR-ve (all time points)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	56	0	7	0	0.89 [0.78, 0.95]	Not estimable
Jia 2020	24	0	9	0	0.73 [0.54, 0.87]	Not estimable
Jin 2020	32	0	2	0	0.94 [0.80, 0.99]	Not estimable
Liu 2020b	67	0	18	0	0.79 [0.69, 0.87]	Not estimable

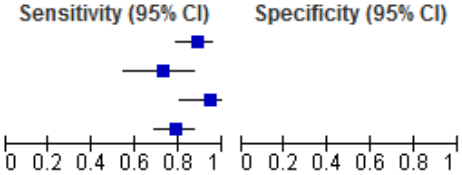


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 60. IgG/IgM in PCR-ve (1 to 7 days)

IgG/IgM in PCR-ve (1 to 7 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020b	0	0	8	0	0.00 [0.00, 0.37]	Not estimable
Pan 2020a	4	0	5	0	0.44 [0.14, 0.79]	Not estimable

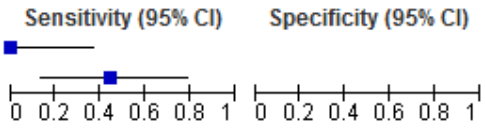

Test 61. IgG/IgM in PCR-ve (8 to 14 days)

IgG/IgM in PCR-ve (8 to 14 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	15	0	3	0	0.83 [0.59, 0.96]	Not estimable
Liu 2020b	9	0	7	0	0.56 [0.30, 0.80]	Not estimable
Pan 2020a	5	0	1	0	0.83 [0.36, 1.00]	Not estimable

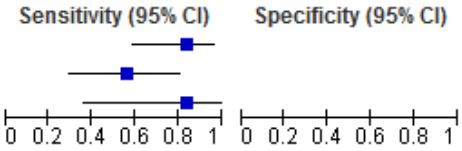

Test 62. IgG/IgM in PCR-ve (15 to 21 days)

IgG/IgM in PCR-ve (15 to 21 days)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Garcia 2020 (B)	41	0	4	0	0.91 [0.79, 0.98]	Not estimable
Liu 2020b	58	0	3	0	0.95 [0.86, 0.99]	Not estimable
Pan 2020a	5	0	2	0	0.71 [0.29, 0.96]	Not estimable

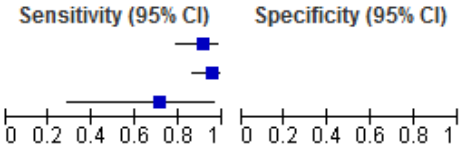

Test 63. IgG (moderate)

IgG (moderate)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	41	0	3	0	0.93 [0.81, 0.99]	Not estimable



Test 64. IgG (severe)

IgG (severe)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	52	0	0	0	1.00 [0.93, 1.00]	Not estimable




Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 65. IgG (critical)

IgG (critical)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	36	0	1	0	0.97 [0.86, 1.00]	Not estimable		



Test 66. IgM (moderate)

IgM (moderate)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	35	0	9	0	0.80 [0.65, 0.90]	Not estimable		



Test 67. IgM (severe)

IgM (severe)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	43	0	9	0	0.83 [0.70, 0.92]	Not estimable		



Test 68. IgM (critical)

IgM (critical)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Liu 2020c	27	0	10	0	0.73 [0.56, 0.86]	Not estimable		



Test 69. RT-PCR (all time points - throat)

RT-PCR (all time points - throat)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	14	0	24	0	0.37 [0.22, 0.54]	Not estimable		
Liu 2020b	153	0	85	0	0.64 [0.58, 0.70]	Not estimable		




Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 70. RT-PCR (1 to 7 days throat)

RT-PCR (1 to 7 days throat)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	9	0	4	0	0.69 [0.39, 0.91]	Not estimable
Liu 2020b	41	0	13	0	0.76 [0.62, 0.87]	Not estimable

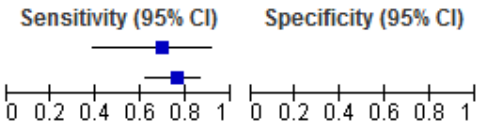

Test 71. RT-PCR (8 to 14 days - throat)

RT-PCR (8 to 14 days - throat)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	2	0	6	0	0.25 [0.03, 0.65]	Not estimable
Liu 2020b	92	0	42	0	0.69 [0.60, 0.76]	Not estimable

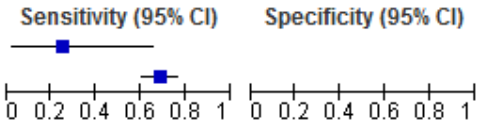

Test 72. RT-PCR (15 to 21 days - throat)

RT-PCR (15 to 21 days - throat)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	3	0	20	0	0.13 [0.03, 0.34]	Not estimable
Liu 2020b	20	0	30	0	0.40 [0.26, 0.55]	Not estimable

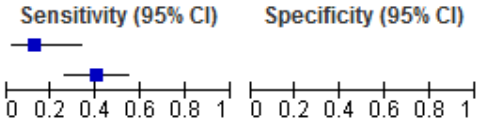

Test 73. RT-PCR (all time points - sputum)

RT-PCR (all time points - sputum)


Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	29	0	24	0	0.55 [0.40, 0.68]	Not estimable



Test 74. RT-PCR (1 to 7 days - sputum)

RT-PCR (1 to 7 days - sputum)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	12	0	1	0	0.92 [0.64, 1.00]	Not estimable



Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Test 75. RT-PCR (8 to 14 days - sputum)

RT-PCR (8 to 14 days - sputum)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	3	0	5	0	0.38 [0.09, 0.76]	Not estimable	0 0.2 0.4 0.6 0.8 1	0 0.2 0.4 0.6 0.8 1

Test 76. RT-PCR (15 to 21 days - sputum)

RT-PCR (15 to 21 days - sputum)

Study	TP	FP	FN	TN	Sensitivity (95% CI)	Specificity (95% CI)	Sensitivity (95% CI)	Specificity (95% CI)
Gao 2020a	14	0	9	0	0.61 [0.39, 0.80]	Not estimable	0 0.2 0.4 0.6 0.8 1	0 0.2 0.4 0.6 0.8 1

ADDITIONAL TABLES

Table 1. Description of studies

Participants		**Studies (percentage) (n=54 studies)**
Sample size	Median (IQR) 129.5 (57 to 347)	Min 10, max 3481
Number of COVID-19 cases	Median (IQR) 62 (31 to 151)	Min 3, max 555
Setting	Hospital inpatient	44 (81%)
	Hospital outpatient	1 (2%)
	Hospital accident and emergency	2 (4%)
	Community	2 (4%)
	Mixed or unclear	5 (9%)
Patient group	Asymptomatic	0 (0%)
	Asymptomatic and acute	1 (2%)
	Acute	23 (43%)
	Acute and convalescent	22 (41%)
	Convalescent	2 (4%)
	Mixed or unclear	6 (11%)
Study design		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 1. Description of studies *(Continued)*

Recruitment structure	Single group, both COVID-19 and non-COVID-19 cases	6 (11%)
	Single group, only COVID-19 cases	19 (35%)
	Two or more groups with COVID-19 and non-COVID-19 cases	29 (54%)
Reference standard for COVID-19 cases	All RT-PCR-positive	32 (59%)
	China CDC criteria including RT-PCR-negative patients	11 (20%)
	WHO criteria including RT-PCR-negative patients	1 (2%)
	Other criteria including RT-PCR-negative patients	3 (6%)
	Other	2 (4%)
	Mixed or unclear	5 (9%)
Reference standard for non-COVID-19	Pre-pandemic healthy	4 (7%)
	Pre-pandemic other disease	3 (6%)
	Pre-pandemic healthy + other disease	4 (7%)
	Current healthy (untested)	5 (9%)
	Current other disease (untested)	1 (2%)
	Current healthy + other disease (untested)	2 (4%)
	Current healthy + other disease (RT-PCR-negative)	2 (4%)
	COVID suspects, single RT-PCR-negative	8 (15%)
	COVID suspects, two or more RT-PCR–negative results	3 (6%)
	Mixed/other	3 (6%)
Tests		
Number of tests per study	1	40 (74%)
	2	8 (15%)
	3-5	4 (8%)
	6-10	2 (2%)
Test technology (n = 89)	CGIA	23 (26%)
	CLIA	20 (22%)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 1. Description of studies *(Continued)*

	ELISA	28 (31%)
	FIA	2 (2%)
	IIFT	1 (1%)
	LFA (no details)	10 (11%)
	LIPS	4 (4%)
	S-flow	1 (1%)
Test brand (n = 89)	Withheld	13 (%)
	Acro Biotech - IgG/IgM	1 (1%)
	Artron Laboratories IgM/IgG	1 (1%)
	Autobio Diagnostics IgM/IgG	1 (1%)
	Beijing Beier Bioengineering CGIA	1 (1%)
	Beijing Beier Bioengineering CLIA	1 (1%)
	Beijing Beier Bioengineering ELISA	1 (1%)
	Beijing Diagreat	1 (1%)
	Beijing Hotgen CGIA	1 (1%)
	Beijing Hotgen ELISA	2 (3%)
	Beijing Wantai CGIA	1 (1%)
	Beijing Wantai ELISA	3 (3%)
	Bioscience Co (Chongqing)	3 (3%)
	CTK Biotech OnSite IgG/IgM	1 (1%)
	Darui Biotech	1 (1%)
	Dynamiker Biotechnology IgG/IgM	1 (1%)
	EUROIMMUN	3 (3%)
	EUROIMMUN Anti-SARS-Cov	1 (1%)
	EUROIMMUN Beta	1 (1%)
	Hangzhou Alltest - IgG/IgM	3 (3%)
	Innovita Biological - Ab test (IgM/IgG)	2 (3%)
	Jiangsu Medomics IgG-IgM	1 (1%)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 1. Description of studies *(Continued)*

	Shenzhen YHLO	7 (8%)
	Snibe Diagnostic - MAGLUMI	2 (3%)
	Vivachek - VivaDiag IgM/IgG	3 (3%)
	Xiamen InnodDx Biotech	1 (1%)
	Zhuhai Livzon CGIA	2 (3%)
	Zhuhai Livzon ELISA	5 (6%)
	In-house, S-based ELISA	1 (1%)
	In-house, S-based LIPS	1 (1%)
	In-house, rN-based ELISA	1 (1%)
	In-house, rS-based ELISA	1 (1%)
	In-house CGIA	2 (2%)
	In-house CLIA	5 (6%)
	In-house ELISA	6 (7%)
	In-house FIA	1 (1%)
	In-house S-flow	1 (1%)
	In-house - N-based ELISA	1 (1%)
	In-house - N-based LIPS	2 (2%)
	In-house - S1-based LIPS	1 (1%)
	In-house - tri-S-based ELISA	1 (1%)
	In-house Anti-SARS-Cov ELISA	1 (1%)

Ab: antibody; **CDC:** Center for Disease Control and Prevention; **CGIA:** colloidal gold immunoassay; **CLIA:** chemiluminescence immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **FIA:** fluorescence immunoassay; **IQR:** interquartile range; **IIFT:** indirect immunofluorescence assay; **LFA:** lateral flow assay; **LIPS:** luciferase immunoprecipitation system; **max:** maximum; **min:** minimum; **N-based:** nucleocapsid protein; **RT-PCR:** reverse transcription polymerase chain reaction; **S-based:** spike protein; **S-flow:** flow-cytometry assay; **WHO:** World Health Organization

Table 2. Test sensitivity by time since onset of symptoms

	Days 1-7	Days 8-14	Days 15-21	Days 22-35	Days > 35	Comparison
Test groups [studies] (true positives/COVID cases)						

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 2. Test sensitivity by time since onset of symptoms *(Continued)*

	Sensitivity (95% CI)					
IgG	33 [23] (165/568)	34 [22] (766/1200)	34 [22] (974/1110)	20 [12] (417/502)	11 [4] (213/252)	
	29.7% (22.1 to 38.6)	66.5% (57.9 to 74.2)	88.2% (83.5 to 91.8)	80.3% (72.4 to 86.4)	86.7% (79.6 to 91.7)	P < 0.00005
IgM	34 [24] (207/608)	32 [21] (724/1171)	32 [21] (800/1074)	19 [11] (378/507)	11 [4] 118/215	
	23.2% (14.9 to 34.2)	58.4% (45.5 to 70.3)	75.4% (64.3 to 83.8)	68.1% (55.0 to 78.9)	53.9% (38.4 to 68.6)	P < 0.00005
IgA	4 [4] (54/100)	3 [3] (38/53)	3 [3] (66/68)	2 [2] (81/82)	1 [1] (23/23)	
	28.4% (0.9 to 94.3)	78.1% (9.5 to 99.2)	98.7% (39.0 to 100)	98.7% (91.9 to 99.8)	100% (85.2 to 100)	*
Total antibodies	5 [4] (62/144)	6 [5] (220/247)	6 [5] (174/176)	4 [3] (11/19)	2 [1] (15/28)	
	24.5% (9.5 to 50.0)	84.0% (64.1 to 93.9)	98.1% (90.1 to 99.6)	69.5% (34.8 to 90.7)	79.0% (49.8 to 93.4)	P < 0.00005
IgG/IgM	17 [9] (81/259)	21 [9] (441/608)	21 [9] (636/692)	16 [5] (146/152)	9 [2] (122/153)	
	30.1% (21.4 to 40.7)	72.2% (63.5 to 79.5)	91.4% (87.0 to 94.4)	96.0% (90.6 to 98.3)	77.7% (66.0 to 86.2)	P < 0.00005
IgA/IgG	1 [1] (0/12)	1 [1] (5/10)	1 [1] (7/8)	1 [1] (1/1)	0 [0]	
	0% (0 to 26.5)	50.0% (18.7 to 81.3)	87.5% (47.3 to 99.6)	100% (2.5 to 100)		*
IgA/IgM	0 [0]	0 [0]	0 [0]	0 [0]	0 [0]	

CI: confidence interval; * inadequate data to make a formal statistical comparison

Table 3. Specificity and impact of reference standard for non-COVID cases

	Overall specificity[a]	COVID suspects deemed negative	Current healthy or other disease	Pre-pandemic	Comparison of control groups
	Test groups [studies] (false positives/non-COVID cases) Specificity (95% CI)				
IgG	62 [44] (159/6136)	6 [6] (10/396)	14 [10] (60/2614)	19 [10] (88/2633)	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 3. Specificity and impact of reference standard for non-COVID cases *(Continued)*

	99.1% (98.3% to 99.6%)	98.0% (91.0% to 99.6%)	99.2% (97.6% to 99.8%)	99.2% (97.8% to 99.7%)	P = 0.56
IgM	59 [41] (183/6103)	5 [5] (12/384)	14 [10] (89/3069)	17 [9] (38/2075)	
	98.7% (97.4% to 99.3%)	98.1% (89.9% to 99.7%)	98.6% (96.0% to 99.5%)	99.3% (98.0% to 99.8%)	P = 0.50
IgG/IgM	34 [23] (78/5761)	7 [7] (33/454)	7 [5] (20/506)	18 [6] (22/1104)	No formal comparison possible
	98.7% (97.2% to 99.4%)	92.8% (89.7% to 95.0%)	99.9% (65.2% to 100%)	98.7% (96.6% to 99.5%)	
Total antibodies	16 [10] (41/3585)				
	99.2% (98.3% to 99.6%)				
IgA	4 [4] (10/663)				
	98.5% (97.2% to 99.2%)				
IgA/IgG [b]	2 [2] (1/528)				
	99.8% (98.9% to 100%)				
IgA/IgM [b]	1 [1] (1/483)				
	99.8% (99.2% to 100%)				

CI: confidence interval

[a]Includes studies that are categorised as mixed/other not included in the subgroups.
[b]Confidence intervals computed using binomial exact on totals.

Table 4. Reported cross-reactivity with SARS-CoV-2 antigens

Study	Test(s) evaluated	What the study says about cross-reactivity
Cai 2020	In-house CLIA	Reported no cross-reactivity in 167 sera from patients with infection with other pathogens (influenza A virus (25), respiratory syncytial virus (7), parainfluenza virus (8), influenza B virus (5), adenovirus (6), *Klebsiella pneumoniae* (8), *Streptococcus pneumoniae* (3), mycoplasma (5), *Acinetobacter baumannii* (10), *Candida albicans* (2), *Staphylococcus aureus* (3), *Mycobacterium tuberculosis* (4), hepatitis B virus (33), hepatitis C virus (22), syphilis (23) and saccharomycopsis (3)).
Freeman 2020	In-house ELISA	Reported cross-reactivity to SARS-CoV-2 spike protein in sera from patients with SARS-1 and MERS-CoV, and no cross-reactivity with NL63, OC43, HKU1, 229E

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 4. Reported cross-reactivity with SARS-CoV-2 antigens *(Continued)*

Guo 2020a	In-house ELISA	Reported Western Blot cross-reactivity analysis in plasma samples positive for human CoV-229E, -NL63, -OC43, -HKU1, and SARS-CoV. Strong cross-reactivity was observed only for SARS-CoV.
Infantino 2020	Shenzhen YHLO CLIA	Observed no cross-reactivity in sample from blood donors from the COVID-19 era (winter 2019) but positive results in two samples from people with CMV infections and 2 with rheumatic disease.
Lassauniere 2020 [A]	[A] Beijing Wantai ELISA [B] EUROIMMUN IgG ELISA [C] EUROIMMUN IgA ELISA [D] Dynamiker Biotechnology LFA [E] CTK Biotech - OnSite LFA [F] Autobio Diagnostics LFA [G] Artron Laboratories LFA [H] Acro Biotech LFA [I] Hangzhou Alltest LFA	Included sera from patients with acute viral respiratory tract infections caused by other coronaviruses (n = 5) or non-coronaviruses (n = 45), and sera from patients positive for dengue virus (n = 9), CMV (n = 2) and Epstein Barr virus (n = 10). Cross reaction was observed for the EUROMIMMUN IgA ELISA (> 1 respiratory virus present, adenovirus, dengue virus) and for the EUROMIMMUN IgG ELISA (coronavirus HKU1 and adenovirus). Some cross-reactivity also observed for CGIA tests. Study authors suggest related to antigen target and ELISA format.
Ma 2020a	In-house CLIA	Limited detail but suggests limited cross-reaction
Wang 2020a [A]	A. Beijing Hotgen IgM CGIA B. Beijing Hotgen IgM ELISA	Demonstrated considerable cross-reaction with rheumatoid factor IgM (22/36 false positive results). Other pathogens included influenza A virus (n = 5), influenza B virus (n = 5), *Mycoplasma pneumoniae* (n = 5), *Legionella pneumophila* (n = 5), HIV infection (n = 6), hypertension (n = 5) and diabetes mellitus (n = 5)
Zhang 2020b	Shenzhen YHLO CLIA	Observed false positive results in influenza A and B (2 each), adenovirus (n = 4) and *Mycoplasma pneumoniae* (n = 17).
Zhang 2020d	In-house CGIA (co-author Beijing Hotgen)	Appears to report a separate cross-reactivity study for influenza A, influenza B, respiratory syncytial virus, *Mycoplasma pneumoniae* and *Chlamydia pneumoniae*. No cross reactions were observed.

CGIA: colloidal gold immunoassay; **CLIA:** Chemiluminescence immunoassay; **CMV:** cytomegalovirus; **ELISA:** enzyme-linked immunosorbent assay; **LFA:** lateral flow assay; **MERS:** Middle East respiratory syndrome; **SARS:** severe acute respiratory syndrome

Table 5. Investigation of impact of reference standard on sensitivity

	RT-PCR-positive COVID-19 cases	RT-PCR-negative COVID-19 cases	Comparison
	Test groups [studies] (true positives/COVID cases)		

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 5. Investigation of impact of reference standard on sensitivity *(Continued)*

	Sensitivity (95% CI)[a]		
IgG	26 [15] (1555/2280)	8 [8] (925/1300)	
	87.9% (82.7 to 91.7)	91.2% (83.9 to 95.4)	P = 0.36
IgM	23 [13] (1368/2166)	10 [9] (792/1292)	
	70.8% (56.3 to 82.0)	87.5% (73.7 to 94.6)	P = 0.06
IgG/IgM	17 [6] (966/1278)	4 [4] (400/499)	
	90.6% (86.6 to 93.5)	93.6% (88.9 to 96.4)	P = 0.22

CI: confidence interval; **RT-PCR:** reverse transcription polymerase chain reaction

[a]We obtained sensitivity estimates from a model of all data stratified by week, estimating the average difference in sensitivity across follow-up. The figures quoted correspond to the week 3 strata (15-21 days) in the model.

Table 6. Studies reporting sensitivity in both RT-PCR-positive and RT-PCR-negative subgroups

	RT-PCR-positive COVID-19 cases		RT-PCR-negative COVID-19 cases	
	Test groups [studies] (True positives/COVID-19 cases)	**Sensitivity (95% CI)**	**Test groups [studies] (True positives/COVID-19 cases)**	**Sensitivity (95% CI)**
IgG				
Days 1-7[b]	2 [2] (1/28)		2 [2] (8/13)	
Days 8-14[b]	2 [2] (21/33)		3 [3] (25/30)	
Days 15-21[b]	2 [2] (39/40)		3 [3] (64/72)	
Pooled[a] (stratified by time)		72.6% (46.2% to 89.1%)		84.0% (64.4% to 93.9%)
Test for difference in sensitivity between RT-PCR-positive and RT-PCR-negative groups: P = 0.18				
IgM				
Days 1-7[b]	2 [2] (3/28)		2 [2] (4/13)	
Days 8-14[b]	2 [2] (25/33)		3 [3] (11/30)	
Days 15-21[b]	2 [2] (8/16)		3 [3] (31/72)	
Pooled[a] (stratified by time)		64.6% (49.7% to 77.1%)		49.0% (34.2% to 63.9%)
Test for difference in sensitivity between RT-PCR-positive and RT-PCR-negative group: P = 0.07				
IgG/IgM				

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 6. Studies reporting sensitivity in both RT-PCR-positive and RT-PCR-negative subgroups *(Continued)*

Days 1-7[b]	2 [2] (8/36)	2 [2] (4/17)	
Days 8-14[b]	2 [2] (37/53)	3 [3] (29/40)	
Days 15-21[b]	2 [2] (141/150)	3 [3] (104/113)	
Pooled[a] (stratified by time)		71.9% (58.7% to 82.2%)	71.1% (57.0% to 82.0%)
Test for difference in sensitivity between RT-PCR-positive and RT-PCR-negative group: P = 0.90			

CI: confidence interval; **RT-PCR:** reverse transcription polymerase chain reaction

[a]The sensitivity estimates are produced from a model that combines all data from both subgroups and time-groups, stratifying by time-group. The estimate corresponds to sensitivity in Days 15-21.
[b]RT-PCR-positive data have only been included here when the study includes a RT-PCR-negative subgroup as well.

Table 7. Sensitivity and specificity by test technology

		Test method				
	Test method	**CGIA**	**CLIA**	**ELISA**	**LFA**	**Comparison**
IgG						
	Test groups [studies] **(True positives/COVID cases)**	6 [5] (268/397)	10 [10] (1112/1432)	12 [11] (1014/1552)	7 [1] (133/238)	
	Sensitivity (95% CI)[a]	87.3% (77.0 to 93.4)	94.6% (90.7 to 97.0)	85.8% (78.0 to 91.1)	76.0% (61.0 to 86.5)	P = 0.004
	Test groups [studies] **(True negatives/non-COVID cases)**	11 [11] (409/415)	12 [12] (318/322)	18 [16] (2003/2102)	6 [1] (354/360)	
	Specificity (95% CI)[a]	99.5% (96.5 to 99.9)	99.0% (91.6 to 99.9)	98.8% (96.5 to 99.6)	99.0% (95.3 to 99.8)	P = 0.85
IgM						
	Test groups [studies] **(True positives/COVID cases)**	7 [6] (109/411)	10 [10] (884/1355)	12 [11] (1083/1568)	7 [1] (78/228)	
	Sensitivity (95% CI)[a]	69.5% (44.3 to 86.7)	80.9% (63.8 to 91.0)	84.5% (70.7 to 92.5)	51.4% (26.5 to 75.6)	P = 0.11
	Test groups [studies] **(True negatives/non-COVID cases)**	12 [11] (455/487)	13 [13] (609/621)	14 [12] (1674/1710)	6 [1] (357/360)	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 7. Sensitivity and specificity by test technology *(Continued)*

	Specificity (95% CI)[a]	97.3 (90.0 to 99.3)	98.5 (92.3 to 99.7)	99.1 (97.2 to 99.7)	99.6 (97.3 to 99.9)	P = 0.40
IgG/ IgM						
	Test groups [studies] **(True positives/COVID cases)**	4 [3] (232/316)	3 [3] (344/420)	5 [4] (595/770)	11 [2] (255/358)	
	Sensitivity (95% CI)[a]	90.7% (82.7 to 95.2)	97.5% (94.0 to 99.0)	90.7% (83.3 to 95.0)	88.6% (82.0 to 93.0)	P = 0.02
	Test groups [studies] **(True negatives/non-COVID cases)**	11 [11] (330/353)	5 [4] (230/244)	5 [4] (387/391)	13 [3] (3797/3827)	
	Specificity (95% CI)[a]	96.0 (90.1 to 98.5)	94.1 (82.7 to 98.2)	99.4 (97.4 to 99.9)	98.2 (96.3 to 99.1)	P = 0.05

CGIA: colloidal gold immunoassay; **CI:** confidence interval; **CLIA:** chemiluminescence immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **LFA:** lateral flow assay (no further detail)

[a]We obtained sensitivity estimates from a model of all data stratified by week, estimating the average difference in sensitivity across follow-up. The figures quoted correspond to the Week 3 (15-21 days) strata in the model.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 8. Sensitivity and specificity by test brand (IgG)

Test name[a]	Test method	IgG sensitivity by time since onset of symptoms Studies (true positives/COVID-19 cases) Sensitivity (95% CI)					IgG specificity Studies (false positives/COVID-19 cases) Specificity (95% CI)
		1-7 days	8-14 days	15-21 days	22-35 days	> 35 days	
Beijing Beier Bioengineering	CGIA	1 (2/10)	1 (6/13)	1 (11/14)			
		20.0% (2.5 to 55.6)	46.2% (19.2 to 74.9)	78.6% (49.2 to 95.3)			
Beijing Beier Bioengineering	CLIA	1 (4/10)	1 (6/13)	1 (9/14)			
		40.0% (12.2 to 73.8)	46.2% (19.2 to 74.9)	64.3% (35.1 to 87.2)			
Beijing Beier Bioengineering	ELISA	1 (4/10)	1 (8/13)	1 (12/14)			
		40.0% (12.2 to 73.8)	61.5% (31.6 to 86.1)	85.7% (57.2 to 98.2)			
Beijing Hotgen	ELISA	1 (9/22)	1 (60/92)	1 (51/55)	1 (39/45)		2 (22/172)
		40.9% (20.7 to 63.6)	65.2% (54.6 to 74.9)	92.7% (82.4 to 98.0)	86.7% (73.2 to 94.9)		87.2% (81.3 to 91.8)
Beijing Wantai	ELISA	2 (31/133)	2 (130/210)	2 (127/149)			2 (2/297)
		23.3% (16.4 to 31.4)	61.9% (55.0 to 68.5)	85.2% (78.5 to 90.5)			99.3% (97.6 to 99.9)
Beijing Wantai	CGIA						1 (1/209)
							99.5% (97.4 to 100)
Bioscience Co (Chongqing)	CLIA	2 (43/92)	2 (129/212)	2 (208/244)	2 (98/164)	1 (75/76)	
		46.7% (36.3 to 57.4)	60.8% (53.9 to 67.5)	85.2% (80.2 to 89.4)	59.8% (51.8 to 67.3)	98.6% (92.9 to 100)	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 8. Sensitivity and specificity by test brand (IgG) *(Continued)*

Darui Biotech	ELISA						1 (0/64)
							100% (94.4 to 100)
EUROIMMUN	ELISA	1 (2/13)	2 (13/25)	2 (14/15)	2 (98/164)		2 (3/82)
		15.4% (1.9 to 45.4)	52.0% (31.3 to 72.2)	93.3% (68.1 to 99.8)	59.8% (51.8 to 67.3)		96.3% (89.7 to 99.2)
EUROIMMUN Anti-SARS-Cov	IIFT	1 (1/4)	1 (3/5)	1 (3/3)	1 (1/1)		1 (0/10)
		25.0% (0.6 to 80.6)	60.0% (14.7 to 94.7)	100% (29.2 to 100)	100% (2.5 to 100)		100% (69.2 to 100)
EUROIMMUN Beta	ELISA	1 (0/12)	1 (3/10)	1 (7/8)	1 (1/1)		1 (0/45)
		0% (0 to 26.5)	30%.0% (14.7 to 94.7)	87.5% (47.3 to 99.7)	100% (2.5 to 100)		100% (92.1 to 100)
Hangzhou Alltest - IgG/IgM	CGIA	1 (1/8)	2 (21/42)	2 (57/68)			2 (0/45)
		12.5% (0.3 to 52.7)	50.0% (34.2 to 65.8)	83.8% (72.9 to 91.6)			100% (92.1 to 100)
Innovita Biological - Ab test (IgM/IgG)	CGIA	1 (7/13)	1 (7/8)	1 (21/23)			
		53.8% (25.1 to 80.8)	87.5% (47.3 to 99.7)	91.3% (72.0 to 98.9)			
Shenzhen YHLO	CLIA	2 (2/8)	2 (28/29)	2 (25/26)	2 (64/64)	1 (7/7)	7 (4/322)
		25.0% (3.2 to 65.1)	96.6% (82.2 to 99.9)	96.2% (80.4 to 99.9)	100% (94.4 to 100)	100% (59.0 to 100)	98.8% (96.9 to 99.7)
Snibe Diagnostic - MAGLUMI	CLIA	2 (11/40)	2 (35/48)	25/25			
		27.5% (14.6 to 43.9)	72.9% (58.2 to 84.7)	100.0% (86.3 to 100)			
Vivachek - VivaDiag IgM/IgG	CGIA						2 (0/42)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 8. Sensitivity and specificity by test brand (IgG) *(Continued)*

						100% (91.6 to 100)
Zhuhai Livzon	CGIA	1 (5/36)	1 (20/34)	1 (35/38)		2 (0/35)
		13.9% (4.7 to 29.5)	58.8% (40.7 to 75.4)	92.1% (78.6 to 98.3)		100% (90.0 to 100)
Zhuhai Livzon	ELISA	4 (17/80)	3 (163/288)	3 (197/223)	2 (91/104)	5 (5/351)
		21.3% (12.9 to 31.8)	56.6% (50.7 to 62.4)	88.3% (83.4 to 92.2)	87.5% (79.6 to 93.2)	98.6% (96.7 to 99.5)

CGIA: colloidal gold immunoassay; **CI:** confidence interval; **CLIA:** chemiluminescence immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **FIA:** fluorescence immunoassay; **IIFT:** indirect immunofluorescence assay; **LFA:** lateral flow assay

[a]See Appendix 12 for details of manufacturer product codes, where available.

Table 9. Sensitivity and specificity by test brand (IgM)

Test name[a]	**Test method**	**IgM sensitivity by time since onset of symptoms** **Studies (true positives/COVID-19 cases)** **Sensitiivity (95% CI)**					IgM **specificity** **Studies (false positives/COVID-19 cases)** **Specificity (95% CI)**
		1-7 days	**8-14 days**	**15-21 days**	**22-35 days**	**> 35 days**	
Artron Laboratories IgM/IgG	CGIA		1 (5/7)	1 (12/15)	1 (8/8)		
			71.4% (29.0 to 96.3)	80.0% (51.9 to 95.7)	100% (63.1 to 100)		
Autobio Diagnostics IgM/IgG	CGIA		1 (6/7)	1 (14/15)	1(8/8)		
			85.7% (42.1 to 99.6)	93.3% (68.1 to 99.8)	100% (63.1 to 100)		
Beijing Hotgen	ELISA	1 (10/22)	1 (72/92)	1 (72/92)	1 (41/45)		1 (0/100)

Table 9. Sensitivity and specificity by test brand (IgM) *(Continued)*

		45.5% (24.4 to 67.8)	78.3% (68.4 to 86.2)	78.3% (68.4 to 86.2)	91.1% (78.8 to 97.5)	100% (96.4 to 100)
Beijing Hotgen	CGIA					1 (22/72)
						69.4% (57.5 to 79.8)
Beijing Wantai	ELISA					1 (3/513)
						99.4% (98.3 to 99.9)
Beijing Wantai	CGIA					1 (4/209)
						98.1% (95.2 to 99.5)
Bioscience Co (Chongqing)	CLIA	1 (34/67)	1 (34/67)	1 (131/134)	1 (13/13)	
		50.7% (38.2 to 63.2)	50.7% (38.2 to 63.2)	97.8% (93.6 to 99.5)	100% (75.3 to 100)	
CTK Biotech OnSite IgG/IgM	CGIA		1 (5/7)	1 (14/15)	1 (8/8)	
			71.4% (29.0 to 96.3)	93.3% (68.1 to 99.8)	100% (63.1 to 100)	
Darui Biotech	ELISA					1 (14/64)
						78.1% (66.0 to 87.5)
Dynamiker Biotechnology IgG/IgM	CGIA		1 (5/7)	1 (14/15)	1 (8/8)	
			71.4% (29.0 to 96.3)	93.3% (68.1 to 99.8)	100% (63.1 to 100)	
EUROIMMUN	ELISA					1 (76/82)
						92.7% (84.8 to 97.3)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 9. Sensitivity and specificity by test brand (IgM) *(Continued)*

EUROIMMUN Anti-SARS-Cov	IIFT					1 (1/10)
						90.0% (55.5 to 99.7)
Hangzhou Alltest - IgG/IgM	CGIA	1 (1/8)	2 (23/42)	2 (58/68)		2 (0/45)
		12.5% (0.3 to 52.7)	54.8% (38.7 to 70.2)	85.3% (74.6 to 92.7)		100% (92.1 to 100)
Shenzhen YHLO	CLIA					7 (10/321)
						96.9% (94.3 to 98.5)
Vivachek - VivaDiag IgM/IgG	CGIA					2 (1/42)
						97.6% (87.4 to 99.9)
Xiamen InnodDx Biotech	CLIA					1 (2/300)
						99.3% (97.6 to 99.9)
Zhuhai Livzon	CGIA	1 (7/36)	1 (31/34)	1 (35/38)		2 (0/35)
		19.4% (8.2 to 36.0)	91.2% (76.3 to 98.1)	92.1% (78.6 to 98.3)		100% (90.0 to 100)
Zhuhai Livzon	ELISA	3 (14/66)	2 (150/202)	2 (159/166)	1 (43/45)	5 (3/351)
		21.2% (12.1 to 33.0)	74.3% (67.7 to 80.1)	95.8% (91.5 to 98.3)	95.6% (84.9 to 99.5)	99.1% (97.5 to 99.8)

CGIA: colloidal gold immunoassay; **CI:** confidence interval; **CLIA:** chemiluminescence immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **FIA:** fluorescence immunoassay; **IIFT:** indirect immunofluorescence assay; **LFA:** lateral flow assay

[a]See Appendix 12 for details of manufacturer product codes, where available.

Table 10. Sensitivity and specificity by test brand (IgG/IgM)

Test name[a]	Test method	IgG/IgM sensitivity by time since onset of symptoms				IgG/IgM specificity

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 10. Sensitivity and specificity by test brand (IgG/IgM) *(Continued)*

		Studies (true positives/COVID-19 cases) Sensitiivity (95% CI)					Studies (false positives/COVID-19 cases) Specificity (95% CI)
		1-7 days	**8-14 days**	**15-21 days**	**22-35 days**	**> 35 days**	
Acro Biotech - IgG/IgM	CGIA						1 (3/15)
							80.0% (51.9 to 95.7)
Artron Laboratories IgM/IgG	CGIA		1 (5/7)	1 (12/15)	1 (8/8)		1 (0/17)
			71.4% (29.0 to 96.3)	80.0% (51.9 to 95.7)	100% (63.1 to 100)		100% (80.5% to 100)
Autobio Diagnostics IgM/IgG	CGIA		1 (6/7)	1 (14/15)	1(8/8)		1 (0/32)
			85.7% (42.1 to 99.6)	93.3% (68.1 to 99.8)	100% (63.1 to 100)		100% (89.1 to 100)
Beijing Hotgen	ELISA	1 (10/22)	1 (72/92)	1 (72/92)	1 (41/45)		1 (0/100)
		45.5% (24.4 to 67.8)	78.3% (68.4 to 86.2)	78.3% (68.4 to 86.2)	91.1% (78.8 to 97.5)		100% (96.4 to 100)
Bioscience Co (Chongqing)	CLIA	1 (34/67)	1 (34/67)	1 (131/134)	1 (13/13)		2 (7/148)
		50.7% (38.2 to 63.2)	50.7% (38.2 to 63.2)	97.8% (93.6 to 99.5)	100% (75.3 to 100)		95.3% (90.5 to 98.1)
CTK Biotech OnSite IgG/IgM	CGIA		1 (5/7)	1 (14/15)	1 (8/8)		1 (0/32)
			71.4% (29.0 to 96.3)	93.3% (68.1 to 99.8)	100% (63.1 to 100)		100% (89.1 to 100)
Dynamiker Biotechnology IgG/IgM	CGIA		1 (5/7)	1 (14/15)	1 (8/8)		1 (0/32)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Table 10. Sensitivity and specificity by test brand (IgG/IgM) *(Continued)*

			71.4% (29.0 to 96.3)	93.3% (68.1 to 99.8)	100% (63.1 to 100)	100% (89.1 to 100)
Hangzhou Alltest - IgG/IgM	CGIA	1 (1/8)	2 (23/42)	2 (58/68)		3 (2/60)
		12.5% (0.3 to 52.7)	54.8% (38.7 to 70.2)	85.3% (74.6 to 92.7)		96.7% (88.5 to 99.6)
Shenzhen YHLO	CLIA					2 (7/96)
						92.7% (85.6 to 97.0)
Vivachek - VivaDiag IgM/IgG	CGIA					3 (14/162)
						91.4% (85.9 to 95.2)
Zhuhai Livzon	CGIA	1 (7/36)	1 (31/34)	1 (35/38)		2 (0/35)
		19.4% (8.2 to 36.0)	91.2% (76.3 to 98.1)	92.1% (78.6 to 98.3)		100% (90.0 to 100)
Zhuhai Livzon	ELISA	3 (14/66)	2 (150/202)	2 (159/166)	1 (43/45)	4 (4/291)
		21.2% (12.1 to 33.0)	74.3% (67.7 to 80.1)	95.8% (91.5 to 98.3)	95.6% (84.9 to 99.5)	98.6% (96.5 to 99.6)

CGIA: colloidal gold immunoassay; **CI:** confidence interval; **CLIA:** chemiluminescence immunoassay; **ELISA:** enzyme-linked immunosorbent assay; **FIA:** fluorescence immunoassay; **IIFT:** indirect immunofluorescence assay; **LFA:** lateral flow assay

[a]See Appendix 12 for details of manufacturer product codes, where available.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

APPENDICES

Appendix 1. Summary of World Health Organization and Chinese National Health Commission Guidelines for the diagnosis of SARS-CoV-2

Table A: World Health Organization guidelines for the diagnosis of SARS-CoV-2[a]

Includes laboratory testing guidelines and global surveillance guidelines

Date range (2020)	Definition of confirmed case	Definition of confirmed non-case	Definition of suspect case	Definition of probable case	Role of serology in testing
10-30 January	10-30 January: no documentation to define at this time (before first date of global guidelines) 31 January onwards: a confirmed case is a person with laboratory confirmation of COVID-19 infection, irrespective of clinical signs and symptoms. No prescribed test in laboratory guidelines, suggested tests from 10 January include broad coronavirus RT-PCR (with sequencing of precise virus in test positives), whole genome sequencing, broad coronavirus serology on paired samples, microscopy, culture. (Lab 10 January) Four suggested tests from 17 January: broad coronavirus RT-PCR (with sequencing of precise virus in test positives), NAAT for SARS-CoV-2 when it becomes available, whole genome sequencing, and broad coronavirus serology on paired samples.	None stated	No definition of 'suspect case' at this time, but case definitions for surveillance are defined as a combination of symptoms and exposure, with more severe symptoms requiring less evidence for exposure	No definition at this time	Serological testing may be useful to confirm immunologic response to a pathogen from a specific viral group, e.g. coronavirus. Best results from serologic testing requires the collection of paired serum samples (in the acute and convalescent phase) from cases under investigation.
31 January-26 February	States that once specific NAAT assays are developed and validated, confirmation will be based on specific detection of unique sequences of viral nucleic acid by RT-PCR.	None stated	Suspect case defined as combination of symptoms and exposure, with more severe symptoms requiring less evidence for exposure	A suspect case with inconclusive laboratory results or is test-positive using a pan-coronavirus assay without laboratory evidence of other respiratory pathogens. (global 31 January)	
27 February-1 March		None stated	Suspect case defined as combination of symptoms and exposure, with more severe symp-	A suspected case with inconclusive laboratory results	
2 March-19 March	A person with laboratory confirmation of COVID-19 infection, irrespective of clinical signs and symptoms. (global 31 January, 27 February, 20 March)	One or more negative			In cases where NAAT assays are negative and

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

19 March-present	Laboratory confirmation of cases by NAAT specific to SAR-CoV-2 such as real-time reverse-transcription polymerase chain reaction (rRT-PCR) with confirmation by nucleic acid sequencing when necessary. The viral genes targeted so far include the N, E, S and RdRP genes. In areas with no known COVID-19 virus circulation confirmation requires: • NAAT positive for at least two different targets on the COVID-19 virus genome, of which at least one target is preferably specific for COVID-19 virus (or SARS-like coronavirus) using a validated assay; OR • NAAT-positive result for betacoronavirus, and COVID-19 virus identified by sequencing partial/whole genome of virus (sequence target larger or different from the amplicon probed in the NAAT assay). Discordant results should be resampled. In areas where COVID-19 virus is widely spread a simpler algorithm might be adopted (e.g. RT-PCR of a single discriminatory target)	results do not rule out the possibility of COVID-19 virus infection.	toms requiring less evidence for exposure, OR defined by symptoms requiring hospitalisation and an absence of alternative explanation.	(global 27 February) Probable case A suspect case for whom testing for the COVID-19 virus is inconclusive. OR A suspect case for whom testing could not be performed for any reason.	there is a strong epidemiological link to COVID-19 infection, paired serum samples (in the acute and convalescent phase) could support diagnosis once validated serology tests are available. Serological assays will play an important role in research and surveillance but are not currently recommended for case detection.

NAAT: nucleic acids amplification test; **RT-PCR:** reverse transcription polymerase chain reaction; Source: WHO 2020.

[a]Source data from *Laboratory testing of 2019 novel coronavirus (2019-nCoV) in suspected human cases: interim guidance, World Health Organization*. (2020), 10 January, 17January, 2nd March, 19 March, 21st March, and *Global surveillance for COVID-19 caused by human infection with COVID-19 virus, interim guidance*, 31st January, 27 February, and 20 March.

Table B: Summary of Chinese National Health Commission guidelines for diagnosis and treatment for novel coronavirus pneumonia (trial versions 1-7)

Dates in effect	Definition of confirmed case	Definition of confirmed non-case	Definition of suspect case	Role of serology in testing
16-17 January 2020 (version 1)	Cases (not confirmed cases) defined as virus genome highly homologous to coronaviruses	Not defined	Observation cases: defined as combination of exposure in Wuhan and symptoms focused on pneumonia, leukopenia and lack of improvement.	No role
18 January-2 March (versions 2, 3, 4, 5, 5 revised, and 6)	Suspect cases with either • real-time fluorescent RT-PCR indicates positive for new coronavirus nucleic acid; OR • viral gene sequence is highly homologous to known new coronaviruses.	Suspect cases can be ruled out after 2 consecutive negative respiratory tract nucleic acid tests taken at least 24-hours apart.	Suspect cases: combination of exposure (such as residence in/travel to Wuhan or exposure to a confirmed case within 14 days of onset) AND clinical features (such as symptoms: fever, respiratory symptoms, and tests: chest imaging, white blood cell and lymphocyte count). Exact definition varies slightly with version	No role
3 March-present (version 7)	Suspect cases with either	Suspect cases can be ruled out after 2 negative NAATs,	Suspect cases: combination of exposure (such as residence in/travel to Wuhan or exposure to a confirmed	Part of definition of cases and

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

• real-time fluorescent RT-PCR indicates positive for new coronavirus nucleic acid; OR • viral gene sequence is highly homologous to known new coronaviruses. OR • NCP virus-specific IgM and IgG are detectable in serum; NCP virus-specific IgG is detectable or reaches a titration of at least 4-fold increase during convalescence compared with the acute phase.	taken at least 24-hours apart, and the NCP virus-specific IgM and IgG are negative after 7 days from onset.	case within 14 days of onset) AND clinical features (such as symptoms: fever, respiratory symptoms, and tests: chest imaging, white blood cell and lymphocyte count).	confirmed non-cases

NAAT: nucleic acids amplification test; **NCP:** novel coronavirus pneumonia; **RT-PCR:** reverse transcription polymerase chain reaction; Source: CDC China 2020.

Appendix 2. Antibody test 'use case' scenarios

Use Case[a]	Advantages	Limitations	Considerations
Diagnosis			
Aid diagnosis of suspect cases, especially when RT-PCR negative but X-Ray/CT suggestive	May improve overall sensitivity of diagnosis Diagnosis of patients presenting late or for post-infectious syndromes (low viral load) Diagnosis of patients when lower respiratory tract sampling not available	Unlikely to catch early-stage infection (< 7 days) May not detect asymptomatic cases Negative test cannot rule out infection IgM appears early, but is less specific	Total antibody may have best sensitivity Should be confirmed by PCR, where possible Rising titres and seroconversion can improve sensitivity and specificity
Aid diagnosis of suspect cases when PCR is not available **(would require careful development of interpretive guidelines)**	As above and could enable decentralised/community testing in settings where the availability of PCR testing is limited.		
Identification of individuals with protective immune status **(conditional upon identifying correlates of protection for SARS-CoV-2)**			
Identify convalescent plasma donors	Treatment for critically ill patients	Ideal timing of collection unknown to optimise efficaciousness	Preferentially patients recovered from moderate to severe disease (high titre). Theoretically may be derived from vaccinated donors

CT: computed tomography; **RT-PCR:** reverse transcription polymerase chain reaction;

[a]Table from Cheng 2020b

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Appendix 3. Cochrane COVID-19 Study Register searches

Source	Strategy
CT.gov	COVID-19[a]
WHO ICTRP	Health topic: 2019-nCov / COVID-19
PubMed	(("2019 nCoV"[tiab] OR 2019nCoV[tiab] OR "2019 novel coronavirus"[tiab] OR "COVID 19"[tiab] OR COVID19[tiab] OR "new coronavirus"[tiab] OR "novel coronavirus"[tiab] OR "novel corona virus"[tiab] OR "SARS CoV-2"[tiab] OR (Wuhan[tiab] AND (coronavirus[tiab] OR "corona virus"[tiab])) OR "COVID-19"[Supplementary Concept] OR "severe acute respiratory syndrome coronavirus 2"[Supplementary Concept]) NOT ("animals"[MeSH Terms] NOT "humans"[MeSH Terms])) NOT (editorial[pt] OR comment[pt] OR letter[pt] OR newspaper article[pt])

[a]Automatic term mapping links results for 2019-nCoV, 2019 novel coronavirus, SARS-CoV-2, severe acute respiratory syndrome coronavirus 2.

Appendix 4. Living search from the University of Bern

The following information is taken from the university of Bern website (see: ispmbern.github.io/covid-19/living-review/collectingdata.html).

The register is updated daily and CSV file downloads are made available.

1 April 2020

From 1 April 2020, we will retrieve the curated BioRxiv/MedRxiv dataset (connect.medrxiv.org/relate/content/181).

26 to 31 March 2020

MEDLINE: (\"Wuhan coronavirus\" [Supplementary Concept] OR \"COVID-19\" OR \"2019 ncov\"[tiab] OR ((\"novel coronavirus\"[tiab] OR \"new coronavirus\"[tiab]) AND (wuhan[tiab] OR 2019[tiab])) OR 2019-nCoV[All Fields] OR (wuhan[tiab] AND coronavirus[tiab])))))

Embase: (nCoV or 2019-nCoV or ((new or novel or wuhan) adj3 coronavirus) or covid19 or covid-19 or SARS-CoV-2).mp.

BioRxiv/MedRxiv: ncov or corona or wuhan or COVID or SARS-CoV-2

With the kind support of the Public Health & Primary Care Library PHC (www.unibe.ch/university/services/university_library/faculty_libraries/medicine/public_health_amp_primary_care_library_phc/index_eng.html), and following guidance of the Medical Library Association (www.mlanet.org/p/cm/ld/fid=1713).

1 January 2020 to 25 March 2020

MEDLINE: ("Wuhan coronavirus" [Supplementary Concept] OR "COVID-19" OR "2019 ncov"[tiab] OR (("novel coronavirus"[tiab] OR "new coronavirus"[tiab]) AND (wuhan[tiab] OR 2019[tiab])) OR 2019-nCoV[All Fields] OR (wuhan[tiab] AND coronavirus[tiab])))))

Embase: ncov OR (wuhan AND corona) OR COVID

BioRxiv/MedRxiv: ncov or corona or wuhan or COVID

Appendix 5. CDC Library, COVID-19 Research Articles Downloadable Database

Embase records from the Stephen B. Thacker CDC Library, Covid-19 Research articles Downloadable database

Records were obtained by the CDC library by searching Embase through Ovid using the following search strategy.

Source	Strategy

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Embase	coronavir* OR corona virus* OR betacoronavir* OR covid19 OR covid 19 OR nCoV OR novel CoV OR CoV 2 OR CoV2 OR sarscov2 OR 2019nCoV OR wuhan virus*).mp. OR ((wuhan OR hubei OR huanan) AND (severe acute respiratory OR pneumonia*) AND outbreak*).mp. OR Coronavirus infection/ OR coronavirinae/ OR exp betacoronavirus/ Limits: 2020- OR (novel coronavir* OR novel corona virus* OR covid19 OR covid 19 OR nCoV OR novel CoV OR CoV 2 OR CoV2 OR sarscov2 OR 2019nCoV OR wuhan virus*).mp. OR ((wuhan OR hubei OR huanan) AND (severe acute respiratory OR pneumonia*) AND outbreak*).mp. OR ((wuhan OR hubei OR huanan) AND (coronavir* OR betacoronavir*)).mp. Limits: 2019-

Appendix 6. Data extraction items

Patient sampling items	Patient characteristics and setting items	Index test items	Reference standard items	Flow and timing items	Notes items
A0 Test type (antibody/antigen etc)	COVID patients (or all patients if single group study)				
A1 Purpose	B1 Setting	D1.1 Test name	E1 Reference standard for cases including threshold	F1 What was the time interval between index and reference tests?	G1: Funding
A2 Design (and description of groups labelled [1] [2] …)	B2 Location (include name of institution if available)	D1.2 Manufacturer	E2 Samples used	F2 Did all patients receive the same reference standard?	G2: Publication status
A3 Recruitment	B3 Country	D1.3 Antibody targets	E3 Timing of reference standard (preferably since symptom onset only, if not from a different time points)	F3 Missing data	G3: Source (preprint or journal name)
A4 Were cases recruited prospectively or retrospectively?	B4 Dates	D1.4 Antigens used	E4 Was it blind to index test?	F4 Uninterpretable results	G4: Study author COI (including any manufactur-

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

					er affiliations)
A5 Sample size (virus/ COVID cases)	B5 Symptoms and severity	D1.5 Point-of-care or laboratory (is the test designed to be used at point-of-care or in laboratory, and was it used as point-of-care or in laboratory)?	E5 Did it incorporate index test?	F5 Indeterminate results	G5 Comment
A6 Inclusion and exclusion criteria	B6 Demographics	D1.6 Test method		F6 Samples or patients	
A7 Comment	B7 Exposure history	D1.7 When were samples taken (preferably since symptom onset only, if not from a different time points)?	E6 Reference standard for non-cases	F7 Comment	
	B8 Comment	D1.8 Samples used	E7 Samples used		
	Non-COVID patients (if additional groups)	D1.9 Who applied the test	E8 Timing of reference standard (preferably since symptom onset only, if not from a different time points)		
	C1.1 Group name	D1.10 How was positive defined?	E9 Was it blind to index test?		
	C1.2 Source and time	D1.11 Blinded to reference standard	E10 Did it incorporate index test?		
	C1.3 Characteristics	D1.12 Threshold predefined	E11 Comment		
	C2.1 Group name	D1.13 Comment			
	C2.2 Source and time				
	C2.3 Characteristics				
	C4 Comment				

Appendix 7. Criteria for assessment of study quality (QUADAS-2)

DOMAIN: PARTICIPANT SELECTION	
Was a consecutive or random sample of patients enrolled?	This will be similar for all index tests, target conditions, and populations. YES: if a study explicitly stated that all participants within a certain time frame were included; that this was done consecutively; or that a random selection was done. NO: if it was clear that a different selection procedure was employed; for example, selection based on clinician's preference, or based on institutions.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

	UNCLEAR: if the selection procedure was not clear or not reported.
Was a case-control design avoided?	This will be similar for all index tests, target conditions, and populations. YES: if a study explicitly stated that all participants came from the same group of (suspected) patients. NO: if it was clear that a different selection procedure was employed for the participants depending on their COVID-19 status or SARS-CoV-2 infection status; or if only participants with SARS-CoV-2 infection were included UNCLEAR: if the selection procedure was not clear or not reported.
Did the study avoid inappropriate exclusions?	Studies may have excluded patients, or selected patients in such a way that they avoided including those who were difficult to diagnose or likely to be borderline. Although the inclusion and exclusion criteria will be different for the different index tests, inappropriate exclusions and inclusions will be similar for all index tests: for example, only elderly patients excluded, or children (as sampling may be more difficult). This needs to be addressed on a case-to-case basis. YES: if a high proportion of eligible patients was included without clear selection. NO: if a high proportion of eligible patients was excluded without providing a reason; if, in a retrospective study, participants without index test or reference standard results were excluded. UNCLEAR: if the exclusion criteria were not reported.
Did the study avoid inappropriate inclusions?	Some laboratory studies may have intentionally included groups of patients in whom the accuracy was likely to differ, such as those with particularly low or high viral loads, or who had other diseases, such that the sample over-represented these groups. This needs to be addressed on a case-to-case basis. Artificial spiked samples are a clear example. YES: if samples included were likely to be representative of the spectrum of disease. NO: if the study oversampled patients with particular characteristics likely to affect estimates of accuracy. UNCLEAR: if the exclusion criteria were not reported.
Could the selection of patients have introduced bias?	HIGH: if one or more signalling questions were answered with NO, as any deviation from the selection process may lead to bias. LOW: if all signalling questions were answered with YES. UNCLEAR: all other instances.
Is there concern that the included participants do not match the review question?	HIGH: for two-group studies that included healthy or other disease controls, whether pre-pandemic or contemporaneous; studies that only included people with COVID-19 (whether reverse transcription polymerase chain reaction (RT-PCR)-confirmed only, participants meeting official guideline criteria); LOW: for single-group studies recruiting participants with signs and symptoms of COVID-19; or for two-group studies where control groups suspected of COVID-19 were separately recruited. UNCLEAR: if a description about the participants was lacking.
DOMAIN: INDEX TESTS	
Were the index test results interpreted without knowledge of the results of the reference standard?	YES: if blinding was explicitly stated or index test was recorded before the results from the reference standard were available. NO: if it was explicitly stated that the index test results were interpreted with knowledge of the results of the reference standard.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

	UNCLEAR: if blinding was unclearly reported.
If a threshold was used, was it prespecified?	YES: if the test was dichotomous by nature, or if the threshold was stated in the methods section, or if study authors stated that the threshold as recommended by the manufacturer was used. NO: if a receiver operating characteristic curve was drawn or multiple threshold reported in the results section; and the final result was based on one of these thresholds. UNCLEAR: if threshold selection was not clearly reported.
Could the conduct or interpretation of the index test have introduced bias?	HIGH: if one or more signalling questions were answered with NO, as even in a laboratory situation knowledge of the reference standard may lead to bias. LOW: if all signalling questions were answered with YES. UNCLEAR: all other instances.
Is there concern that the index test, its conduct, or interpretation differ from the review question?	For evaluations of laboratory-based tests, HIGH: if tests were built in-house, or if commercially available tests using SARS-Cov antigens instead of SARS-CoV-2-specific antigens. LOW: most other laboratory-evaluations UNCLEAR: name of the test was withheld For evaluations of lateral flow assays, HIGH: if tests were built in-house; if only serum or plasma instead of fingerprick or whole blood samples were used; if test evaluated in laboratory settings rather than at the point of care LOW: commercially available tests, using whole blood or fingerprick samples, and that were conducted in the intended setting for the test (i.e. point-of-care). UNCLEAR: name of the test was withheld; mixed sample types; or did not report the evaluation setting
DOMAIN: REFERENCE STANDARD	
Is the reference standard likely to correctly classify the target condition?	We will define acceptable reference standards using a consensus process once the list of reference standards that have been used has been obtained from the eligible studies. For COVID-19 cases YES: RT-PCR; confirmed or suspected case using official criteria (WHO, CDC) or a clearly set out combination of signs/symptoms/exposure. NO: RT-PCR not used, or if inadequate combination of clinical characteristics used in PCR negatives, e.g. computed tomography alone UNCLEAR: if definition of COVID-19 was not reported For absence of COVID-19 YES: if at least 2 negative RT-PCR results reported if suspected COVID-19 based on signs/symptoms; single negative RT-PCR test for asymptomatic contacts or contemporaneous controls with no clinical suspicion of COVID-19; only pre-pandemic sources of control samples used. NO: single RT-PCR or number of negative RT-PCRs not reported for COVID-19 suspects; no RT-PCR reported (untested) for asymptomatic contacts or contemporaneous controls UNCLEAR: if timing of control samples (pre-pandemic or contemporaneous) was not reported
Were the reference standard results interpreted without	YES: if it was explicitly stated that the reference standard results were interpreted without knowledge of the results of the index test, or if the result of the index test was obtained after the reference standard.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

knowledge of the results of the index test?	NO: if it was explicitly stated that the reference standard results were interpreted with knowledge of the results of the index test or if the index test was used to make the final diagnosis. UNCLEAR: if blinding was unclearly reported.
Did the definition of the reference standard incorporate results from the index test(s)?	YES: if results from the index test were a component of the reference standard definition. NO: if the reference standard did not incorporate the index standard test. UNCLEAR: if it was unclear whether the results of the index test formed part of the reference standard.
Could the conduct or interpretation of the reference standard have introduced bias?	HIGH: if one or more signalling questions were answered with NO. LOW: if all signalling questions were answered with YES. UNCLEAR: all other instances.
Is there concern that the target condition as defined by the reference standard does not match the review question?	Applicability was judged primarily on the definition of disease-positive. HIGH: if RT-PCR alone used to define cases LOW: if clinical criteria, including RT-PCR, were used to define cases, regardless of whether official criteria were used, as long as the criteria were explicitly described. UNCLEAR: if definition of COVID-19 cases was not provided, including if some clinically diagnosed cases were included but the clinical criteria used were not described.
DOMAIN: FLOW AND TIMING	
Did all participants receive the same reference standard?	YES: if all participants received the same reference standard (clearly no differential verification). NO: if (part of) the index test-positives or index test-negatives received a different reference standard. UNCLEAR: if it was not reported.
Were all participants included in the analysis?	YES: if it is clear that all eligible participants were included in the analyses. NO: if after the inclusion/exclusion process, participants were removed from the analyses for different reasons: no reference standard done, no index test done, intermediate results of both index test or reference standard, indeterminate results of both index test or reference standard, samples unusable. UNCLEAR: if it is not possible to determine whether all participants were included (e.g. from a STARD style participant flow diagram)
Did all participants receive a reference standard?	YES: if all participants received a reference standard (clearly no partial verification). NO: if only (part of) the index test positives or index test negatives received the complete reference standard. UNCLEAR: if it was not reported.
Were results presented per participant?	YES: if either only one sample per participant (regardless of disaggregation of results over time), or if multiple samples per participant but results are disaggregated by time period (at least week by week) NO: if multiple samples per participant and results are not disaggregated by time period UNCLEAR: if it is not possible to tell whether results presented are per participant or per sample

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Could the participant**flow have introduced bias?**	HIGH: if one or more signalling questions were answered with NO. LOW: if all signalling questions were answered with YES. UNCLEAR: all other instances.

CDC: Centers for Disease Control; **ICU:** intensive care unit; **RT-PCR:** real-time polymerase chain reaction; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **WHO:** World Health Organization

Footnotes

Appendix 8. Summary details of study design and participants

This Appendix includes two tables. Please note that square brackets indicate different tests within one study.

1. Table A. Single-group studies estimating sensitivity (and specificity)
2. Table B. Two-group or more studies estimating sensitivity and specificity

Table A. Single-group studies estimating sensitivity (and specificity)

Study (source)	Inclusion criteria • **method used to rule out COVID-19**	Instititution (recruitment dates)	Age (median) n, % male	Exposure history Symptoms/severity	Reference details (cases)	Missing or uninterpretable data
Single-group studies estimating sensitivity and specificity						
Cassaniti 2020 (B) (published; letter) 50 participants (50 samples)	COVID-19-suspected cases presenting at A&E with fever and respiratory syndrome (n = 50, including 38 RT-PCR-positive); • 2 x RT-PCR-negative required to rule out disease (Additional groups reported in Cassaniti 2020 (A))	A&E; Pavia, Italy (not stated)	61.5 years 34, 68%	Not stated Not stated	RT-PCR detecting RNA polymerase and E genes; nasal swab (On presentation at A&E)	Weakly positive results counted as test positive
Liu 2020a (preprint) 179 participants (179 samples)	Inpatients and outpatients attending hospital during pandemic including COVID-19-suspected cases (all inpatient, n = 114) and outpatients (n = 64) with 'other disease'. (n = 179, including 90 PCR-confirmed and 5 clinically confirmed cases) • Negative PCR and insufficient evidence for clinical confirmation required to rule out disease	Inpatient and outpatient; Wuhan, China (1 January-12 March 2020)	[1] mean 76 years [2+3] mean 56 years [1] 60, 67% [2+3] 38, 43%	Not reported Of 90 RT-PCR+, 44, 49% severe/critical cases	Clinical criteria (not clearly described) ≤ RT-PCR; nasal and pharyngeal swabs (NR)	Per sample data by time period is based on

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Long 2020 (A) (preprint) 164 participants (164 samples)	Cohort of close contacts of 2 index cases (n = 164, 16 PCR-positive cases) • 1 x RT-PCR-negative required to rule out disease	Close contacts; Wanzhou, China (31 January-9 February)	Not stated Not stated	All exposed 151 (92%) asymptomatic	RT-PCR; NP (within 17 days of contact with confirmed cases)	None stated
Paradiso 2020a (preprint) 191 participants (191 samples)	Symptomatic patients accessing A&E (n = 191, including 70 PCR-positive) • 1 x RT-PCR-negative required to rule out disease	A&E; Bari, Italy (23-29 March)	58.5 years 116, 61%	Not stated 14, 9% asymptomatic	RT-PCR (Allplex 2019-nCoV Assay; Seegene, Seoul, Republic of Korea); NP, OP (Simultaneous)	1 D+ missing from results
Zhang 2020b (preprint) 228 participants (228 samples)	Suspected COVID-19 cases admitted to fever clinic (n = 228, including 3 PCR-positive) • 1 x RT-PCR negative required to rule out disease (review team excluded additional reported groups)	Inpatients, Shengjing, China (21 January-16 February)	Mean 51 years (cases only) Not stated	1, 33% Wuhan contact history (cases only) Not stated	RT-PCR (required presence of ORF1ab and N gene for positive result); NP, OP (Timing not stated)	Not stated
Zhang 2020d (preprint) 814 participants (814 samples)	Participants suspected of harbouring COVID-19 (n = 814, including 154 cases; 122 RT-PCR-positive and 32 clinically diagnosed by CT) • 1 x RT-PCR negative required to rule out disease; unclear if CT used in all D- (n = 663)	Samples from 5 hospitals (in/outpatient not stated); centres including Wuhan, Shenyang and Beijing, China (Not stated)	Not stated	Not stated	Real-time PCR kit (no details on threshold); CT used in at least some PCR-negative NP swabs. (Timing not stated)	None stated
Single group studies estimating sensitivity alone						
Du 2020 (published; letter) 60 participants (60 samples)	Single group of convalescent inpatients 6-7 weeks after symptom onset (n = 60) • Non-COVID-19 cases not included	Hospital inpatients; Wuhan, China (12 January-5 February 2020)	Not stated	Not stated	Not described; not stated (During hospital stay)	None described
Gao 2020a (published; letter) 38 participants (38 samples)	Inpatient cohort of COVID-19 patients confirmed by Chinese Government-issued guidelines (5th edition) • non-COVID-19 cases not included	Inpatient; Fuyang, China (22 January-28 February 2020)	40.5 years 21, 55.3%	Not stated 3, 8% severe or critical, 35 mild	Chinese guideline (5th edition)	Not reported
Gao 2020b [A] (accepted manuscript	Confirmed COVID-19 cases (n = 22) • non-COVID-19 cases not included	Hospital inpatient; Shijiazhuang, Hebei, China (21 Janu-	40 years 14, 64%	11 (50%) recent travel to epidemic areas,	RT-PCR assay (2019-nCoV RNA Test Kit, Daan Gene Company, China); Nasal and	None described

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

(peer reviewed; pre-proof) 22 participants (37 samples)		ary-24 February 2020)		10 (45%) close contacts with confirmed COVID-19 cases 22 (100%) typical CT findings; 'most' received oxygen therapy	pharyngeal swab specimens	
Garcia 2020 (B) (preprint) 63 participants (63 samples)	Patients admitted with a clinical and radiological diagnosis of pneumonia of unknown aetiology but RT-PCR-negative (n = 63) • non-COVID-19 cases not included Addional reported cohort extracted as Garcia 2020 (A)	Inpatient hospital (9 February-2 April)	67 years 47, 74%	Not stated	Clinical diagnosis of COVID-19 (no further detail); all PCR-negative	None reported
Hu 2020a (preprint) 211 participants (993 samples)	Confirmed COVID-19 patients (221) • non-COVID-19 cases not included	Inpatient; Chongqing, China (23 January-3 March)	Mean 47.8 years 135, 64%	Not stated 137, 62% with fever; 40, 19% severe	Chinese Government guidelines (version 6); included RT-PCR	None described; text states 993 samples but only 409 reported for IgM and 507 for IgG
Jia 2020 (preprint) 57 participants (57 samples)	1. RT-PCR confirmed (24) 2. Clinical diagnosis for RT-PCR negative (2 x negative results) according to Chinese Government guideline (6th ed) (33) • non-COVID-19 cases not included	Inpatients; Shenzhen, China (Not stated)	Not stated	Not stated	1. RT-PCR 2. Chinese CDC guideline (6th ed). (1 to 34 days from exposure to first PCR test)	None described
Li 2020a (accepted for publication and undergone full peer review) 525 participants	COVID-19 according to Chinese CDC guideline (5th ed) (525; 397 PCR-positive)) • non-COVID-19 cases not included	Potentially inpatient and outpatient; 6 provinces, China (Not stated)	Not stated	Not stated	Chinese CDC guideline (6th ed), including PCR; pharyngeal, sputum (Not stated)	None stated

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

(525 samples)						
Lippi 2020 [A] (published; letter) 48 participants (48 samples)	Participants with suspected COVID-19; subgroup of cases (48/131 patients) with available data on days post-symptom onset data can be included • non-COVID-19 cases not included	Inpatients; Verona, Italy (Not stated)	Totlal sample of 131: mean 56 years 60/131, 46%	Not stated	RT-PCR (Seegene Allplex 2019-nCoV Assay. OP, NP swabs (During hospitalisation)	Excluded 83 patients with no time pso data
Liu 2020c (preprint) 133 participants (133 samples)	Patients diagnosed with SARS-Cov-2 according to Chinese CDC guideline (5th ed) (133) • non-COVID-19 cases not included	Inpatients; Wuhan, China (17 February-1 March)	Moderate 67.5 years; severe 68 years; critical 70 years 70, 53%	Not stated moderate 44, 33%; severe 52, 39%; critical 37, 29%	Clinical diagnosis (seems to be Chinese CDC guideline, 5th ed) Includes RT-PCR (GeneoDx Biotech, Shanghai, China); 2 tests per participant; Table 2 refers to NP.	None described
Long 2020 (B) (preprint) 262 participants (363 samples)	RT-PCR-positive confirmed cases (n = 285). No further detail of inclusion or exclusion criteria. Additional cohort extracted as Long 2020 (A); some additional cohorts excluded (see Characteristics of included studies) • non-COVID-19 cases not included	Inpatients; Chongqing, China (38384)	47 years 158, 55.4%	103, 36% exposure to transmission sources 39, 14% severe or critical in ICU	RT-PCR; nasal and pharyngeal swabs (during hospital stay)	23 patients with no information on time pso were excluded leaving 363 samples from 262 patients
Padoan 2020 (peer reviewed; published) 37 participants (87 samples)	Hospitalised patients with confirmed COVID-19 (n = 37) • non-COVID-19 cases not included	Inpatients; Padova, Italy (18 March-26 March 2020)	Not stated	Not stated	RT-PCR; NP (Not stated)	None described

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Pan 2020a (peer reviewed; published) 105 participants (134 samples)	COVID-19 patients according to CDC guideline (5th ed); confirmed by PCR (67) or clinical diagnosis (37) • non-COVID-19 cases not included	Inpatients; Wuhan, China (Not stated (symptom onset 7 January-18 February))	58 years 48, 46%	Not stated	RT-PCR following WHO guidelines (BioGerm, Shanghai, China), Clinical diagnosis according to CDC guideline (5th ed); throat swabs (Not stated)	Data reported only for those with symptom onset information; 26 samples excluded
To 2020a [A] (peer reviewed; published) 23 participants (108 serum samples)	Confirmed COVID-19 patients from 2 hospitals (n = 23, can only extract data for 16 with > 14-day pso data) • non-COVID-19 cases not included	Hospital inpatient, Hong Kong (22 January-12 February)	Not stated 13/23 (57%) age: median 62 years (range 37–75)	Not stated 10/23 (43%) severe; 5/23(22%) admitted to ICU, 3/23(13%) required intubation, 2/23(9%) died Fever in 22/23 (96%) patients, cough in 5/23 (22%), chills in 4/23 (17%), dyspnoea in 4/23 (17%)	Laboratory-confirmed - not further described; NP or sputum (Unclear)	7/23 (30%) were not tested between days 14 and 30
Xiao 2020a (accepted manuscript; pre-proof) 34 participants (34 samples)	Confirmed cases of COVID-19 according to Chinese CDC (5th ed) (34) • non-COVID-19 cases not included	Inpatients; Wuhan, China (1-29 February)	49 years (review team estimated) 22, 65%	Not stated Not described	COVID-19 according to CDC diagnosis and treatment guideline (5th ed)	None reported

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Xie 2020a (accepted manuscript; pre-proof) 56 participants (56 samples)	Participants with suspected COVID-19 based on Chinese CDC (5th ed) criteria (n = 56, including 16 PCR confirmed) • non-COVID-19 cases not included	Inpatients; Wuhan, China (15-25 February 2020)	56.5 years 24, 43%	Not stated 34, 61% severe	[1] RT-PCR QIAamp RNA virus kit (Qiagen, Heiden, Germany); NP and throat [2] clinical diagnosis (guideline, 5th edition	None reported
Xu 2020a (preprint) 10 participants (10 samples)	Confirmed (PCR) COVID-19 cases (n = 10) • non-COVID-19 cases not included	Hospital inpatients; Shanghai, China (Not stated)	Not stated 6, 60%	Not stated 10, 100% required oxygen	RT-PCR (cycle threshold value (Ct) < 37 defined as positive and Ct ≥ 40 defined as negative; pharyngeal swab (Not stated)	None reported
Yongchen 2020 (peer reviewed; published) 21 participants (≥ 42 samples)	Participants with COVID-19 (n = 16) and asymptomatic carriers (n = 5) • non-COVID-19 cases not included	Mixed; Jiangsu, China (25 January-18 March 2020)	37 years 13, 62%	Not stated 5, 24% severe; 5, 24% asymptomatic cases Illness severity defined according to the Chinese management guideline for COVID-19 (version 6.0).	RT-PCR, confirmed after 2 sequential positive respiratory tract sample results; throat swabs	None described
Zhang 2020a (preprint) 222 participants (222 samples)	Confirmed COVID-19 patients (RT-PCR detection or antibody assay) (n = 222) • non-COVID-19 cases not included	Inpatients; Wuhan, China (admitted 13 January 13-1 March)	62 years Not stated	Not stated 87, 39% severe	RT-PCR or anti-SARS-CoV-2 assay ; nasal or pharyngeal swabs (Not stated)	None reported
Zhang 2020c (peer reviewed; published) 16 participants (16 samples)	RT-PCR-confirmed COVID-19 patients (n = 139); included those with around 10 days of medical treatment after admission (n = 16) • non-COVID-19 cases not included	Inpatients; Wuhan, China (Not stated)	Not stated	Not stated	RT-PCR	< 10 days' medical treatment (n = 123)

A&E: Accident and Emergency Department; **CDC:** Center for Disease Control; **CT:** computed tomography; **CGIA:** colloidal gold immunoassay; **D+:** disease positive: **D-:** disease negative; **ed:** edition; **ELISA:** enzyme-linked immunosorbent assay; **HCW:** healthcare worker; **ICU:** intensive care unit; **LFA:** lateral flow assay; **n:** number; **NP:** nasopharyngeal; **NR:** not reported; **OP:** oropharyngeal; **PCR:**

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

polymerase chain reaction; **pso:** post-symptom onset; **RNA:** ribonucleic acid; **RT-PCR:** reverse transcriptase polymerase chain reaction; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **suppl:** supplementary; **TB:** tuberculosis

Table B. Two-group studies or more estimating sensitivity and specificity

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study (source)	COVID-19 cases (n)	Non-COVID cases (n) (including method of verification)	Institution (Recruitment dates)	Age (median) n, % male	Exposure history Symptoms/severity	Reference details (cases)	Missing or uninterpretable data
Adams 2020 [A] (preprint) 182 participants (40 samples)	RT-PCR confirmed COVID-19 cases (n = 40)	Pre-pandemic controls (n = 142); prior to December 2019	Acute hospital (n = 16), recovering HCWs (n = 6), convalescent (n = 18); UK (Not stated)	57y Not stated	Not stated Asymptomatic (n = 1); mild (n = 26); severe (n = 4); critical (n = 9)	RT-PCR; nose/throat swabs (Not stated)	[B]–[J] tests evaluated in different numbers
Bendavid 2020 (preprint) 3481 samples participants (3324 samples)	COVID-19 cases were obtained from 3 different sources (n = 157 specimens) Confirmed cases from manufacturer data (n = 85); local cases (PCR- and ELISA-confirmed) (n = 37) or PCR-confirmed (6-10 days pso) (n = 35)	Non-COVID-19 cases were obtained from 13 different sources (n = 3324 specimens), Pre-pandemic (10 sources; n = 2811); pandemic era PCR-negative (n = 202); not stated (n = 311)	Multiple sources; USA, China, unclear (Not described)	Not stated	Not stated	PCR-positive only (n = 35); PCR and IgG or IgM confirmed by ELISA (n = 37); not stated (n = 85)	None described
Burbelo 2020 [A] (preprint) 67 participants (140 samples)	SARS-CoV-2 cases confirmed by PCR (n = 35 in results, n = 39 in methods)	Pre-pandemic blood donors (n = 32); prior to 2018 [Review authors excluded 3rd group with no reference standard reported (n = 10)]	Hospital (unclear whether inpatient or outpatient); San Diego, Seattle, Washington, USA (Not stated)	44 years 0.87	Not stated 13, 37% on a ventilator	RT-PCR; nasal and/or throat swabs (No information)	none described
Cai 2020 (preprint) 443 participants (443 samples)	RT-PCR confirmed (276)	Healthy, other controls; pre-December 2019 (167)	Inpatient (cases only); Chongqing, China (Not stated)	48 years 151, 55%	99, 36% known exposure	RT-PCR; no further details	None described

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Cassaniti 2020 (A) (published; letter) 60 participants (60 samples)	COVID-19-positive patients in ICU (n = 30) [Additional cohort reported in Cassaniti 2020 (B)]	Healthy volunteers with negative RT-PCR results (n = 30)	Infectious Diseases Unit or ICU, Tertiary hospital; Pavia, Italy (Not stated)	73.5 years 25, 42%	Not stated	RT-PCR detecting RNA polymerase and E genes; Respiratory samples (During patient care)	Weakly positive results counted as test positive
Chen 2020a (Accepted manuscript; peer reviewed, preproof) 19 participants (19 samples)	RT–PCR positive samples (n = 7)	RT–PCR-negative samples, but clinically suspicious for COVID-19 (n = 12) [Additional group of 'normal' samples (n = 51) used to derive threshold]	Unclear, presumably inpatients; Guangzhou, China (Not described)	Not stated	Not stated	RT–PCR; not stated (Not stated; prior to LFA)	None reported
Dohla 2020 (peer reviewed; published) 49 participants (49 samples)	[1] Attendees at community screening centre for COVID-19 (n = 12 PCR-positive), [2] Stored samples from 10 patients with confirmed diagnosis of COVID-19	[1] Attendees at community screening centre for COVID-19 (n = 27 PCR-negative)	Community screening centre [1] and unclear setting [2]; author institutions Bonn, Germany (Not stated)	46 years 25, 51%	Probable date of exposure identified in 22, 45% 5/49 (10%) asymptomatic. 71% dry cough; 65% fatigue; 46% runny nose (only %s reported)	[1] RT–qPCR (Altona Diagnostics) [2] RT–qPCR (unknown if same kit); throat swabs group [1]; not stated for group [2]. ([1] same time as index test. [2] not stated)	Weak signals counted as positive; no missing data reported
Freeman 2020 (preprint) 618 participants (618 samples)	Confirmed COVID-19 cases (n = 99)	Pre-pandemic healthy (n = 377) + other infection (n = 142)	Convalescent; USA (reference to CDC National Center for Immunization and Respiratory Diseases) (Not stated)	Not stated	Not stated	PCR; no further detail	None mentioned

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Garcia 2020 (A) (preprint) 100 participants (100 samples)	Suspected COVID-19 patients admitted to A&E; all RT-PCR-positive (n = 55) [Third cohort reported as Garcia 2020 (B)]	Pre-pandemic healthy controls (n = 45); 1 October-30 November, 2019	Inpatient; Madrid, Spain (1 March-6 April 2020)	63 years 33, 60%	Not stated	RT-PCR	None described
Grzelak 2020 [A] (preprint) 542 participants (652 samples)	Hospitalized COVID-19 patients (51) Review team excluded 2 additional cohorts with no reference standard (See COIS)	Pre-pandemic sera from healthy individuals (491)	Inpatient; Paris, France (Not stated)	Not described 47, 74%	Not stated	Not stated	None reported
Guo 2020a (accepted manuscript; corrected proof now available online) 275 participants (343 samples)	Confirmed (82) or probable (58) COVID-19 cases (provided 208 samples)	Pre-pandemic acute lower respiratory tract infection (135) Healthy individuals (150) used to define threshold	Inpatients; Wuhan and Beijing, China (cases) (43,831)	Not stated	Not stated Confirmed cases - 28, 34% severe Pobable cases - 5, 9% severe	Confirmed: deep sequencing or qPCR assay Probable: cases - clinical manifestation, chest X-ray and epidemiology but no virus detected by deep sequencing or qPCR; throat (Not stated)	None reported
Infantino 2020 (accepted publication; peer reviewed; preproof) 125 participants (125 samples)	[1] confirmed COVID-19 cases (n = 61)	[2] pre-pandemic (2018-19) control group with rheumatic and infectious diseases (n = 44) [3] blood donors (winter 2019) (n = 20)	Inpatient; Florence, Italy (Not stated)	mean 59 years 26, 43%	Not stated 30, 49% mild to moderate symptoms 31, 51% severe pneumonia requiring admission to ICU	RT-PCR (2 positive results required for confirmation); OP and NP swabs (Not stated)	None reported
Jin 2020 (peer reviewed; published)	Laboratory confirmed COVID-19 patients (n = 43)	COVID-19 suspects, discharged with 2 x RT-PCR-negative results with an interval of 24 h and who quarantined at home (n = 33)	Hospital inpatients; Hangzhou, China (January to 4 Mar 2020)	47 years 17, 40%	Not stated [1] COVID-19 patients: 27 (63%) fever;	RT-PCR; oral swab or sputum specimens	No data reported for 16 patients while PCR positive.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

76 participants (98 samples from 43 cases samples)	[Review team excluded results for 34 participants after becoming PCR-negative]				26 (61%) cough [2] Non-COVID-19 patients: 24/43 (73%) fever; 15/33 (46%) cough	(During hospital stay)	
Lassauniere 2020 [A] (preprint) 112 participants (112 samples)	COVID-19 PCR-positive patients (n = 30) admitted to intensive care	Pre-pandemic (n = 82) including blood donors (n = 10) and other infections (n = 72)	Intensive care; Hillerod, Denmark (Not stated)	Not stated	Not stated	Viral nucleic acid detection (no further detail)	Borderline results for tests [B] and [C] were considered test negative; for POC tests weak signals for IgM and IgG were considered positive. Some samples not tested with all assays.
Lin 2020a [A] (preprint) 159 participants (159 samples)	[1] Suspected COVID-19 cases (epidemiological risk, clinical features and RT-PCR respiratory specimen positive) from inpatient setting (specialised COVID-19 hospital) (n = 79)	RT-PCR negative controls (reportedly at least 3 x negative), including: [2] healthy volunteers; timing not reported, presumed contemporaneous (n = 29) [3] TB patients; timing not reported, presumed contemporaneous (n = 51)	Inpatients (specialised COVID hospital); Shenzhen, China (Not stated)	Not stated	Not stated	Epidemiological risk, clinical features and RT-PCR respiratory specimen positive' 'GeneoDX kit (Taqman RT-PCR method)	Only 65/79 D + and 64/80 D- serum samples available for ELISA; reason not given.
Liu 2020b (preprint) 358 participants (358 samples)	Confirmed (153) or suspected (85) COVID-19	Ordinary patients (70) and randomly sampled healthy blood donors (50); timing not reported, presumed to be contemporaneous	Inpatients; Hubei, China (6 -14 February)	55 years 138, 58%	Not stated Fever (87%); dry cough (54%); fatigue (33%). 235/238 (99%) had CT ground glass opac-	RT-PCR (Daan Gene) targeting ORF1ab and N gene (≤ 40 Ct); Clinical diagnosis according to Chinese Government-issued guideline (5th ed); pharyngeal swabs	None reported

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

					ity/patchy shadowing	RT-PCR sampling throughout inpatient stay	
Liu 2020d [A] (evaluation; accepted manuscript) 314 participants (314 samples)	RT-PCR-confirmed COVID-19 cases (n = 214)	Healthy blood donors, presumed to be contemporaneous (n = 100)	Inpatient, Hubei, China (18 January-26 February)	Not stated	Not stated	RT-PCR; pharyngeal swabs. Median 15 days pso (range 0–55 days)	None described
Lou 2020 [A] (preprint) 380 participants (380 samples)	Confirmed COVID-19 cases according to Chinese Government-issued guidelines (6th edition) (n = 80)	Healthy people enrolled from the community, presumed contemporaneous selection (n = 300)	inpatient; Hangzhou, China (19 January-9 February 2020)	Mean 55 years 0.61	26, 33% critical	CDC guideline (6th ed); criteria described including PCR; deep sputum samples' (On admission)	Not all control group participants were tested by all index tests (range 100-300/300)
Ma 2020a (preprint) 570 participants (216 samples from 87 cases samples)	Confirmed (PCR-positive) COVID-19 patients (n = 87)	[2] Pre-pandemic healthy donors (n = 330) [3] Contemporaneous 'other diseases' (no mention of PCR) (n = 138) [4] Suspected COVID pneumonia but negative PCR (n = 15)	Inpatient; Hefei, China (26 January-5 March 2020)	Not stated	Not stated 56, 67% clinically moderate 17 severe 5 critical "few mild" [page 7]	Chinese Government-issued guidelines (7th edition) including RT-qPCR; serum (During hospital admission as part of "routine clinical testing". Performed before index test)	For comparison of sensitivity and specificity of 2 antigens only 20/total of 479 control sera were used (20/138 from 'other disease' group)
Okba 2020c (accepted manuscript; early release) 54 participants (76 samples)	RT-PCR-confirmed SARS-CoV-2 cases (n = 9, 31 samples)	Contemporaneous healthy blood donors (n = 45)	Inpatient; Munich, Germany (occurred after 23 January, discovered (presume PCR-positive) on 27 January 27)	Not stated	All identified through exposure to known cases Not stated	RT-PCR; OP, NP (day 1-5 of symptoms)	Indeterminate or unclear index results on graphs considered negative by review team

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Qian 2020 (preprint) 2113 participants (2113 samples)	[1] Confirmed COVID-19 cases (RT-PCR-positive) (n = 503) and [2] suspected COVID-19 cases based on epidemiological history, clinical symptoms and chest X-ray but 3 x PCR-negative (n = 52)	Apparently contemporaneous controls, including: [3] hospitalised with non-COVID-19 conditions (PCR testing not described) (n = 972) [4] healthy controls (n = 586)	Hospital inpatients; Hubei and other provinces, China (Unclear)	Not stated	Not stated	RT-PCR; NP ("early onset of the symptoms of COVID-19")	None described
Wan 2020 [A] (preprint) 17 participants (36 samples)	SARS-Cov-2 positive cases confirmed by RT-PCR (n = 7, 26 samples)	Prepandemic sera (n = 5); plus controls SARS-Cov-2 negative on two occasions (n = 5)	Inpatients; Singapore (Not stated)	Not stated	Not stated	RT-PCR	not stated
Wang 2020a [A] (accepted manuscript) 86 participants (86 samples)	COVID-19 patients, meeting Chinese Government guideline criteria (14)	Contemporaneous patients with different pathogen infections and related chronic diseases with no clinical symptoms or imaging evidence of COVID-19 (no PCR testing reported) (72)	Inpatient; Nanchong, China (25 January-15 February)	Not stated	Not stated	Chinese CDC guideline (5th ed)	none described
Xiang 2020a [A] (preprint) 98 participants (ELISA samples) , 126 participants (LFA samples) , 81 participants (PCR samples)	COVID-19 patients according to WHO interim guidance (suppl data reports PCR results for a subgroup); (n = 63 for ELISA, n = 91 for GICA, some overlap of cases)	Contemporaneous healthy individuals (n = 35)	Inpatient; Wuhan, China (admitted 1-28 January; sampled 2-4 February)	ELISA 65 years; LFA 61 years ELISA 35, 56% male LFA 49, 54% male	Not stated ELISA 4, 6% severe LFA 4, 4%	WHO interim guidance (subgroup of 82 also have PCR results); (PCR using throat swabs) (Not stated (PCR at 6-37 days post-admission))	Not stated
Xiang 2020b (peer reviewed; published)	[1] RT-PCR confirmed cases (n = 85) [2] Suspected cases with COVID-19 pneumonia	[3] Contemporaneous control group of healthy blood donors (hospital staff) or patients with other diseases	Hospital patients (likely inpatients but not explicit);	51 years 31, 26%	Not stated 18/85 (21%) severe	[1] RT-PCR [2] Clinical manifestations and PCR ; NP and/or OP	Not stated

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

150 participants (216 samples from 85 cases samples)	manifestations and ≥ 2 negative RT-PCR (n = 24) classed as D+ for review purposes	in the same hospital (all PCR-negative) (n = 60)	Wuhan, China (19 January-2 March 2020)			(Unclear)	
Zeng 2020a (accepted manuscript; pre-proof) 63 participants (63 samples)	COVID-19 cases (n = 27); no details of confirmation process	Healthy controls, presume contemporaneous but not stated (n = 36)	Hospital inpatient; Wuhan, China (Not stated)	62 years 14, 52%	Not stated 17, 63% severe	No information; 'confirmed'; No information (No information)	None reported
Zhao 2020a (accepted manuscript; pre-proof) 386 participants (386 samples)	Confirmed RT-PCR positive COVID-19 cases (173)	Pre-pandemic healthy individuals (213)	Inpatients; Shenzhen, China (11 January-9 February)	48 years 84, 49%	126, 73% clear exposure 32, 18% critical	RT-PCR; respiratory (Not stated)	inadequate plasma samples for 2 IgM tests and 1 IgG test
Zhao 2020b (preprint) 481 participants (481 samples)	Hospitalised and/or recovered COVID-19 patients (n = 69)	Pre-pandemic 'normal' samples ("strong negatives"); presumed healthy (n = 257) Contemporaneous 'normal' samples ("negatives"); presumed healthy (n = 155)	Hospital (no detail); multiple author institutions, China (Not stated)	Not stated	Not stated	Not described; "hospitalized and/or recovered patients confirmed SARS-CoV-2 virus infection."	None reported
Zhong 2020 [A] (published; letter) 347 participants (347 samples)	PCR-positive COVID-19 patients (n = 47)	Pre-pandemic healthy controls (n = 300)	Not stated; China (Not described (symptom onset 15 January-13 February))	48 years 16, 34%	Not stated 11, 24% severe (6) or critical (5)	PCR	None reported

A&E: Accident and Emergency Department; **CDC:** Center for Disease Control; **COIS**: Characteristics of included studies table; **CT:** computed tomography; **CGIA:** colloidal gold immunoassay; **D+:** disease positive: **D-:** disease negative; **ed:** edition; **ELISA:** enzyme-linked immunosorbent assay; **HCW:** healthcare worker; **ICU:** intensive care unit; **LFA:** lateral flow assay; **n:** number; **NP:** nasopharyngeal; **NR:** not reported; **OP:** oropharyngeal; **PCR:** polymerase chain reaction; **pso:** post-symptom onset; **RNA:** ribonucleic

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

acid; **RT-PCR:** reverse transcriptase polymerase chain reaction; **RT-qPCR:** reverse transcriptase quantitative polymerase chain reaction; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **suppl:** supplementary; **TB:** tuberculosis;

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Appendix 9. Summary details of index tests per study

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Study	Test type	Index test (manufacturer)	Antigen	Antibodies measured (threshold)	Sample used	Index sample timing (days pso)	Data by time pso
Adams 2020 [A]	[A][a] Laboratory [B] to [J] LFAs	[A] ELISA (In-house) [B] to [J] name withheld	[A] tri S-based [B] to [J] details withheld	[A] IgG (> 0.4) and IgM (IgM > 0.07) (set in study) [B] and [C] not known [D] to [J] IgG and IgM (presumed from reported results)	Plasma	Day 4-62 (median and range per group: acute 10 (4 to 27); recovering HCW 13 (8 to 19); convalescent 48 (31 to 62))	Yes; per week
Bendavid 2020	LFA	No details (Premier Biotech, Minneapolis, MN))	Not specified	IgG, IgM (threshold not specified)	Serum, plasma, fingerstick blood, venous whole blood	Not described	No
Burbelo 2020 [A]	Laboratory	LIPS (in-house)	[A] N-based [B] S-based	Appears to be total Ab (threshold set in healthy control sample)	plasma or serum	Day 2-50	Yes; ≤ 14 d, and > 14 d
Cai 2020	Laboratory	CLIA (in-house)	S-based	IgM, IgG (both ≥ 0.7 CL)	Serum (day 2-27 pso)	Day 2-27	No
Cassaniti 2020 (A)	LFA	CGIA: VivaDiag COVID-19 IgM/IgG (VivaChek)	Not stated	IgM, IgG (visible line)	Serum or whole blood	On presentation at A&E	No
Cassaniti 2020 (B)	LFA	CGIA: VivaDiag COVID-19 IgM/IgG (VivaChek)	Not stated	IgM, IgG (visible line)	Serum or blood	Median 7 days (IQR 4 to 11) after first test	No
Chen 2020a	LFA	FIA (in-house; using lanthanide-doped polystyrene nanoparticles)	N-based	IgG (threshold: At (florescence peak of test line)/Ac (florescence peak of control line) ratio (R) > 0.0666)	Serum	Not stated	No
Dohla 2020	LFA	CGIA (suspect this is a description of an anonymised test; no manufacturer stated)	SARS-CoV-2 antigen	IgG/IgM (weakly visible or clearly visible (strong positive) test line)	Fingerprick blood (n = 39 in cohort [1]);	Median time from exposure–to–test	No

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

					stored serum for cohort [2]	18.5 d (IQR 15 to 24)	
Du 2020	Laboratory	Not stated; coded as CLIA based on reported threshold in AU/mL (Manufacturer not reported)	Not stated	IgM, IgG (threshold > 10 AU/mL)	Not stated	day 22 to > 35	Yes; by week from day 22
Freeman 2020	Laboratory	ELISA (in-house)	S-based	IgG and IgM (based on optical density signal)	Serum	All day ≥ 10	No
Gao 2020a	LFA	CGIA (Innovita Biological Technology Co)	Not reported	IgG, IgM (coloured line)	Serum	day 0 to > 14	Yes; by week from day 22
Gao 2020b [A]	[A] Laboratory [B] CGIA [C] Laboratory	[A] CLIA [B] CGIA [C] ELISA (all Beier Bioengineering Company, Beijing)	[A], [B], and [C] all S- and N-based	IgG and IgM ([A] ≥ 8 arbitrary unit (AU)/mL; [B] visible line; [C] method to calculate threshold reported)	Serum	Day 1-24	Yes; by week
Garcia 2020 (A)	LFA	CGIA, AllTest COV-19 IgG/IgM kit (AllTest Biotech, Hangzhou, China)	Not reported	IgG, IgM (visible line for either)	Serum	Day 0 to ≥ 14	Yes; by week
Garcia 2020 (B)	LFA	CGIA, AllTest COV-19 IgG / IgM kit (AllTest Biotech, Hangzhou, China))	Not reported	IgG and IgM (visible line for either)	Serum	Day 8 to ≥ 14	Yes; by week
Grzelak 2020 [A]	[A] to [E] all Laboratory	5 tests evaluated: [A] and [B] LIPS (in-house) [C] and [E] ELISA [D] S-flow	[A] S1-based [B] and [C] N-based [D] S-based [E] tri-S-based	a. IgG b. total Ab c. IgM or IgG d. total Ab (Not clearly stated, plotted on Figure 1)	Serum	Not stated; day 2-18 for 5 patients	No
Guo 2020a	Laboratory	In-house ELISA	N-based	IgM, IgG, IgA (threshold set in healthy control sample)	Blood/plasma	Day 1-39	Yes; week 1 only
Hu 2020a	Laboratory	Magnetic MCLIA kit (Bioscience Co., Ltd (Chongqing, China))	N- and S-based	IgM, IgG (S/CO ≥ 1.0 considered positive (ratio of the chemiluminescence signal to the cut-off value)	Serum	Day 1 to > 37	Yes; by week
Infantino 2020	Laboratory	SARS CoV-2 IgM and IgG CLIA kits (Shenzhen YHLO Biotech Co)	N- and S-based	IgM, IgG (multiple thresholds reported, including manufac-	Blood (discussion mentions serum)	Day 8-19	No

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

				turer recommended threshold ≥ 10 AU/mL)			
Jia 2020	LFA	FIA method (Beijing Diagreat Biotechnologies)	Not described	IgM (≥ 0.88 Flu) IgG (≥ 1.02 Flu) (threshold set in healthy control sample)	Not stated	Not stated	No
Jin 2020	Laboratory	SARS CoV-2 IgM and IgG CLIA kits (Shenzhen YHLO Biotech Co)	N- and S-based	IgM, IgG (> 10 AU/mL)	Serum	Day 1-55	Yes; by week
Lassauniere 2020 [A]	[A] to [C] laboratory, [D] to [I] LFA	[A] ELISA (Beijing Wantai) [B] IgG ELISA (EUROIMMUN) [C] IgA ELISA ELISA (EUROIMMUN) [D] to [F] all presumed to be CGIA [D] Dynamiker Biotech 2019-nCOV IgG/IgM Rapid Test [E] CTK Biotech - OnSiteTM COV-ID-19 IgG/IgM Rapid Test [F] Autobio Diagnostics Anti-SARS-CoV-2 Rapid Test [G] Artron Labs Coronavirus Diseases 2019 (COVID-19) IgM/IgG Antibody Test [H] Acro Biotech 2019-nCoV IgG/IgM Rapid Test Cassette [I] Hangzhou All test 2019-nCoV IgG/IgM Rapid Test Cassette	[A] S-based [B] and [C] S1-based [D] to [I] not stated	[A] Total Ab (calculated negative control value to 0.160) [B] IgG and [C] IgM (ratio < 0.8 is considered negative, ≥ 0.8 and < 1.1 borderline, and ≥ 1.1 positive) [D] to [I] IgG/IgM (Visual line change)	Serum	Day 7 to ≥ 21	Yes
Li 2020a	LFA	CGIA (Jiangsu Medomics Medical Technologies)	S-based	IgM, IgG (coloured line)	Serum, plasma	Not stated; for 1 site (n = 58), sampling day 8-33	No
Lin 2020a [A]	[A] and [B] laboratory	[A] In-house CLIA [B] ELISA (Darui Biotech, China)	[A] and [B] N-based	[A] IgM (RLU 162296); IgG (RLU 336697) (threshold set using ROC analysis) [B] IgM, IgG	Serum	Day 0 to ≥ 14	Yes; by week
Lippi 2020 [A]	[A] and [B] laboratory	[A] MAGLUMI 2019-nCoV CLIAs (Snibe Diagnostics -Shenzhen New Industries Biomedical Engineering Co., Ltd,)	[A] N- and S-based [B] Not stated	[A] IgM or IgG (≥ 1.10 AU/mL) [B] IgA or IgG (≥ 1.1 (absorbance of patient sample/absorbance of calibrator))	[A] Serum or plasma [B] Not stated	Day < 5-21	Yes; 5 day intervals

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

		[B] ELISAs (Euroimmun AG, Lübeck, Germany)					
Liu 2020a	LFA	CGIA (Not stated: 'Chinese biotechnology company')	Not stated	IgG, IgM (visible line)	Serum	Day 0 to ≥ 14	Yes; by week
Liu 2020b	Laboratory	ELISA kit (Lizhu, Zhuhai, China)	N-based	IgM, IgG (threshold set in healthy control sample)	Serum	Day 0 to ≥ 16	Yes; 5-day intervals
Liu 2020c	Laboratory	iFLash-SARS-CoV-2 CLIA (Shenzhen YHLO Biotech) [based on company contact]	Not described	IgM, IgG (not stated)	Serum	Not stated	No
Liu 2020d [A]	Laboratory	[A] ELISA (Hotgen, Beijing, China) [B] ELISA (Lizhu, Zhuhai, China)	[A] S-based [B] N-based	IgM, IgG (threshold not stated but method of calculation reported)	Serum	Day 0-30	Yes; unequal intervals
Long 2020 (A)	Laboratory	Magnetic CLIA (Bioscience (Chongqing) Co., Ltd)	N- and S-based	IgM, IgG (threshold not stated)	Serum	Not stated; 21-31 days after PCR test	No
Long 2020 (B)	Laboratory	Magnetic CLIA (Bioscience (Chongqing) Co., Ltd)	N- and S-based	IgM, IgG (threshold not described)	Serum	Day 2 to ≥ 23	Yes; by week
Lou 2020 [A]	[A] and [C] laboratory [B] LFA	[A] ELISA (Beijing Wantai) [B] CGIA (Beijing Wantai) [C] CLIA (Xiamen InnoDx)	[A] N- and S-based [B] and [C] not stated	IgG, IgM, Ab (thresholds as per manufacturer; NR)	Serum	Day 0-29	Yes; by week
Ma 2020a	Laboratory	CLIA (in-house)	S-based (RBD)	IgM, IgG, IgA (ROC analysis to determine optimal cut-off in RLU, which is not stated	Serum	Day 4-41	Yes; 5-day intervals
Okba 2020a	Laboratory	ELISA, beta version (EUROIMMUN)	Not stated	IgA, IgG IgM, IgG (threshold not stated but method of calculation reported)	Serum	Day 3 to > 23	Yes; by week
Padoan 2020	Laboratory	CLIA - MAGLUMI 2000 Plus nCoV (Snibe Diagnostics)	Not stated	IgM (1.0 AU/mL); IgG (1.1 AU/mL)	Serum	Day 0 to ≥ 13	Yes; by week
Pan 2020a	LFA	CGIA (Zhuhai Livzon Diagnositic Inc)	Not described	IgM, IgG (appearance of T line)	Serum or plasma	Day 1 to ≥ 15	Yes; by week

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Paradiso 2020a	LFA	VivaDiag (Jiangsu Medomics Medical Technologies) [VivaChek?]	S-based	IgM, IgG (both indicated by presence of red/purple line)	Venous blood	Day 0 to > 15	No
Qian 2020	Laboratory	CLIA (states analysed using fully automated immune analyser from Shenzhen YHLO Biotech Co)	N- and S-based	IgM and IgG (RLU ≥ 10 AU/mL)	Serum	Not stated	Patients
To 2020a [A]	Laboratory	EIAs (in-house, considered with ELISA tests for analysis purposes)	[A] N-based [B] S-based	IgG, IgM (set as the mean value of 93 anonymous archived serum specimens from 2018, plus 3 SDs)	Used serum remnant from blood samples taken for routine biochemical testing	Day ≥ 14 (for subgroup with 2x2 data)	Samples
Wan 2020 [A]	[A] and [B] laboratory	[A] IIFT (EUROIMMUN) [B] In-house ELISA	[A] and [B] both SARS-CoV	a. Total antibody (≥ 400) b. IgM, IgG (threshold not stated)	Serum	Day 3-24	Yes; per week
Wang 2020a [A]	[A] Laboratory [B] LFA	[A] ELISA (Beijing Hotgen Biotechnology Co) [B] CGIA (Beijing Hotgen Biotechnology Co)	Not stated	IgM ([A] not stated; [B] coloured line)	Serum	Day 3-7	Yes (week 1 only)
Xiang 2020a [A]	[A] Laboratory [B] LFA	[A] ELISA (Zhu Hai Livzon Diagnostics) [B] CGIA (Zhu Hai Livzon Diagnostics)	Not stated	IgM, IgG ([A] threshold not stated; [B] coloured line)	[A] Serum, [B] Plasma	Not stated (can be estimated as 5-35 days post-admission)	No
Xiang 2020b	Laboratory	ELISA (ELISA kits, Zuhai Livzon Inc)	N-based	IgG, IgM (method to calculate threshold reported	Serum	day 0 to > 21	Yes; per week
Xiao 2020a	Laboratory	CLIA (Shenzhen YHLO Biotechnology Co. Ltd)	Not described	IgM, IgG (≤ 10 AU/mL)	Blood	Day 1-49	Yes; per week
Xie 2020a	Laboratory	CLIA (Shenzhen YHLO Biological Technology)	N- and S-based	IgG, IgM (≥ 10 AU/mL)	Serum	Day 0-41	No
Xu 2020a	LFA	CGIA (in-house)	S-based	IgG, IgM (coloured line)	Not stated	Day 15-30 of observation	No

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Yongchen 2020	LFA	CGIA (Innovita Co. Ltd, China)	N- and S-based	IgG, IgM (coloured line)	Serum	Day 8-42	Yes; by week
Zeng 2020a	Laboratory	ELISA (Zhuhai Livzon Diagnostics)	Not stated	IgG and IgM (OD = 0.105)	Serum	Day 3-39; can extract for day 6 only	Yes; week 1 only
Zhang 2020a	Laboratory	CLIA - iFlash-SARS-CoV-2 IgG and iFlash-SARS-CoV-2 (Shenzhen YHLO Biotech Co. Ltd.)	Not described	IgM, IgG (threshold not described)	Serum	Day 1-35	No
Zhang 2020b	Laboratory	CLIA - iFlash-SARS-CoV-2 (Shenzhen YHLO Biotechnology Co Ltd) [derived from company contact]	N- and S-based	IgM, IgG (> 10.0 AU/mL); AU - antibody concentration per mL	Serum (frozen until analysis)	Day 4-18	No
Zhang 2020c	Laboratory	ELISA (in-house; anti-SARSr-CoV)	N-based (SARS-CoV)	IgM, IgG (threshold not described)	Serum	Day 0 and day 5	Yes; week 1 only
Zhang 2020d	LFA	CGIA (in-house)	S-based	Total antibodies (IgM, IgG) (Visible test and control lines)	Serum	Not stated	No
Zhao 2020a	Laboratory	ELISA (Shenzhen YHLO Biotech Co)	N- and S-based	Ab, IgM, IgG (Not stated)	Plasma	Day 1-39	Yes; week 1, 2 and 3+
Zhao 2020b	Laboratory	ELISA (in-house)	S1-based	Total antibodies (IgG or IgM) (threshold calculation method reported)	Plasma	Not stated; n = 45 during week 1	No
Zhong 2020 [A]	Laboratory	[A] and [B] in-house ELISA [C] CLIA (author institution is Maccura Biotech)	[A] N-based [B] S-based [C] N- and S-based (unclear)	IgM, IgG (optimal cut-off based on ROC analysis)	Serum	Day 1-29	No

A&E: Accident and Emergency Department; **Ab:** antibody; **AU:** arbitrary units; **CGIA:** colloidal gold immunoassay; **CL:** chemilumonescence units; **CLIA:** chemiluminescence immunoassay; **d:** days; **ELISA:** enzyme-linked immunosorbent assay; **FIA:** fluorescence immunoassay; **Flu:** fluorescence units; **HCW:** healthcare workers; **IIFT:** indirect immunofluorescence assay; **IQR:** interquartile range; **LFA:** lateral flow assay; **LIPS:** luciferase Immunoprecipitation System; **mL:** millilitre; **N-based:** nucleocapsid protein; **NR:** not reported; **OD**: Optical density; **pso:** post-symptom onset; **RBD:** receptor binding domain; **RLU:** relative light units; **ROC:** receiver operating characteristics; **S-based:** spike protein; **SD:** standard deviation; **S-flow:** flow-cytometry based test; **SARS-CoV-2:** severe acute respiratory syndrome coronavirus 2; **SD:** standard deviation

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Footnotes


[a]Please note that square brackets indicate different tests within one study.

Appendix 10. Study level assessments of study quality

Figure 10


Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 10. Risk of bias and applicability concerns summary: review authors' judgements about each domain for each included study

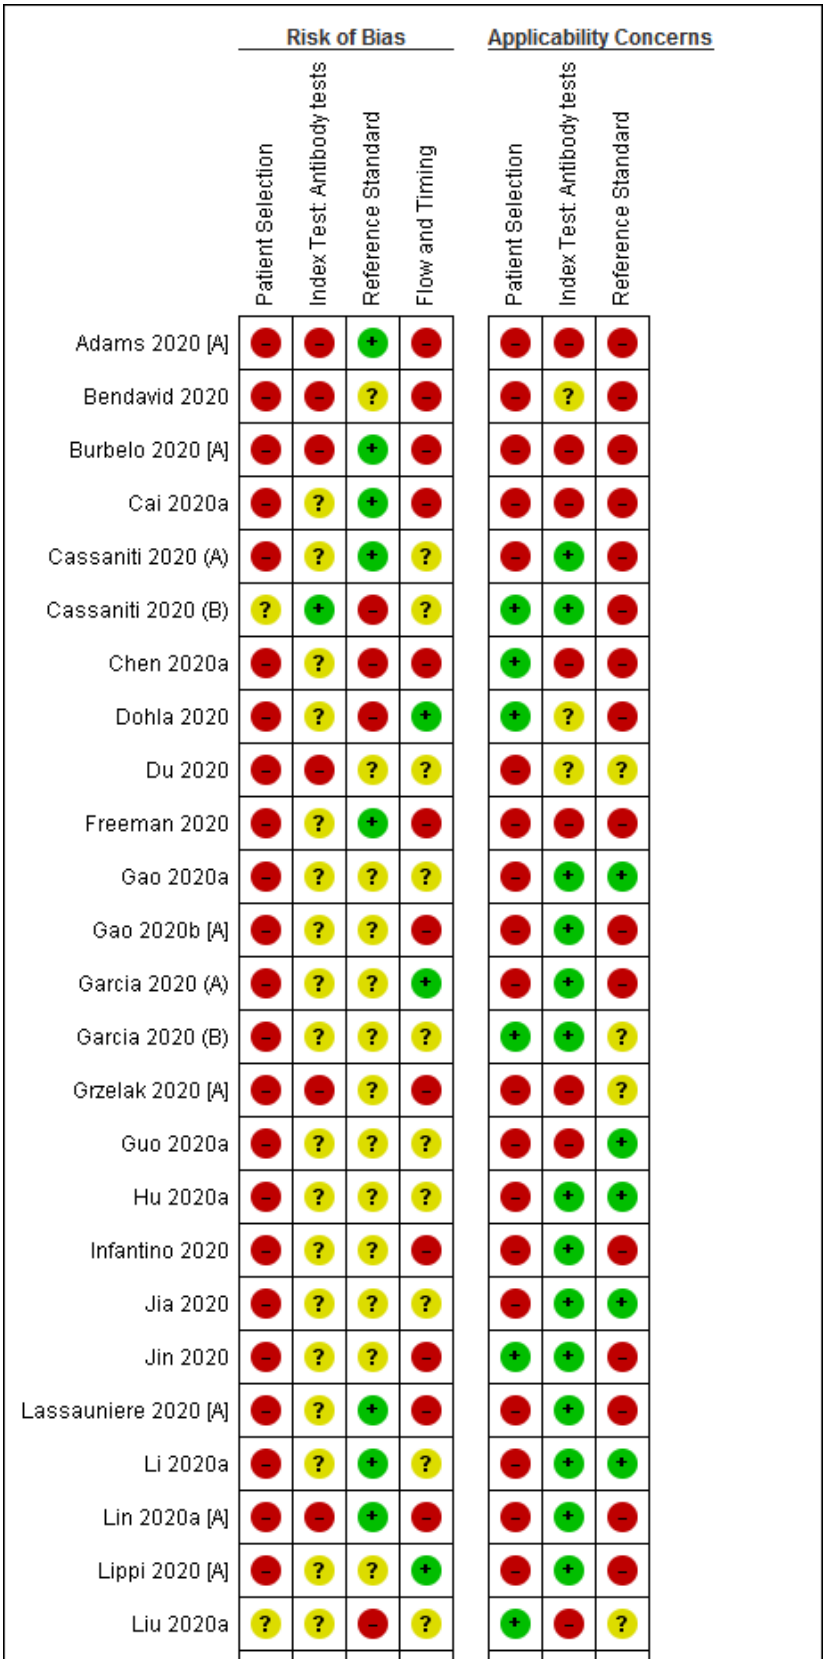

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 10. (Continued)

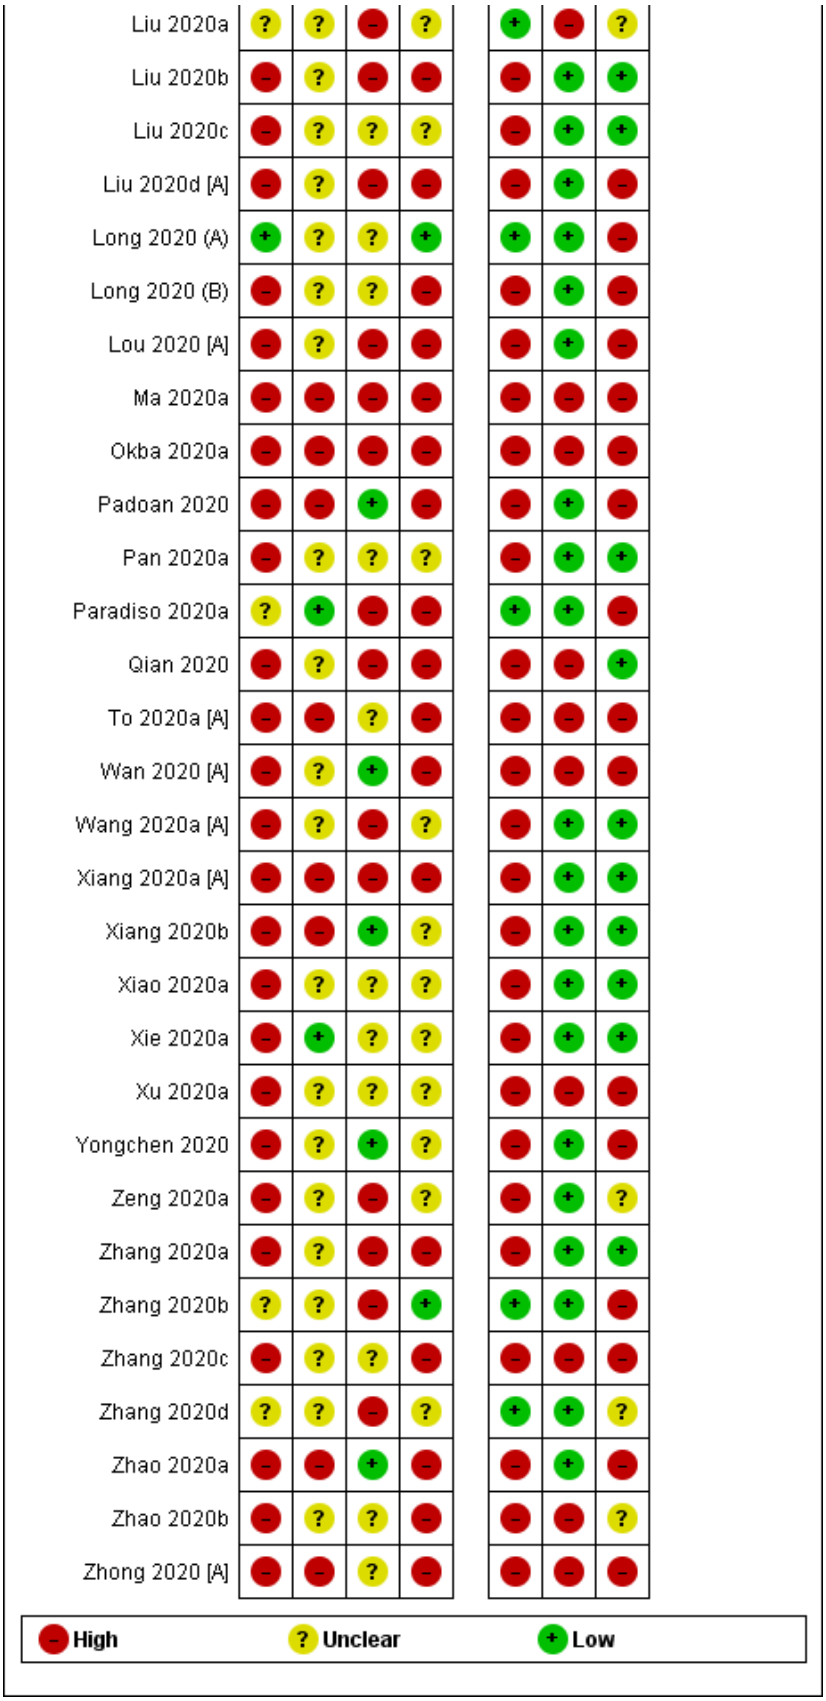

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Appendix 11. Results of all studies across all time periods

Figure 11

Figure 11. Forest plot of studies evaluating tests for detection of IgG at all time post-symptom onset

Study	TP	FP	FN	TN	Setting	Reference standard (cases)	Reference standard (non-cases)	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	34	0	6	50	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	ELISA	0.85 [0.70, 0.94]	1.00 [0.93, 1.00]
Adams 2020 [D]	21	2	12	58	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.64 [0.45, 0.80]	0.97 [0.88, 1.00]
Adams 2020 [E]	25	1	13	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.66 [0.49, 0.80]	0.98 [0.91, 1.00]
Adams 2020 [F]	18	1	13	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.58 [0.39, 0.75]	0.98 [0.91, 1.00]
Adams 2020 [G]	17	0	14	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.55 [0.36, 0.73]	1.00 [0.94, 1.00]
Adams 2020 [H]	20	2	13	58	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.61 [0.42, 0.77]	0.97 [0.88, 1.00]
Adams 2020 [I]	15	0	17	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.47 [0.29, 0.65]	1.00 [0.94, 1.00]
Adams 2020 [J]	17	0	23	142	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.42 [0.27, 0.59]	1.00 [0.97, 1.00]
Cai 2020a	197	0	79	167	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.71 [0.66, 0.77]	1.00 [0.98, 1.00]
Cassaniti 2020 (A)	24	0	6	30	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CGIA	0.80 [0.61, 0.92]	1.00 [0.88, 1.00]
Cassaniti 2020 (B)	5	0	33	12	Hospital A&E	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CGIA	0.13 [0.04, 0.28]	1.00 [0.74, 1.00]
Chen 2020a	7	1	0	11	Unclear	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	FIA	1.00 [0.59, 1.00]	0.92 [0.62, 1.00]
Du 2020	60	0	0	0	Hospital in-patient	Unclear		CLIA	1.00 [0.94, 1.00]	Not estimable
Freeman 2020	94	0	5	0	Unclear	All RT-PCR+ve	Pre-pandemic healthy+other disease	ELISA	0.95 [0.89, 0.98]	Not estimable
Gao 2020a	35	0	3	0	Hospital in-patient	China criteria including RT-PCR -ves		CGIA	0.92 [0.79, 0.98]	Not estimable
Gao 2020b [A]	19	0	18	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.51 [0.34, 0.68]	Not estimable
Gao 2020b [B]	19	0	18	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.51 [0.34, 0.68]	Not estimable
Gao 2020b [C]	24	0	13	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.65 [0.47, 0.80]	Not estimable
Garcia 2020 (A)	23	0	32	45	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	CGIA	0.42 [0.29, 0.56]	1.00 [0.92, 1.00]
Garcia 2020 (B)	56	0	7	0	Hospital in-patient	Other criteria		CGIA	0.89 [0.78, 0.95]	Not estimable
Grzelak 2020 [C]	127	23	34	468	Hospital in-patient	Unclear	Pre-pandemic healthy	ELISA	0.79 [0.72, 0.85]	0.95 [0.93, 0.97]
Guo 2020a	162	0	46	135	Hospital in-patient	Other criteria including RT-PCR -ves	Pre-pandemic other disease	ELISA	0.78 [0.72, 0.83]	1.00 [0.97, 1.00]
Infantino 2020	44	0	17	64	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.72 [0.59, 0.83]	1.00 [0.94, 1.00]
Jia 2020	31	0	26	0	Hospital in-patient	China criteria including RT-PCR -ves		FIA	0.54 [0.41, 0.68]	Not estimable
Jin 2020	24	3	3	30	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CLIA	0.89 [0.71, 0.98]	0.91 [0.76, 0.98]
Lassauniere 2020 [B]	20	3	10	79	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	ELISA	0.67 [0.47, 0.83]	0.96 [0.90, 0.99]
Li 2020a	280	0	117	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.71 [0.66, 0.75]	Not estimable
Lin 2020a [A]	65	2	14	78	Hospital in-patient	All RT-PCR+ve	Current healthy+other disease (RT-PCR-ve)	CLIA	0.82 [0.72, 0.90]	0.97 [0.91, 1.00]
Lin 2020a [B]	15	0	50	64	Hospital in-patient	All RT-PCR+ve	Current healthy+other disease (RT-PCR-ve)	ELISA	0.23 [0.14, 0.35]	1.00 [0.94, 1.00]
Lippi 2020 [A]	19	0	29	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.40 [0.26, 0.55]	Not estimable
Lippi 2020 [B]	7	0	41	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.15 [0.06, 0.28]	Not estimable
Liu 2020a	77	5	18	79	Hospital in-patient	Other criteria including RT-PCR -ves	COVID suspects (single RT-PCR-ve)	CGIA	0.81 [0.72, 0.88]	0.94 [0.87, 0.98]
Liu 2020b	168	2	70	118	Hospital in-patient	China criteria including RT-PCR -ves	Current healthy+other disease (untested)	ELISA	0.71 [0.64, 0.76]	0.98 [0.94, 1.00]
Liu 2020c	129	0	4	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.97 [0.92, 0.99]	Not estimable
Liu 2020d [A]	150	0	64	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.70 [0.63, 0.76]	1.00 [0.96, 1.00]
Liu 2020d [B]	159	0	55	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.74 [0.68, 0.80]	1.00 [0.96, 1.00]
Long 2020 (B)	287	0	76	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.79 [0.75, 0.83]	Not estimable
Lou 2020 [A]	71	0	9	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.89 [0.80, 0.95]	1.00 [0.96, 1.00]
Lou 2020 [B]	69	1	11	208	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	CGIA	0.86 [0.77, 0.93]	1.00 [0.97, 1.00]
Ma 2020a	209	1	7	482	Hospital in-patient	All RT-PCR+ve	Mixed	CLIA	0.97 [0.93, 0.99]	1.00 [0.99, 1.00]
Okba 2020a	11	0	20	45	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.35 [0.19, 0.55]	1.00 [0.92, 1.00]
Padoan 2020	57	0	13	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.81 [0.70, 0.90]	Not estimable
Pan 2020a	60	0	48	0	Hospital in-patient	China criteria including RT-PCR -ves		CGIA	0.56 [0.46, 0.65]	Not estimable
Qian 2020	531	30	24	1528	Hospital in-patient	China criteria including RT-PCR -ves	Current healthy+other disease (untested)	CLIA	0.96 [0.94, 0.97]	0.98 [0.97, 0.99]
To 2020a [A]	15	0	1	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.94 [0.70, 1.00]	Not estimable
To 2020a [B]	16	0	0	0	Hospital in-patient	All RT-PCR+ve		ELISA	1.00 [0.79, 1.00]	Not estimable
Wan 2020 [A]	6	0	1	10	Hospital in-patient	All RT-PCR+ve	Mixed	IIFT	0.86 [0.42, 1.00]	1.00 [0.69, 1.00]
Wang 2020a [A]	14	22	0	50	Hospital in-patient	China criteria including RT-PCR -ves	Current other disease (untested)	ELISA	1.00 [0.77, 1.00]	0.69 [0.57, 0.80]
Xiang 2020a [A]	52	0	11	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	ELISA	0.83 [0.71, 0.91]	1.00 [0.90, 1.00]
Xiang 2020a [B]	74	0	17	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	CGIA	0.81 [0.72, 0.89]	1.00 [0.90, 1.00]
Xiang 2020b	72	3	18	57	Hospital in-patient	Other criteria including RT-PCR -ves	Current healthy+other disease (RT-PCR-ve)	ELISA	0.80 [0.70, 0.88]	0.95 [0.86, 0.99]
Xiao 2020a	32	0	2	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.94 [0.80, 0.99]	Not estimable
Xie 2020a	56	0	0	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	1.00 [0.94, 1.00]	Not estimable
Xu 2020a	3	0	7	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.30 [0.07, 0.65]	Not estimable
Zeng 2020a	0	0	27	36	Hospital in-patient	Unclear	Current healthy (untested)	ELISA	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]
Zhang 2020a	219	0	3	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.99 [0.96, 1.00]	Not estimable
Zhang 2020b	3	1	0	224	Hospital out-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CLIA	1.00 [0.29, 1.00]	1.00 [0.98, 1.00]
Zhang 2020c	13	0	3	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.81 [0.54, 0.96]	Not estimable
Zhao 2020a	112	2	61	195	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.65 [0.57, 0.72]	0.99 [0.96, 1.00]
Zhong 2020 [A]	46	1	1	299	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.98 [0.89, 1.00]	1.00 [0.98, 1.00]
Zhong 2020 [B]	45	43	2	257	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.96 [0.85, 0.99]	0.86 [0.81, 0.89]
Zhong 2020 [C]	45	10	2	290	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	CLIA	0.96 [0.85, 0.99]	0.97 [0.94, 0.98]

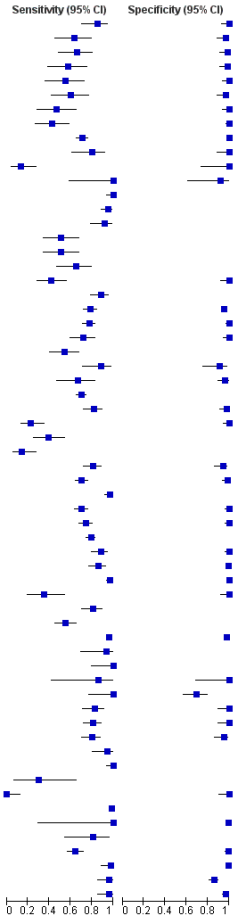


Figure 12;

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 12. Forest plot of studies evaluating tests for detection of IgM at all time post-symptom onset

Study	TP	FP	FN	TN	Setting	Reference standard (cases)	Reference standard (non-cases)	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	28	0	12	50	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	ELISA	0.70 [0.53, 0.83]	1.00 [0.93, 1.00]
Adams 2020 [D]	3	0	30	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.09 [0.02, 0.24]	1.00 [0.94, 1.00]
Adams 2020 [E]	2	0	36	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.05 [0.01, 0.18]	1.00 [0.94, 1.00]
Adams 2020 [F]	15	1	16	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.48 [0.30, 0.67]	0.98 [0.91, 1.00]
Adams 2020 [G]	14	1	17	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.45 [0.27, 0.64]	0.98 [0.91, 1.00]
Adams 2020 [H]	17	1	16	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.52 [0.34, 0.69]	0.98 [0.91, 1.00]
Adams 2020 [I]	14	0	18	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.44 [0.26, 0.62]	1.00 [0.94, 1.00]
Adams 2020 [J]	15	4	25	138	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.38 [0.23, 0.54]	0.97 [0.93, 0.99]
Cai 2020a	158	0	118	167	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.57 [0.51, 0.63]	1.00 [0.98, 1.00]
Cassaniti 2020 (A)	25	0	5	30	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CGIA	0.83 [0.65, 0.94]	1.00 [0.88, 1.00]
Cassaniti 2020 (B)	6	1	32	11	Hospital A&E	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CGIA	0.16 [0.06, 0.31]	0.92 [0.62, 1.00]
Du 2020	47	0	13	0	Hospital in-patient	Unclear		CLIA	0.78 [0.66, 0.88]	Not estimable
Freeman 2020	75	0	24	0	Unclear	All RT-PCR+ve	Pre-pandemic healthy+other disease	ELISA	0.76 [0.66, 0.84]	Not estimable
Gao 2020a	19	0	19	0	Hospital in-patient	China criteria including RT-PCR -ves		CGIA	0.50 [0.33, 0.67]	Not estimable
Gao 2020b [A]	14	0	23	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.38 [0.22, 0.55]	Not estimable
Gao 2020b [B]	19	0	18	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.51 [0.34, 0.68]	Not estimable
Gao 2020b [C]	11	0	26	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.30 [0.16, 0.47]	Not estimable
Garcia 2020 (A)	12	0	43	45	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	CGIA	0.22 [0.12, 0.35]	1.00 [0.92, 1.00]
Garcia 2020 (B)	25	0	38	0	Hospital in-patient	Other criteria		CGIA	0.40 [0.28, 0.53]	Not estimable
Guo 2020a	188	0	20	135	Hospital in-patient	Other criteria including RT-PCR -ves	Pre-pandemic other disease	ELISA	0.90 [0.86, 0.94]	1.00 [0.97, 1.00]
Infantino 2020	46	4	15	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.75 [0.63, 0.86]	0.94 [0.85, 0.98]
Jia 2020	39	0	18	0	Hospital in-patient	China criteria including RT-PCR -ves		FIA	0.68 [0.55, 0.80]	Not estimable
Jin 2020	13	0	14	33	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CLIA	0.48 [0.29, 0.68]	1.00 [0.89, 1.00]
Li 2020a	328	0	69	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.83 [0.79, 0.86]	Not estimable
Lin 2020a [A]	65	15	14	65	Hospital in-patient	All RT-PCR+ve	Current healthy+other disease (RT-PCR-ve)	CLIA	0.82 [0.72, 0.90]	0.81 [0.71, 0.89]
Lin 2020a [B]	30	14	35	50	Hospital in-patient	All RT-PCR+ve	Current healthy+other disease (RT-PCR-ve)	ELISA	0.46 [0.34, 0.59]	0.78 [0.66, 0.87]
Lippi 2020 [A]	6	0	42	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.13 [0.05, 0.25]	Not estimable
Liu 2020a	35	5	60	79	Hospital in-patient	Other criteria including RT-PCR -ves	COVID suspects (single RT-PCR-ve)	CGIA	0.37 [0.27, 0.47]	0.94 [0.87, 0.98]
Liu 2020b	167	3	71	117	Hospital in-patient	China criteria including RT-PCR -ves	Current healthy+other disease (untested)	ELISA	0.70 [0.64, 0.76]	0.97 [0.93, 0.99]
Liu 2020c	105	0	28	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.79 [0.71, 0.86]	Not estimable
Liu 2020d [A]	146	0	68	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.68 [0.62, 0.74]	1.00 [0.96, 1.00]
Liu 2020d [B]	165	0	49	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.77 [0.71, 0.83]	1.00 [0.96, 1.00]
Long 2020 (B)	243	0	120	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.67 [0.62, 0.72]	Not estimable
Lou 2020 [A]	74	0	6	300	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.93 [0.84, 0.97]	1.00 [0.99, 1.00]
Lou 2020 [B]	71	4	9	205	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	CGIA	0.89 [0.80, 0.95]	0.98 [0.95, 0.99]
Lou 2020 [C]	69	2	11	298	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	CLIA	0.86 [0.77, 0.93]	0.99 [0.98, 1.00]
Ma 2020a	209	37	7	446	Hospital in-patient	All RT-PCR+ve	Mixed	CLIA	0.97 [0.93, 0.99]	0.92 [0.90, 0.95]
Padoan 2020	44	0	26	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.63 [0.50, 0.74]	Not estimable
Pan 2020a	56	0	52	0	Hospital in-patient	China criteria including RT-PCR -ves		CGIA	0.52 [0.42, 0.62]	Not estimable
Qian 2020	470	29	85	1529	Hospital in-patient	China criteria including RT-PCR -ves	Current healthy+other disease (untested)	CLIA	0.85 [0.81, 0.88]	0.98 [0.97, 0.99]
To 2020a [A]	14	0	2	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.88 [0.62, 0.98]	Not estimable
To 2020a [B]	15	0	1	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.94 [0.70, 1.00]	Not estimable
Wan 2020 [A]	2	1	5	9	Hospital in-patient	All RT-PCR+ve	Mixed	IIFT	0.29 [0.04, 0.71]	0.90 [0.55, 1.00]
Wang 2020a [B]	14	22	0	50	Hospital in-patient	Other criteria	Current other disease (untested)	CGIA	1.00 [0.77, 1.00]	0.69 [0.57, 0.80]
Xiang 2020a [A]	35	0	28	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	ELISA	0.56 [0.42, 0.68]	1.00 [0.90, 1.00]
Xiang 2020a [B]	52	0	39	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	CGIA	0.57 [0.46, 0.67]	1.00 [0.90, 1.00]
Xiang 2020b	72	0	18	60	Hospital in-patient	Other criteria including RT-PCR -ves	Current healthy+other disease (RT-PCR-ve)	ELISA	0.80 [0.70, 0.88]	1.00 [0.94, 1.00]
Xiao 2020a	28	0	6	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.82 [0.65, 0.93]	Not estimable
Xie 2020a	49	0	7	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.88 [0.76, 0.95]	Not estimable
Xu 2020a	4	0	6	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.40 [0.12, 0.74]	Not estimable
Zeng 2020a	0	0	27	36	Hospital in-patient	Unclear	Current healthy (untested)	ELISA	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]
Zhang 2020a	182	0	40	0	Hospital in-patient	China criteria including RT-PCR -ves		CLIA	0.82 [0.76, 0.87]	Not estimable
Zhang 2020b	3	6	0	219	Hospital out-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CLIA	1.00 [0.29, 1.00]	0.97 [0.94, 0.99]
Zhang 2020c	16	0	0	0	Hospital in-patient	All RT-PCR+ve		ELISA	1.00 [0.79, 1.00]	Not estimable
Zhao 2020a	143	3	30	210	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.83 [0.76, 0.88]	0.99 [0.96, 1.00]
Zhong 2020 [A]	46	1	1	299	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.98 [0.89, 1.00]	1.00 [0.98, 1.00]
Zhong 2020 [B]	42	9	5	291	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	ELISA	0.89 [0.77, 0.96]	0.97 [0.94, 0.99]
Zhong 2020 [C]	46	14	1	286	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	CLIA	0.98 [0.89, 1.00]	0.95 [0.92, 0.97]


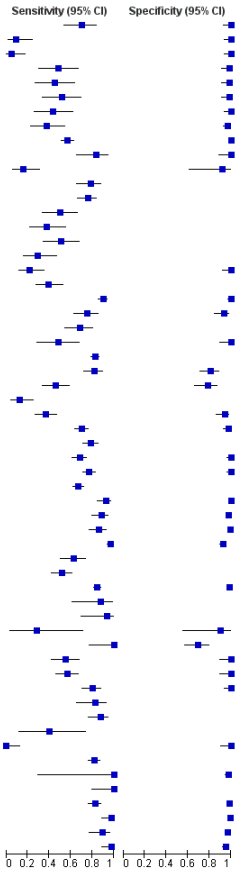


Figure 13

Figure 13. Forest plot of studies evaluating tests for detection of IgG/IgM at all time post-symptom onset.


Study	TP	FP	FN	TN	Setting	Reference standard (cases)	Reference standard (non-cases)	Test method	Sensitivity (95% CI)	Specificity (95% CI)
Adams 2020 [A]	34	0	6	50	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	ELISA	0.85 [0.70, 0.94]	1.00 [0.93, 1.00]
Adams 2020 [D]	21	2	12	58	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.64 [0.45, 0.80]	0.97 [0.88, 1.00]
Adams 2020 [E]	25	1	13	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.66 [0.49, 0.80]	0.98 [0.91, 1.00]
Adams 2020 [F]	19	2	12	58	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.61 [0.42, 0.78]	0.97 [0.88, 1.00]
Adams 2020 [G]	20	1	11	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.65 [0.45, 0.81]	0.98 [0.91, 1.00]
Adams 2020 [H]	23	3	10	57	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.70 [0.51, 0.84]	0.95 [0.86, 0.99]
Adams 2020 [I]	18	0	14	60	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.56 [0.38, 0.74]	1.00 [0.94, 1.00]
Adams 2020 [J]	22	4	18	138	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	LFA (no details)	0.55 [0.38, 0.71]	0.97 [0.93, 0.99]
Bendavid 2020	130	16	27	3308	Mixed	Mixed	Mixed	LFA (no details)	0.83 [0.76, 0.88]	1.00 [0.99, 1.00]
Cai 2020a	225	0	51	167	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.82 [0.76, 0.86]	1.00 [0.98, 1.00]
Cassaniti 2020 (A)	25	0	5	30	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CGIA	0.83 [0.65, 0.94]	1.00 [0.88, 1.00]
Cassaniti 2020 (B)	7	1	31	11	Hospital A&E	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CGIA	0.18 [0.08, 0.34]	0.92 [0.62, 1.00]
Dohla 2020	8	3	14	24	Community	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CGIA	0.36 [0.17, 0.59]	0.89 [0.71, 0.98]
Du 2020	60	0	0	0	Hospital in-patient	Unclear		CLIA	1.00 [0.94, 1.00]	Not estimable
Garcia 2020 (A)	26	0	29	45	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy	CGIA	0.47 [0.34, 0.61]	1.00 [0.92, 1.00]
Garcia 2020 (B)	56	0	7	0	Hospital in-patient	Other criteria		CGIA	0.89 [0.78, 0.95]	Not estimable
Grzelak 2020 [D]	106	0	14	134	Hospital in-patient	Unclear	Pre-pandemic healthy	S-flow	0.88 [0.81, 0.93]	1.00 [0.97, 1.00]
Infantino 2020	49	4	12	59	Hospital in-patient	All RT-PCR+ve	Pre-pandemic healthy+other disease	CLIA	0.80 [0.68, 0.89]	0.94 [0.85, 0.98]
Jia 2020	45	0	12	0	Hospital in-patient	China criteria including RT-PCR -ves		FIA	0.79 [0.66, 0.89]	Not estimable
Jin 2020	24	3	3	30	Hospital in-patient	All RT-PCR+ve	COVID suspects (double+ RT-PCR-ve)	CLIA	0.89 [0.71, 0.98]	0.91 [0.76, 0.98]
Lassauniere 2020 [D]	27	0	3	32	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	0.90 [0.73, 0.98]	1.00 [0.89, 1.00]
Lassauniere 2020 [E]	27	0	3	32	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	0.90 [0.73, 0.98]	1.00 [0.89, 1.00]
Lassauniere 2020 [F]	28	0	2	32	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	0.93 [0.78, 0.99]	1.00 [0.89, 1.00]
Lassauniere 2020 [G]	25	0	5	17	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	0.83 [0.65, 0.94]	1.00 [0.80, 1.00]
Lassauniere 2020 [H]	4	3	1	12	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	0.80 [0.28, 0.99]	0.80 [0.52, 0.96]
Lassauniere 2020 [I]	1	2	0	13	Hospital in-patient	All RT-PCR+ve	Pre-pandemic other disease	CGIA	1.00 [0.03, 1.00]	0.87 [0.60, 0.98]
Li 2020a	352	0	45	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.89 [0.85, 0.92]	Not estimable
Lin 2020a [A]	72	16	7	64	Hospital in-patient	All RT-PCR+ve	Current healthy+other disease (RT-PCR-ve)	CLIA	0.91 [0.83, 0.96]	0.80 [0.70, 0.88]
Liu 2020a	79	6	16	78	Hospital in-patient	Other criteria including RT-PCR -ves	COVID suspects (single RT-PCR-ve)	CGIA	0.83 [0.74, 0.90]	0.93 [0.85, 0.97]
Liu 2020b	194	4	44	116	Hospital in-patient	China criteria including RT-PCR -ves	Current healthy+other disease (untested)	ELISA	0.82 [0.76, 0.86]	0.97 [0.92, 0.99]
Liu 2020d [A]	172	0	42	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.80 [0.74, 0.85]	1.00 [0.96, 1.00]
Liu 2020d [B]	176	0	38	100	Hospital in-patient	All RT-PCR+ve	Current healthy (untested)	ELISA	0.82 [0.76, 0.87]	1.00 [0.96, 1.00]
Long 2020 (A)	16	7	0	141	Community	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CLIA	1.00 [0.79, 1.00]	0.95 [0.90, 0.98]
Long 2020 (B)	302	0	61	0	Hospital in-patient	All RT-PCR+ve		CLIA	0.83 [0.79, 0.87]	Not estimable
Ma 2020a	213	0	3	483	Hospital in-patient	All RT-PCR+ve	Mixed	CLIA	0.99 [0.96, 1.00]	1.00 [0.99, 1.00]
Pan 2020a	73	0	35	0	Hospital in-patient	China criteria including RT-PCR -ves		CGIA	0.68 [0.58, 0.76]	Not estimable
Paradiso 2020a	21	13	49	107	Hospital A&E	All RT-PCR+ve	COVID suspects (single RT-PCR-ve)	CGIA	0.30 [0.20, 0.42]	0.89 [0.82, 0.94]
Wan 2020 [A]	6	0	1	10	Hospital in-patient	All RT-PCR+ve	Mixed	IIFT	0.86 [0.42, 1.00]	1.00 [0.69, 1.00]
Xiang 2020a [A]	55	0	8	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	ELISA	0.87 [0.77, 0.94]	1.00 [0.90, 1.00]
Xiang 2020a [B]	75	0	16	35	Hospital in-patient	WHO criteria including RT-PCR -ves	Current healthy (untested)	CGIA	0.82 [0.73, 0.90]	1.00 [0.90, 1.00]
Xu 2020a	9	0	1	0	Hospital in-patient	All RT-PCR+ve		CGIA	0.90 [0.55, 1.00]	Not estimable
Yongchen 2020	17	0	4	0	Mixed	All RT-PCR+ve		CGIA	0.81 [0.58, 0.95]	Not estimable
Zeng 2020a	0	0	27	36	Hospital in-patient	Unclear	Current healthy (untested)	ELISA	0.00 [0.00, 0.13]	1.00 [0.90, 1.00]
Zhang 2020c	13	0	3	0	Hospital in-patient	All RT-PCR+ve		ELISA	0.81 [0.54, 0.96]	Not estimable

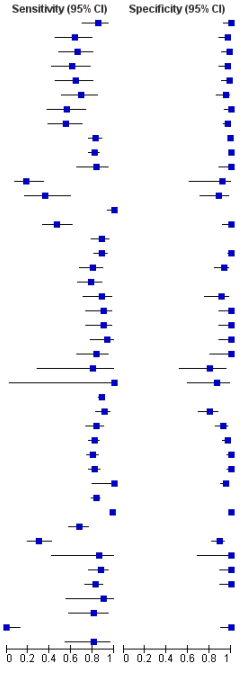

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

Figure 14

Figure 14. Forest plot of tests: 19 IgA (all time points), 25 Total antibodies (Ab) (all time points), 38 IgA/IgM (all time points).

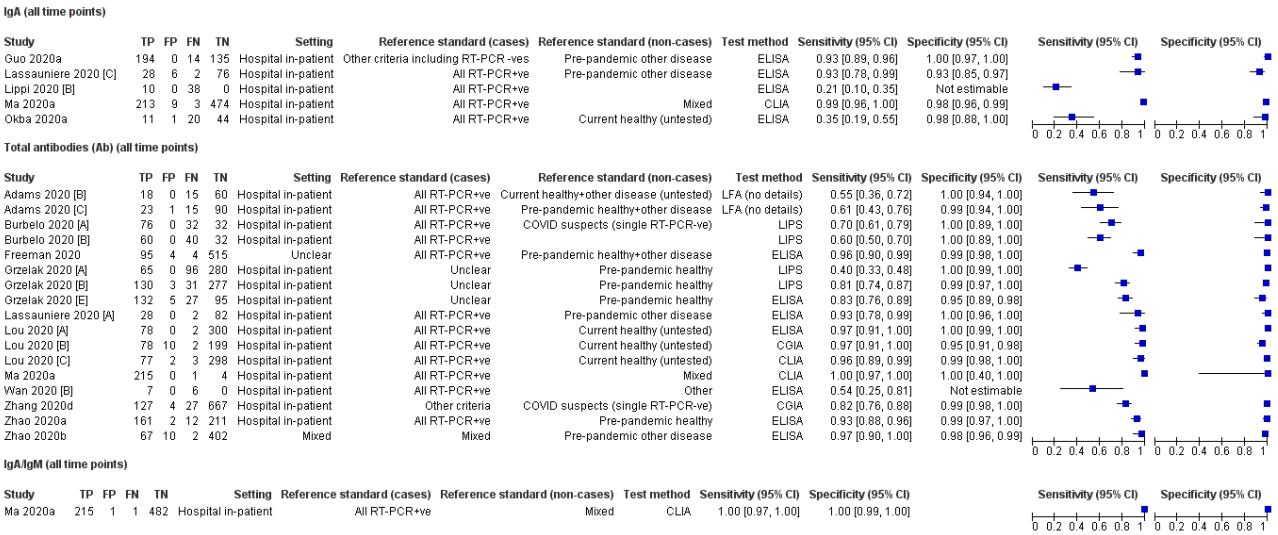

Appendix 12. Manufacturer product code details identified

Test	Study	From paper	From company documentation/website
ELISA: Enzyme-linked immunosorbent assay			
Beijing Beier Bioengineering	Gao 2020b [C]	No product codes provided (Study author contacted 29 May 2020)	No IFU and not on company website, no product code identified
Beijing Hotgen	Wang 2020a [A]	ELISA (20200101 and 20200201)	No IFU, no product code identified www.hotgen.com.cn/ky/upt.html Unclear if test on website is ELISA although the company do produce ELISAs
	Liu 2020d [A]	No product code provided ; "The rS-based ELISA kit (Hotgen, Beijing, China)" Study author contacted 1 June 2020	
Beijing Wantai	Lassauniere 2020 [A]	SARS-CoV-2 Ab ELISA (CE-IVD) (WS-1096)	www.sanbio.nl/ws-1096
	Lou 2020 [A]	IgM, IgG; no product code reported in paper Study author responded: ELISA-Ab lot number NCOA20200201B ELISA-IgM lot number NCOM20200202B	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

		ELISA-IgG lot number NCOnG20200201B	
	Zhao 2020a	No product code reported; "(ELISA) kits supplied by Beijing Wantai Biological Pharmacy Enterprise Co" Study author contacted 1 June 2020	
Darui Biotechnology	Lin 2020a [A]	No product code reported; "commercial enzyme-linked immunosorbent assay kit (Darui Biotech, CHINA)" Study author contacted 1 June 2020	No IFU, no product code on website (www.daruibiotech.com/eproduct/index_33.html)
EUROIMMUN	Lassauniere 2020 [B]; Lassauniere 2020 [C]	Anti-SARS-CoV-2 IgG (EI 2668-9601 G) Anti-SARS-CoV-2 IgA (EI 2606-9601 A)	IFU: Anti-SARS-CoV-2 ELISA (IgG) (EI 2606-9601 G) IFU: Anti-SARS-CoV-2 ELISA (IgA) (EI 2606-9601 A)
	Lippi 2020 [B]	No product code reported; "Anti-SARS-CoV-2 IgA and IgG … ELISAs; Euroimmun AG, Lübeck, Germany" Study author replied but could not supply product code	
	Okba 2020a	No product code reported; "β-versions of 2 commercial kits (EUROIMMUN)" (These are Beta versions)	Not available
Zhuhai Livzon	Xiang 2020a [A]	IgG/IgM antibody ELISA kits (lot number 2020010108)	No IFU identified; website only has the lateral flow assay en.livzon.com.cn/product/98.html No product code identified
	Xiang 2020b	ELISA kits (lot numbers IgM 20200308, IgG 20200308)	
	Zeng 2020a	No product code reported: ELISA "assay kits (Zhuhai Livzon Diagnostics INC.)" Study author contacted 1 June 2020	
Zhuhai Lizhu	Liu 2020b	No product code reported: ELISA kit "(Lizhu, Zhuhai, China)" Study author contacted 1 June 2020	Presumed to be same as above, following contact with FIND
	Liu 2020d [B]	No product code reported: ELISA kit (Lizhu, Zhuhai, China) Study author contacted 1 June 2020	
CLIA: chemiluminescence immunoassay			
Beijing Beier Bioengineering	Gao 2020b [A]	No product codes provided (Study author contacted 29 May 2020)	No IFU, not on website; no product code identified
Bioscience Co (Chongqing)	Hu 2020a	No product code reported; "(MCLIA) kit supplied by Bioscience Co., Ltd (Chongqing, China)" Study author contacted 1 June 2020	Review authors unable to find this company; no product code identified
	Long 2020 (A); Long 2020 (B)	No product code reported; "(MCLIA) kit supplied by Bioscience Co., Ltd China)" Study author supplied NMA approval numbers only:	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

		MCLA IgG: China National Medical Products Administration approval number 20203400183; MCLA IgM: China National Medical Products Administration approval number20203400182	
Shenzhen YHLO	Infantino 2020	No product code reported; "IgM and IgG CLIA kits were from Shenzhen YHLO Biotech Co., Ltd (China)," Study author provided details: IgG anti-SARS Cov2 C86095G; IgM C86095M LOT NUMBER 207	Company flyer: iFlash-SARS-CoV-2 IgG (C86095G) iFlash-SARS-CoV-2 IgM (C86095G)
	Jin 2020	No product code reported; "(CLIA) kits used in this study were supplied by Shenzhen YHLO Biotech Co., Ltd (China)" Study author contacted 1 June 2020	
	Liu 2020c	No product code reported; "SARS-CoV-2 antibody detection kit (YHLO Biotech, Shenzhen, China" Study author contacted 1 June 2020	
	Xiao 2020a	No product code reported; "IgM and IgG were analyzed by … CLIA … (Shenzhen Yahuilong Biotechnology Co., Ltd). Study author contacted 1 June 2020	
	Xie 2020a	No product code reported; "IgG and IgM assays were purchased from YHLO Biological Technology Co., Ltd., Shenzhen, China" Study author contacted 1 June 2020	
	Zhang 2020a	No product code reported; "(CLIA) Assays panel (Shenzhen YHLO Biotech Co., Ltd., Shenzhen, China)" Study author contacted 1 June 2020	
	Zhang 2020b	No product code reported; "CLIA detection kit from Shenzhen Yahuilong Biotechnology Co Ltd" Study author contacted 1 June 2020	
Snibe Diagnostic - MAGLUMI	Lippi 2020 [A]	No product code reported; "MAGLUMI 2019-nCoV IgG and IgM". (IgM - 130219016M; IgG – 130219015M) Study author contacted 1 June 2020 Study author replied 1 June 2020 with IFU (no lot numbers provided; code from IFU added above)	From image on website: IgM - Ref 130219016M; Lot 2712000501 IgG - Ref 130219016M; Lot 2722000501 (www.snibe.com/zh_en/en_newsView.aspx?id=576)
	Padoan 2020	No product code reported; "MAGLUMI 2000 Plus (New Industries Biomedical Engineering Co., Ltd [Snibe], Shenzhen, China)" Study author supplied details: - for SARS-CoV-2 IgG lot number used for all the 87 measurements: 2722000102, kit number 8131;	

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

		- for SARS-CoV-2 IgM lot number used for all the 87 measurements: 2712000201, kit number 5122	
Xiamen InnoDx Biotech	Lou 2020 [C]	No product code reported; "CMIA reagents were supplied by Xiamen InnoDx Biotech Co., Ltd., China Study author supplied following details: CMIA-Ab product code CT0669 lot number 20200201 CMIA-IgM product code CT0667 lot number 20200201	Review authors unable to find website for this company
Other laboratory-based tests			
EUROIMMUN	Wan 2020 [A]	No product code reported; "Anti-SARS CoV Indirect 62 Immunofluorescence test (IIFT) (IgM & IgG) by Euroimmun (Germany)" (Test uses SARS-Cov not SARS-CoV-2)	
Lateral flow assays			
Acro Biotech	Lassauniere 2020 [H]	2019-nCoV IgG/IgM Rapid Test Cassette (INCP-402)	Code from IFU and Assay Genie website: INCP-402
Artron Laboratories	Lassauniere 2020 [G]	Coronavirus Diseases 2019 (COVID-19) IgM/IgG Antibody Test (A03-51-322),	Brochure only; but no product code www.artronlab.com/products/CoVBrochure-ver3.pdf
Autobio Diagnostics	Lassauniere 2020 [F]	Anti-SARS-CoV-2 Rapid Test (RTA0204)	Code from IFU: Anti-SARS-CoV-2 Rapid Test (RTA0203)
Beijing Beier Bioengineering	Gao 2020b [B]	No product codes provided (Study author contacted 29 May 2020)	No IFU and not on company website; Distributor: www.unifier.one/en/beier-new-2019-coronavirus-covid-19-rapid-test.html 2019- New Coronavirus IgM/IgG Rapid Test Casette (WB/S/P) No product code
Beijing Diagreat	Jia 2020	COVID IgM/IgG antibodies kit, which have sent to Beijing Institute of Medical Device Testing (BIMT) for product verification (lot: 20200214)	Manual from 2019-nCoV IgM Antibody Determination Kit (immunochromatographic Assay) Product No. P11802 2019-nCoV IgG Antibody Determination Kit (Immunochromatographic Assay) Product No. P11801

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

Beijing Hotgen	Wang 2020a [B]	Kit provided by Beijing Hotgen Biotechnology Co., Beijing, China: (lot number 20200208 and 105 20200229 for GICA)	No IFU, on website but no product code www.hotgen.com.cn/ky/up-t.html Coronavirus disease (COVID-19) Antibody Test (Colloidal Gold)
Beijing Wantai	Lou 2020 [B]	No product code reported Study author provided: LFIA-Ab lot number JNB20200202F LFIA-IgM lot number JNM20200203F LFIA-IgG lot number JNG20200201F	Code from IFU: WJ-2701, WJ-2710, WJ-2750 Website: Rapid test for coronavirus Ab (CE-IVD) (WJ-2750 www.sanbio.nl/wj-2750)
CTK Biotech - OnSite	Lassauniere 2020 [E]	OnSite COVID-19 IgG/IgM Rapid Test (R0180C)	IFU: OnSite COVID-19 IgG/IgM Rapid Test R0180C
Dynamiker Biotechnology	Lassauniere 2020 [D]	2019-nCOV IgG/IgM Rapid Test (DNK-1419-1)	IFU: 2019-nCOV IgG/IgM Rapid Test Catalogue No: DNK-1419-1
Hangzhou Alltest	Lassauniere 2020 [I]	2019-nCoV IgG/IgM Rapid Test Cassette (INCP-402)	IFU; 2019-nCoV IgG/IgM Rapid Test Cassette (Whole blood/serum/plasma) Package Insert INCP-402
	Garcia 2020 (A)	AllTest COV-19 IgG / IgM kit (no product code)	
	Garcia 2020 (B)	Study author provided IFU (product code NCP-402)	
Innovita Biological	Gao 2020a	No product code reported Study author contacted 1 June 2020	IFU: 2019-nCoV Ab Test (Colloidal gold); Catalogue No. YF 319C
	Yongchen 2020	No product code reported Study author provided lot number: 20200205	
Jiangsu Medomics	Li 2020a	No product code reported "SARS-CoV-2 rapid IgG-IgM combined antibody test kit" Study author contacted 1 June 2020	Review authors were unable to find this company; study was also provided to review authors by Lomina (www.test-covid19.com/); no product code identified
Vivachek - VivaDiag	Paradiso 2020a	No product code reported; "Viva-Diag™ kit *produced by Jiangsu Medomics* Medical Technologies kit (https://www.vivachek.com/vivachek/English/prods/prod-covid19.html)"; link no longer active. test considered to be Vivachek test Study author contacted 1 June 2020	Package insert VivaDiag SARS-CoV-2 IgM/IgG Rapid Test (VID35-08-011 / VID35-08-012 / VID35-08-013 / VID35-08-014 / VID35-08-015)

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

(Continued)

	Cassaniti 2020 (A) Cassaniti 2020 (B)	No product code reported; "VivaDiag COVID-19 IgM/IgG from VivaChek"; study also provided by Vivachek following company contact Study author provided lot number E2002002, REF VID35-08-011	
Zhuhai Livzon	Pan 2020a	No product code reported Study author contacted 1 June 2020	Product flyer; Diagnostic Kit for IgM/IgG Antibody to Coronavirus (SARS-CoV-2); Catalogue number: 01040048
	Xiang 2020a [B]	IgG/IgM antibody GICA kits (lot number 2001010220)	

FIND: Foundation for Innovative Diagnostics; **IFU:** instructions for use; **NMA:** China National Medical Products Administration

HISTORY

Review first published: Issue 6, 2020

CONTRIBUTIONS OF AUTHORS

JJD was the contact person with the editorial base.
JJD co-ordinated contributions from the co-authors and wrote the final draft of the review.
JJD, JDi, YT, CD, STP, IH, AA, LFR, MP, JDr, SB screened papers against eligibility criteria.
RS conducted the literature searches
JJD, JDi, YT, CD, STP, IH, AA, LFR, MP, JDr, SB appraised the quality of papers.
JJD, JDi, YT, CD, STP, IH, AA, LFR, MP, JDr, SB extracted data for the review and sought additional information about papers.
JJD and JDi entered data into Review Manager 2014.
JJD and JDi analysed and interpreted data.
JJD, JDi, YT, CD, STP, RS, ML, LH, AVB, DE, SD worked on the methods sections.
JJD and JDi responded to the comments of the referees.
JJD.is the guarantor of the update.

DECLARATIONS OF INTEREST

Jonathan J Deeks: none known

Jacqueline Dinnes: none known

Yemisi Takwoingi: none known

Clare Davenport: none known

René Spijker: the Dutch Cochrane Centre (DCC) has received grants for performing commissioned systematic reviews. In no situation, the commissioner had any influence on the results of the work.

Sian Taylor-Phillips: none known

Ada Adriano: none known

Sophie Beese: none known

Janine Dretzke: none known

Lavinia Ferrante di Ruffano: none known

Isobel Harris: none known

Malcolm Price: none known

Sabine Dittrich: is employed by FIND with funding from DFID and Australian Aid. FIND is a global non-for profit product development partnership and WHO Diagnostic Collaboration Centre. It is FIND's role to accelerate access to high quality diagnostic tools for low resource

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.

settings and this is achieved by supporting both R&D and access activities for a wide range of diseases, including COVID-19. .FIND has several clinical research projects to evaluate multiple new diagnostic tests against published Target Product Profiles that have been defined through consensus processes. These studies are for diagnostic products developed by private sector companies who provide access to know-how, equipment/reagents, and contribute through unrestricted donations as per FIND policy and external SAC review.

Devy Emperador: is employed by FIND with funding from DFID and KFW. FIND is a global non-for profit product development partnership and WHO Diagnostic Collaboration Centre. It is FIND's role to accelerate access to high quality diagnostic tools for low resource settings and this is achieved by supporting both R&D and access activities for a wide range of diseases, including COVID-19. .FIND has several clinical research projects to evaluate multiple new diagnostic tests against published Target Product Profiles that have been defined through consensus processes. These studies are for diagnostic products developed by private sector companies who provide access to know-how, equipment/reagents, and contribute through unrestricted donations as per FIND policy and external SAC review.

Lotty Hooft: none known

Mariska MG Leeflang: none known

Ann Van den Bruel: none known

SOURCES OF SUPPORT

Internal sources

- Liverpool School of Tropical Medicine, UK
- University of Birmingham, UK

External sources

- Department for International Development, UK

  Project number: 300342-104
- National Institute for Health Research (NIHR), UK
- NIHR Birmingham Biomedical Research Centre at the University Hospitals Birmingham NHS Foundation Trust and the University of Birmingham, UK

DIFFERENCES BETWEEN PROTOCOL AND REVIEW

As we explained in the review, due to poor reporting, we were unable to identify studies that evaluated the test in patients who were symptomatic (active disease) separately from those who had recovered from their symptoms (convalescent). Our stratification of results according to days since onset of symptoms will in part be related to these categorisations.

We planned to check the following websites for eligible index tests, however these did not prove to be very accessible or easy to use and, after initial review, were not further considered:

- National Institute for Health Research (NIHR) Innovation Observatory (www.io.nihr.ac.uk/)
- www.rapidmicrobiology.com/test-method/testing-for-the-wuhan-coronavirus-a-k-a-covid-19-sars-cov-2-and-2019-ncov

We planned to check the following evidence repository for additional eligible studies however, the EPPI-Centre and Norwegian Institute of Public Health resources proved to be more accessible therefore we decided to prioritise our other sources of evidence.

- Meta-evidence (meta-evidence.co.uk/the-role-of-evidence-synthesis-in-covid19/)

QUADAS-2 (Whiting 2011), item "Was there an appropriate interval between index test(s) and reference standard?" was dropped from assessment because for antibody tests, the body's immune response to SARS-CoV-2 infection tends to increase over time such that the time between confirmation of the presence of SARS-CoV-2 an the index test is less relevant than the time from symptom onset to the application of the index test.

Copyright © 2020 The Authors. Cochrane Database of Systematic Reviews published by John Wiley & Sons, Ltd. on behalf of The Cochrane Collaboration.